
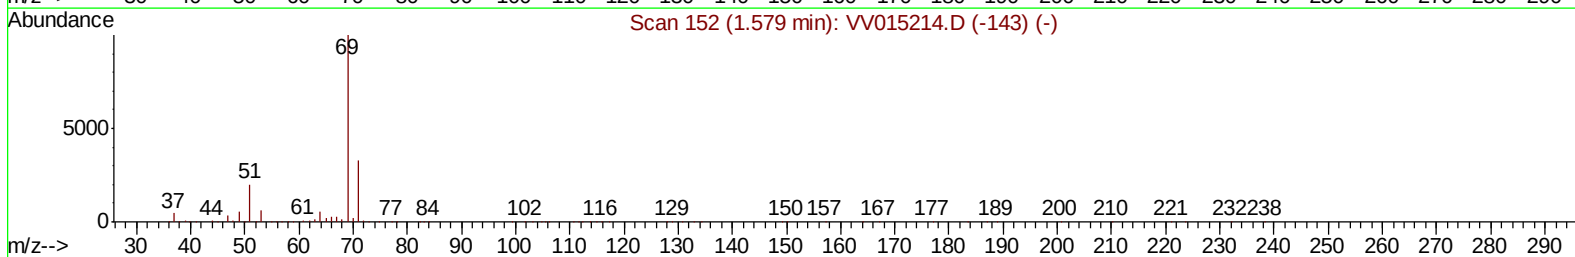
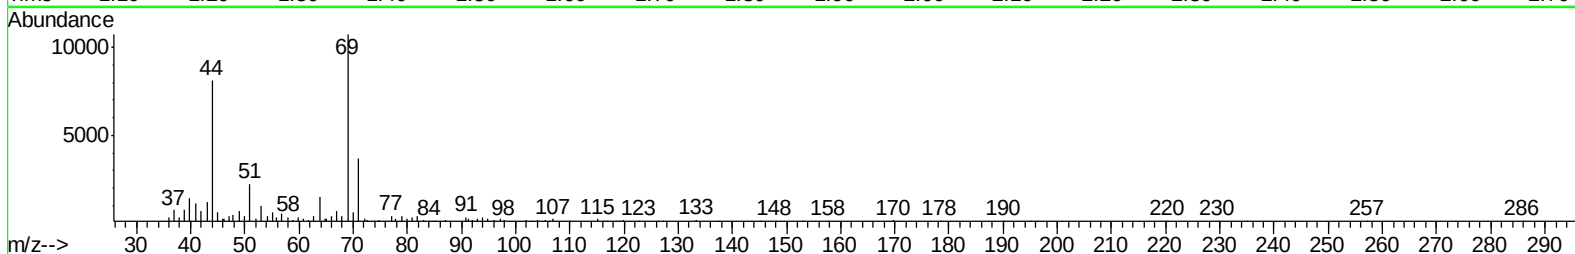


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
Data File : VV015212.D
Acq On : 27 Mar 2020 18:48
Operator : SY/MD
Sample : VSTD00563
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 28 00:29:18 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 28 00:27:30 2020
Response via : Initial Calibration

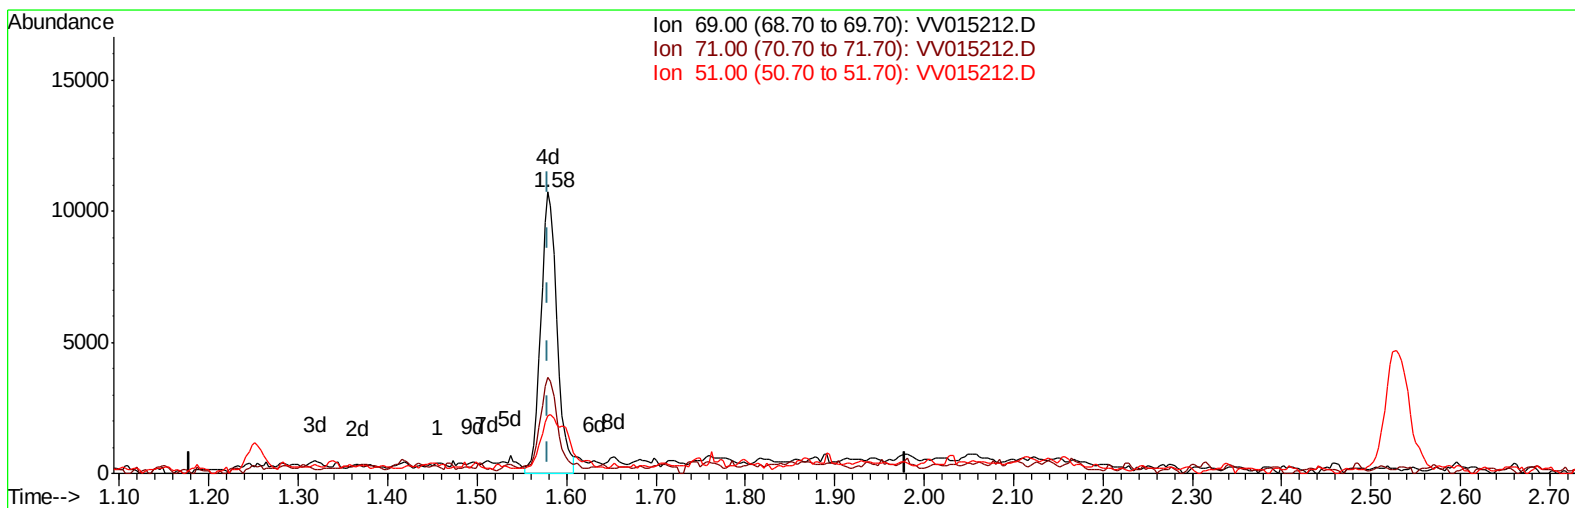

TIC: VV015212.D

(7) Chloroethane-d5 (S)

1.579min (+0.000) 4.51ug/L m

response 13514

Ion	Exp%	Act%
69.00	100	100
71.00	32.80	0.61#
51.00	29.70	0.44#
0.00	0.00	0.00