
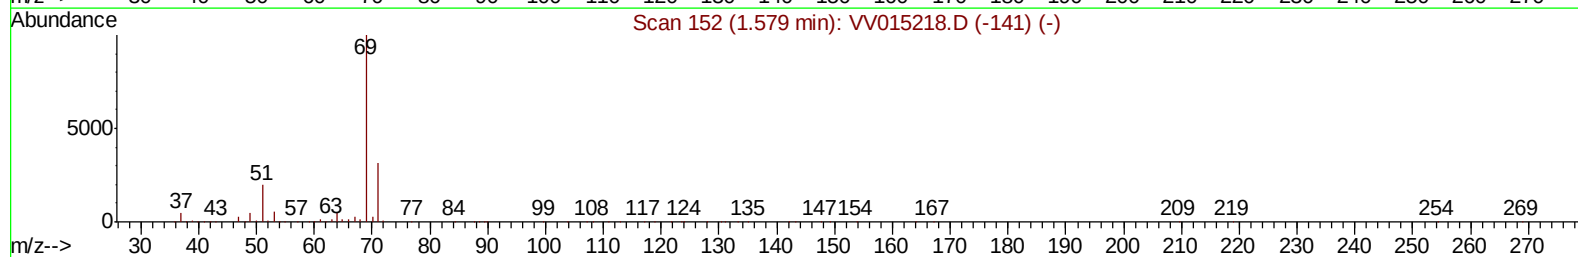
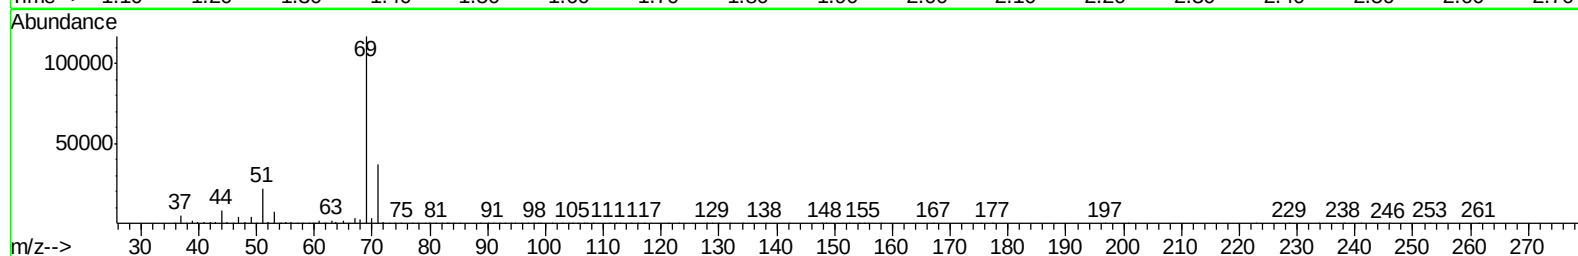


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015225.D
 Acq On : 28 Mar 2020 05:09
 Operator : SY/MD
 Sample : L2003-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 28 07:00:39 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 28 05:21:13 2020
 Response via : Initial Calibration

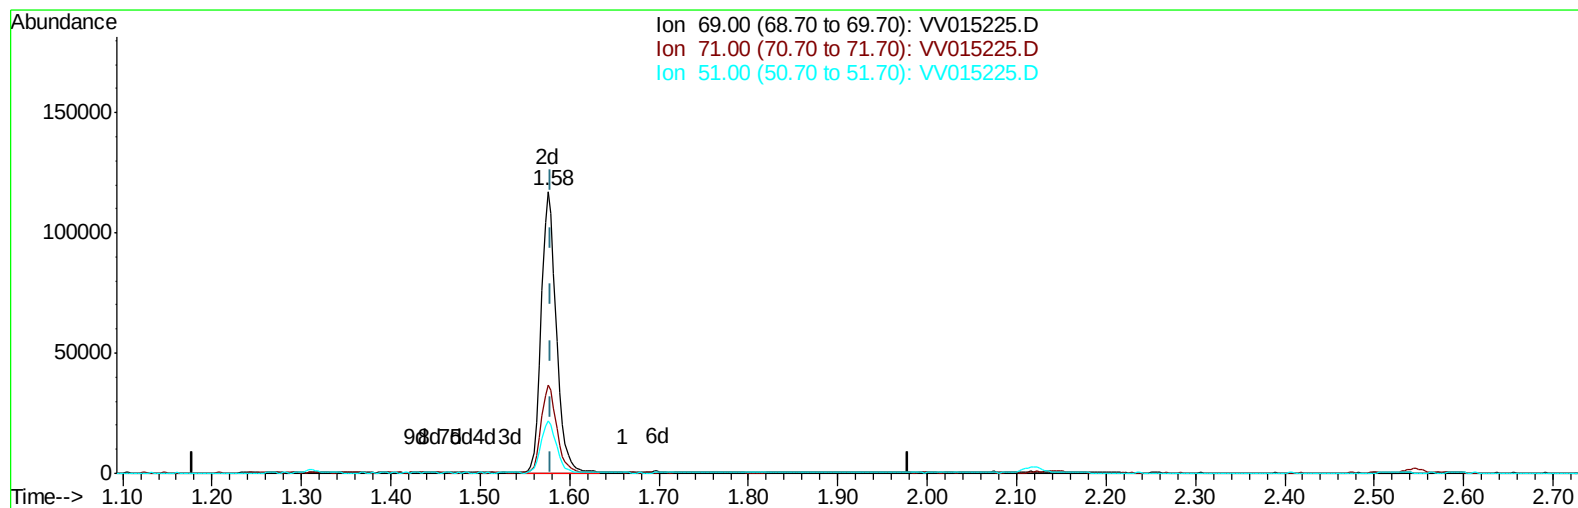

TIC: VV015225.D

(7) Chloroethane-d5 (S)

1.576min (-0.003) 46.86ug/L m

response 137715

Ion	Exp%	Act%
69.00	100	100
71.00	32.80	0.06#
51.00	29.70	0.04#
0.00	0.00	0.00