
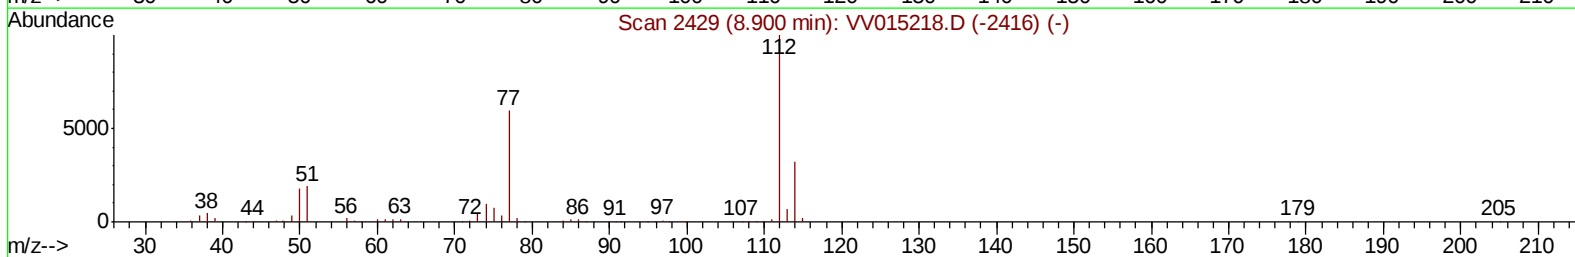
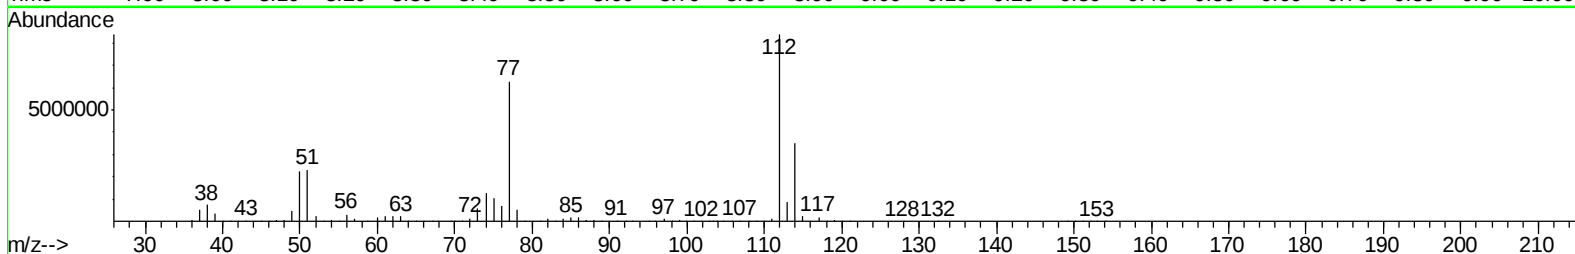


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
Data File : VV015225.D
Acq On : 28 Mar 2020 05:09
Operator : SY/MD
Sample : L2003-01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 28 07:00:39 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 28 05:21:13 2020
Response via : Initial Calibration

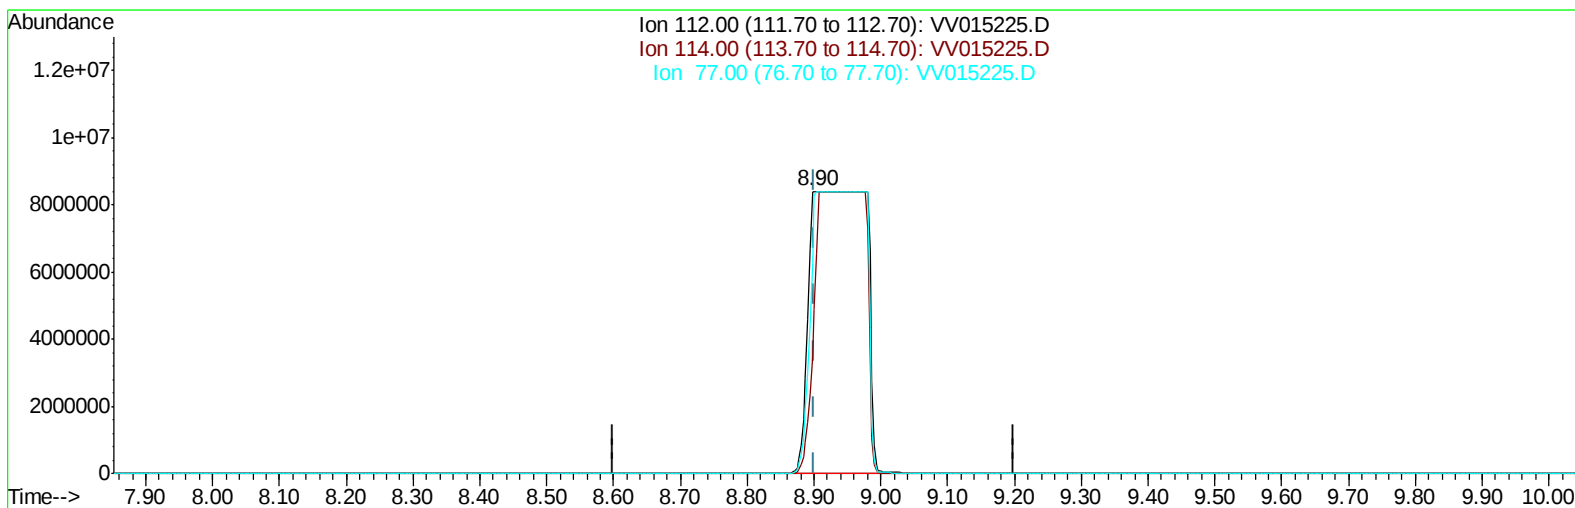

TIC: VV015225.D

(51) Chlorobenzene (T)

8.897min (-0.003) 2676.52ug/L m

response 49117535

Ion	Exp%	Act%
112.00	100	100
114.00	31.90	41.65#
77.00	60.20	74.72#
0.00	0.00	0.00