
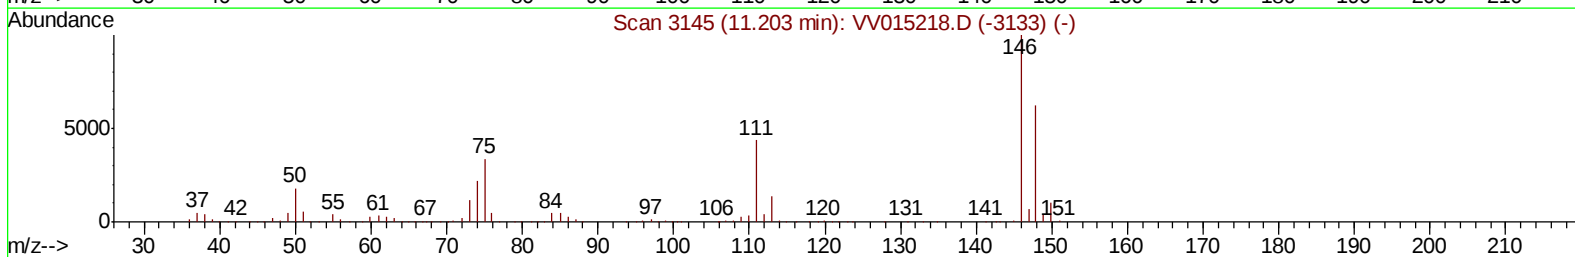
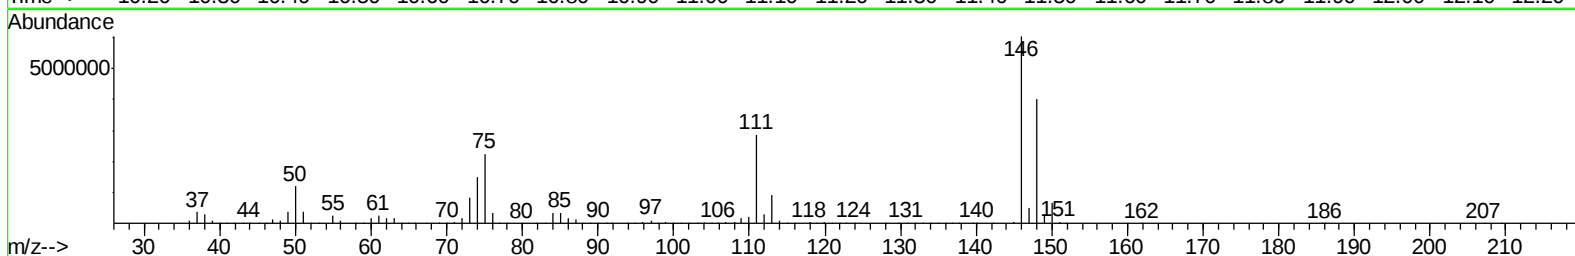


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
Data File : VV015225.D
Acq On : 28 Mar 2020 05:09
Operator : SY/MD
Sample : L2003-01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 28 07:18:36 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 28 05:21:13 2020
Response via : Initial Calibration

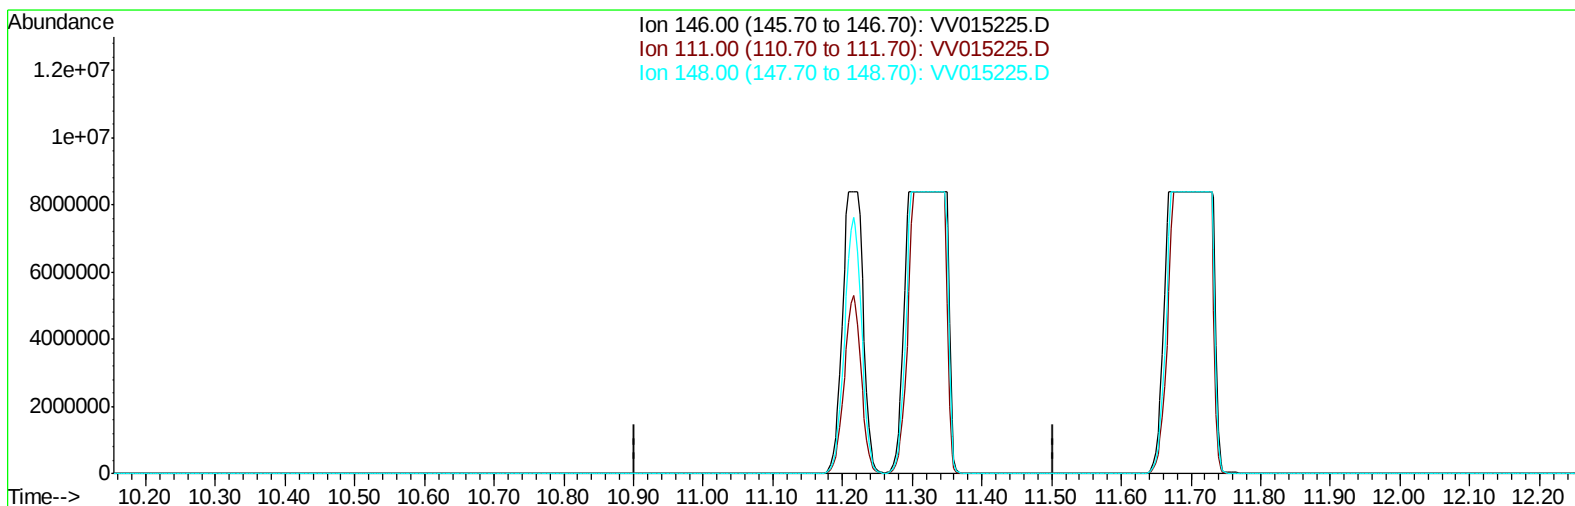

TIC: VV015225.D

(62) 1,3-Dichlorobenzene (T)

11.203min (-11.203) 0.00ug/L

response 0

Ion	Exp%	Act%
146.00	100	0.00
111.00	45.90	0.00#
148.00	62.80	0.00#
0.00	0.00	0.00