
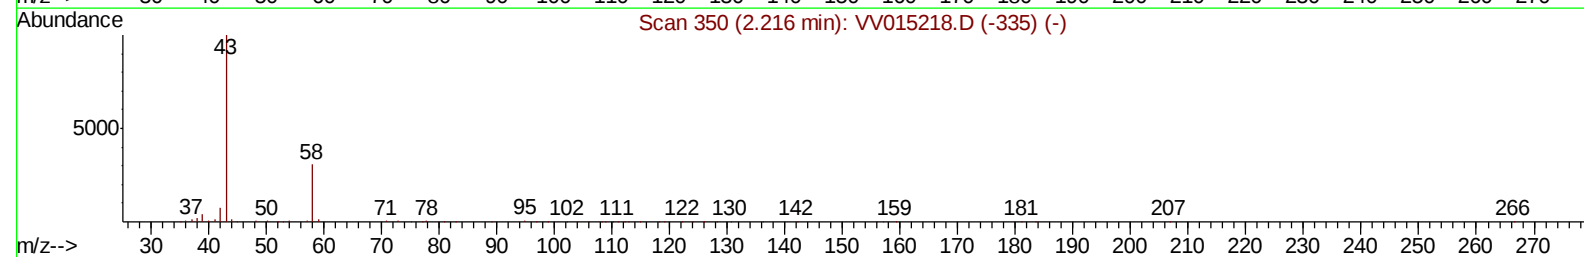
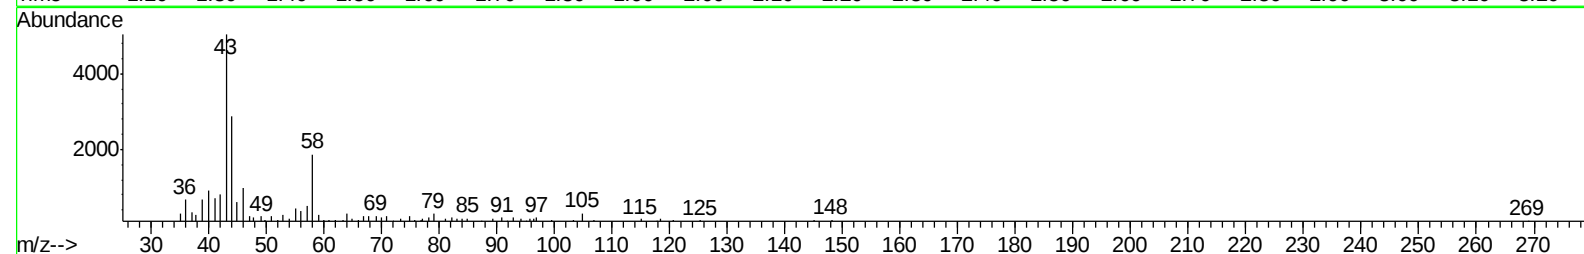


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
Data File : VV015226.D
Acq On : 28 Mar 2020 05:33
Operator : SY/MD
Sample : L2003-02
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 28 07:00:51 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 28 05:21:13 2020
Response via : Initial Calibration

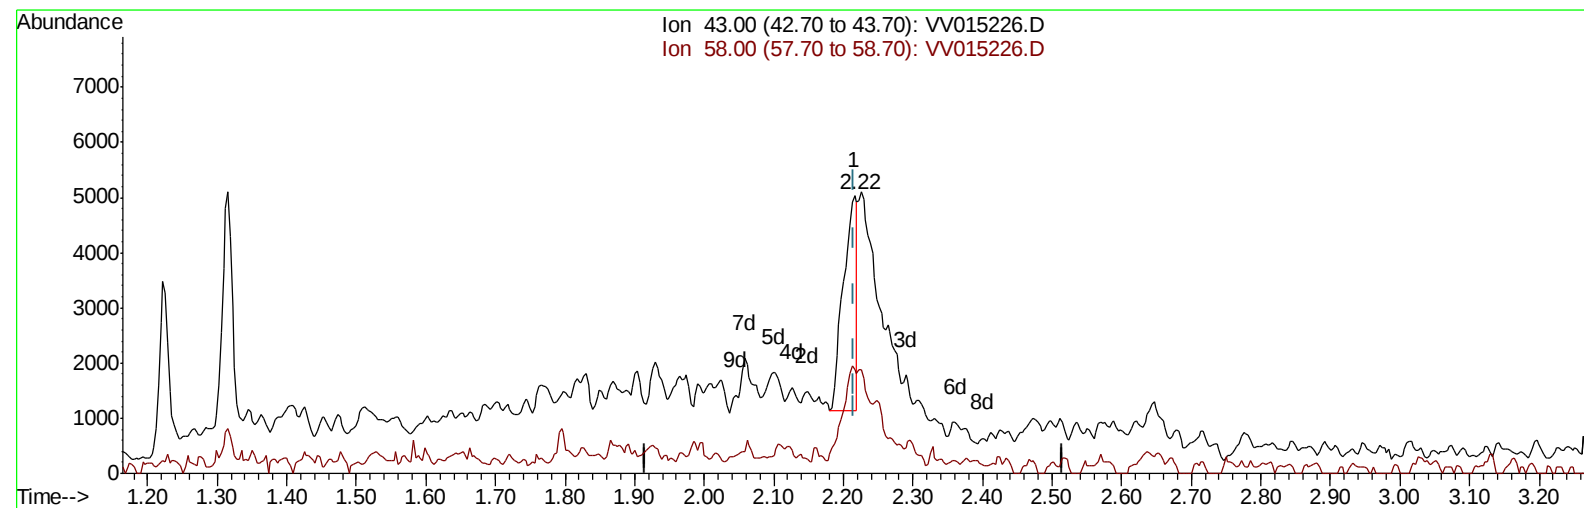

TIC: VV015226.D

(13) Acetone (T)

2.216min (-0.000) 2.81ug/L

response 5310

Ion	Exp%	Act%
43.00	100	100
58.00	0.00	44.54#
0.00	0.00	0.00
0.00	0.00	0.00