
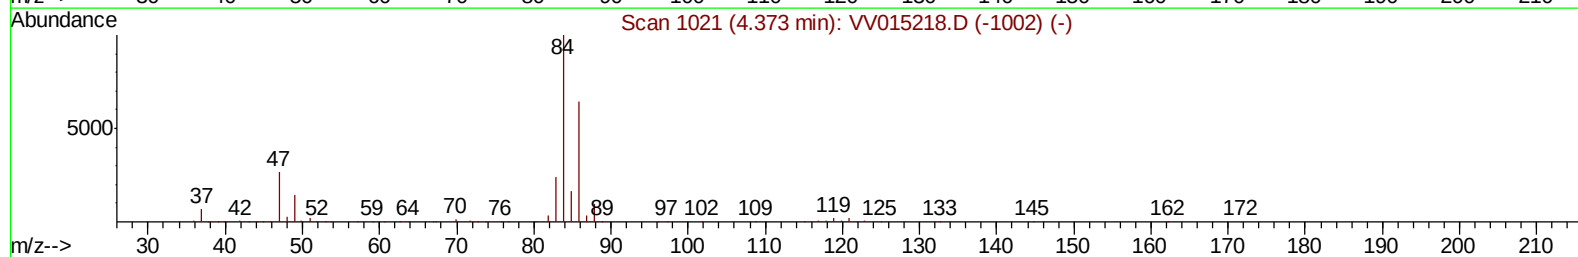
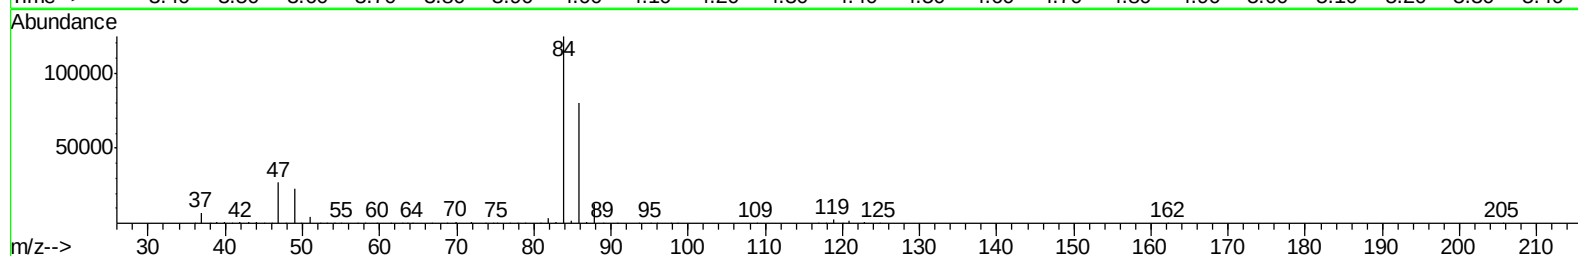


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015226.D
 Acq On : 28 Mar 2020 05:33
 Operator : SY/MD
 Sample : L2003-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 28 07:00:51 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 28 05:21:13 2020
 Response via : Initial Calibration

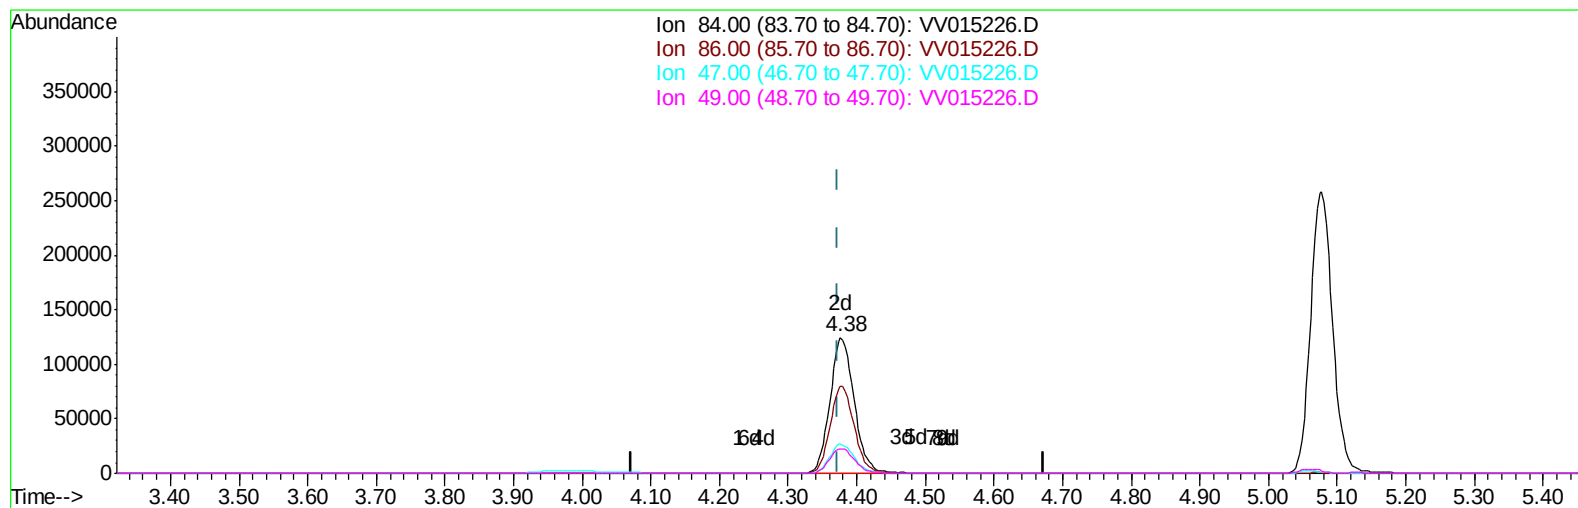

TIC: VV015226.D

(24) Chloroform-d (S)

4.376min (+0.003) 42.51ug/L m

response 302622

Ion	Exp%	Act%
84.00	100	100
86.00	62.30	0.03#
47.00	46.70	0.03#
49.00	27.00	0.02#