

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015220.D
 Acq On : 28 Mar 2020 03:07
 Operator : SY/MD
 Sample : L2003-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampled :
 C0EL6

Manual Integrations
 APPROVED

apatel
 3/31/2020 9:22:40 AM

Quant Time: Mar 28 05:27:59 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 28 05:21:13 2020
 Response via : Initial Calibration

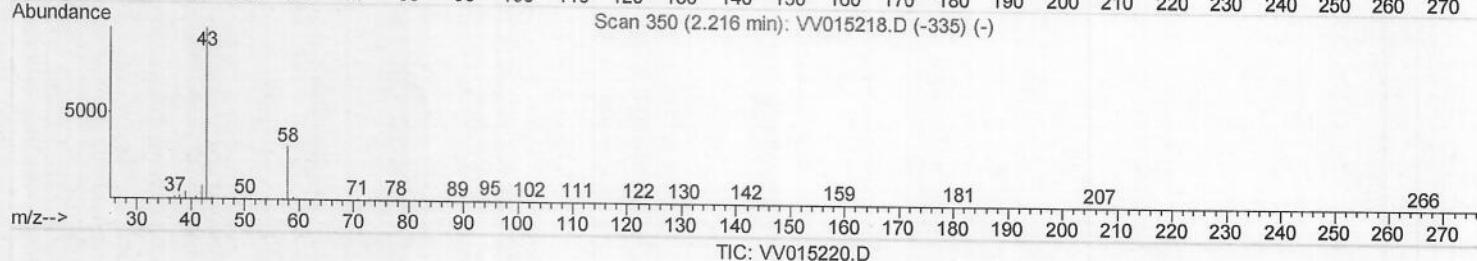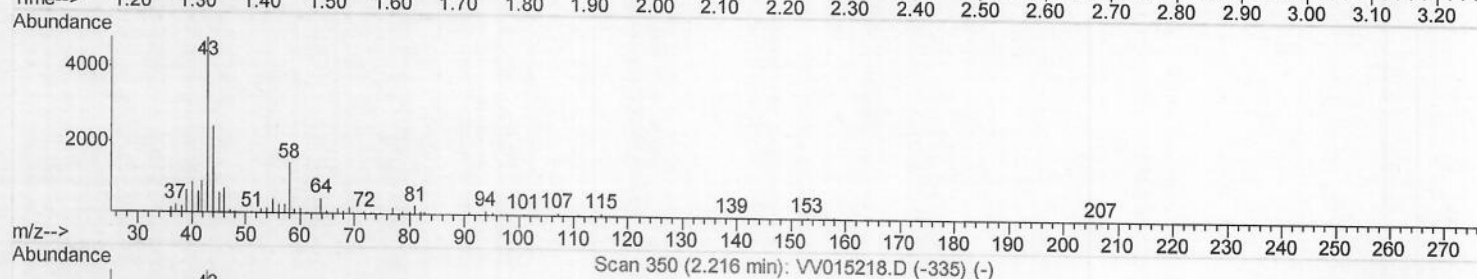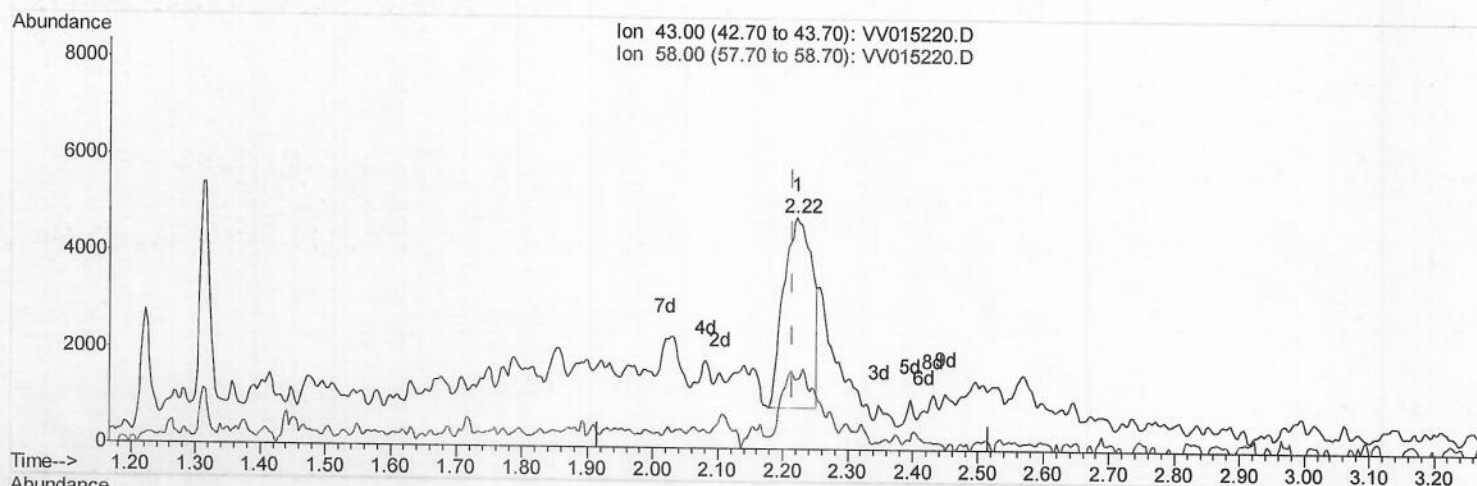

(13) Acetone (T)

2.222min (+0.006) 6.68ug/L

response 11829

Ion	Exp%	Act%
43.00	100	100
58.00	0.00	15.83#
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015220.D
 Acq On : 28 Mar 2020 03:07
 Operator : SY/MD
 Sample : L2003-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EL6

Manual Integrations
 APPROVED

apatel
 3/31/2020 9:22:40 AM

Quant Time: Mar 28 05:27:59 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 28 05:21:13 2020
 Response via : Initial Calibration

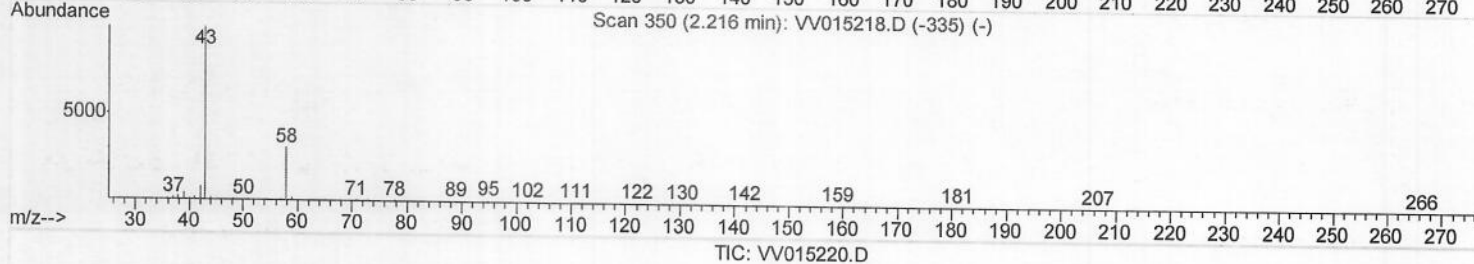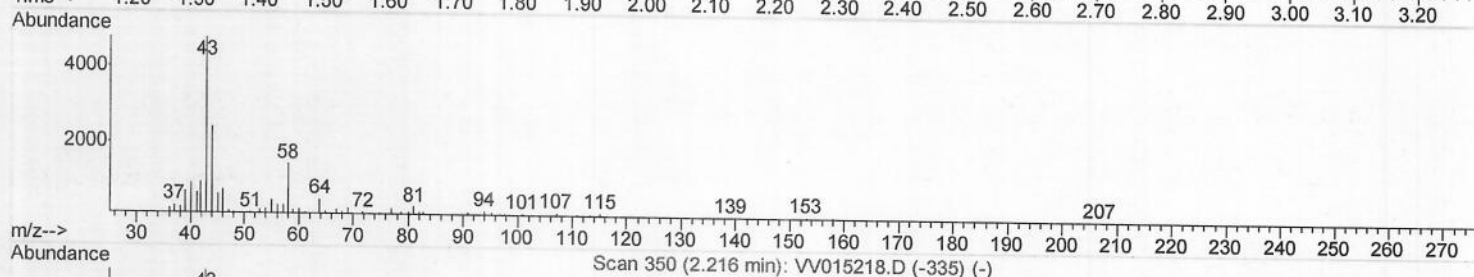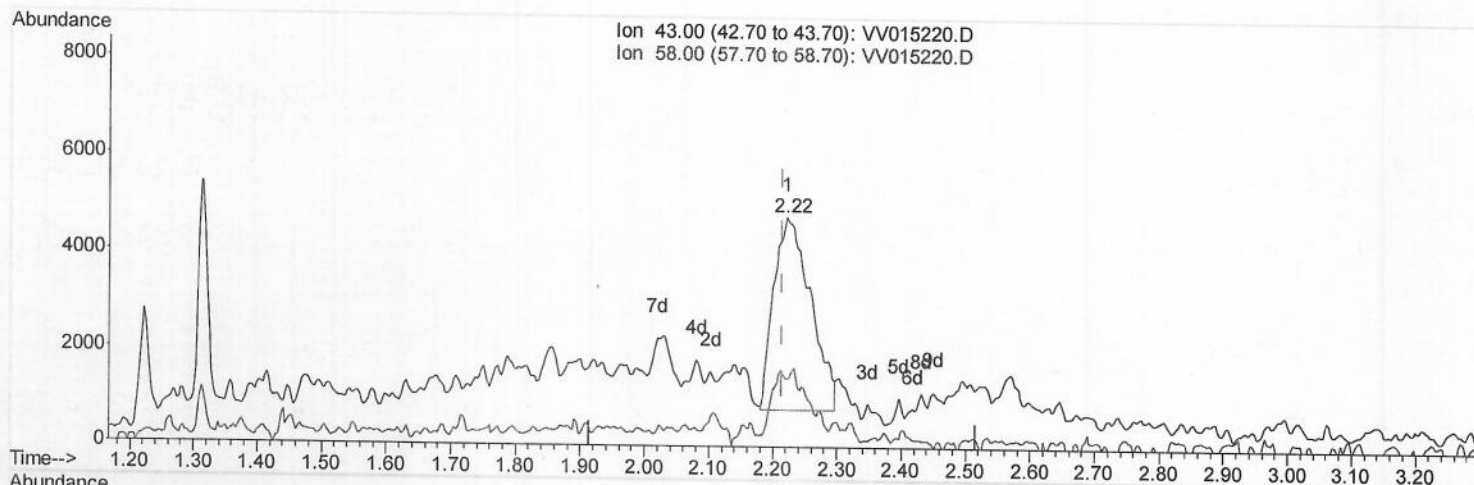

(13) Acetone (T)

2.222min (+0.006) 9.05ug/L m

response 16028

Ion	Exp%	Act%
43.00	100	100
58.00	0.00	11.68#
0.00	0.00	0.00
0.00	0.00	0.00

SY
 03/31/2020

Quantitation Report (QT Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015220.D
 Acq On : 28 Mar 2020 03:07
 Operator : SY/MD
 Sample : L2003-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EL6

Manual Integrations
 APPROVED

apatel
 3/31/2020 9:22:40 AM

Quant Time: Mar 28 06:01:29 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 28 05:21:13 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	630945	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	594186	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	258415	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	135395	52.89	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	105.78%		
7) Chloroethane-d5	1.58	69	131524	47.93	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	95.86%		
11) 1,1-Dichloroethene-d2	2.12	63	217952	34.04	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	68.08%		
21) 2-Butanone-d5	3.94	46	203008	66.94	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	66.94%		
24) Chloroform-d	4.38	84	269935	40.43	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	80.86%		
26) 1,2-Dichloroethane-d4	5.06	65	182003	41.82	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	83.64%		
32) Benzene-d6	5.08	84	506351	48.40	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.80%		
36) 1,2-Dichloropropane-d6	6.10	67	169728	43.31	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	86.62%		
41) Toluene-d8	7.34	98	470066	50.99	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	101.98%		
43) trans-1,3-Dichloropropene-	7.64	79	84723	40.46	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	80.92%		
47) 2-Hexanone-d5	8.12	63	163049	72.09	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	72.09%		
57) 1,1,2,2-Tetrachloroethane-	10.24	84	252074	36.52	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	73.04%		
64) 1,2-Dichlorobenzene-d4	11.65	152	178745	40.55	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	81.10%		

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
13) Acetone	2.22	43	16028m	9.053	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

SX
 03/31/2020

Quantitation Report (QT Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015220.D
 Acq On : 28 Mar 2020 03:07
 Operator : SY/MD
 Sample : L2003-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EL6

Manual Integrations
 APPROVED

apatel
 3/31/2020 9:22:40 AM

Quant Time: Mar 28 06:01:29 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 28 05:21:13 2020
 Response via : Initial Calibration

