

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015222.D
 Acq On : 28 Mar 2020 03:56
 Operator : SY/MD
 Sample : L1985-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTL8

Manual Integrations
 APPROVED

apatel
 3/31/2020 9:22:44 AM

Quant Time: Mar 28 05:28:18 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 28 05:21:13 2020
 Response via : Initial Calibration

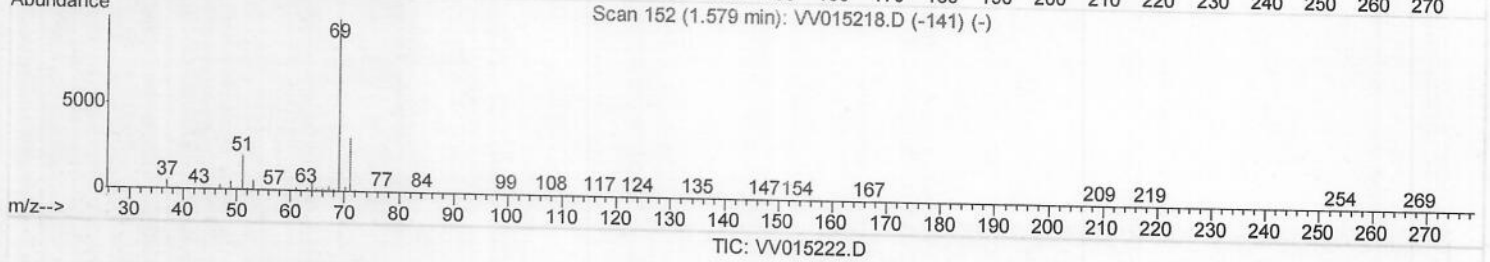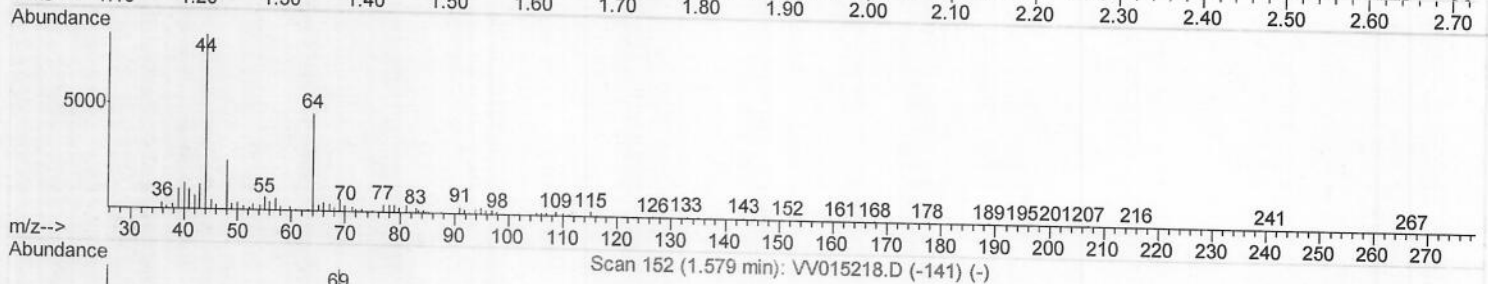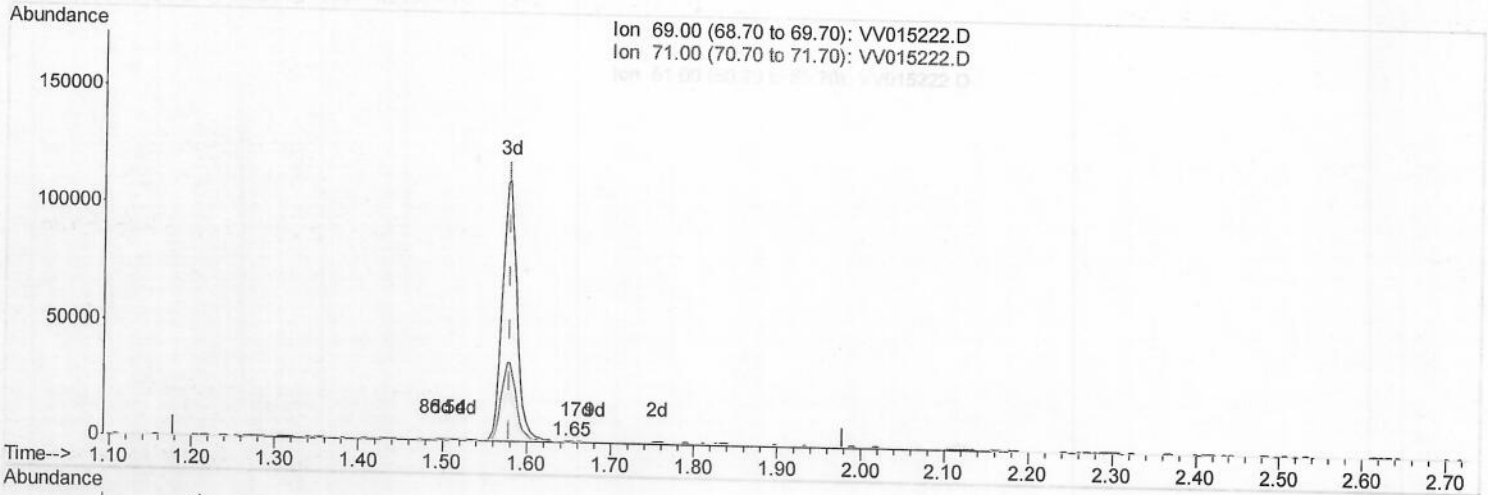

(7) Chloroethane-d5 (S)

1.647min (+0.067) 0.07ug/L

response 193

Ion	Exp%	Act%
69.00	100	100
71.00	32.80	35.23
51.00	29.70	25.39
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015222.D
 Acq On : 28 Mar 2020 03:56
 Operator : SY/MD
 Sample : L1985-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTL8

Manual Integrations
 APPROVED

apatel
 3/31/2020 9:22:44 AM

Quant Time: Mar 28 05:28:18 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 28 05:21:13 2020
 Response via : Initial Calibration

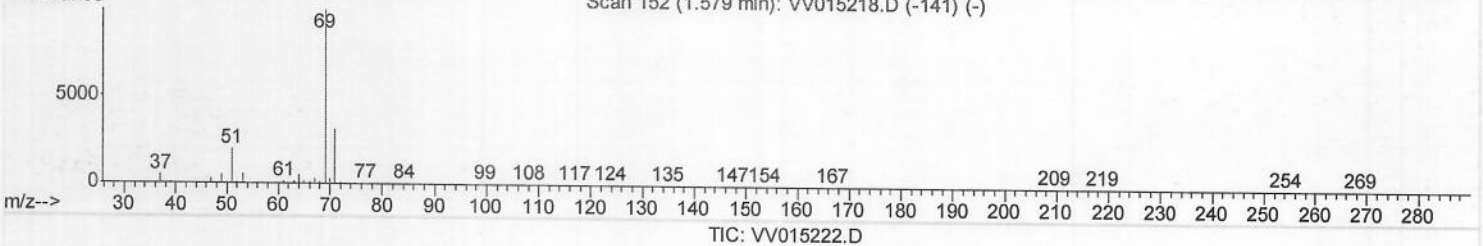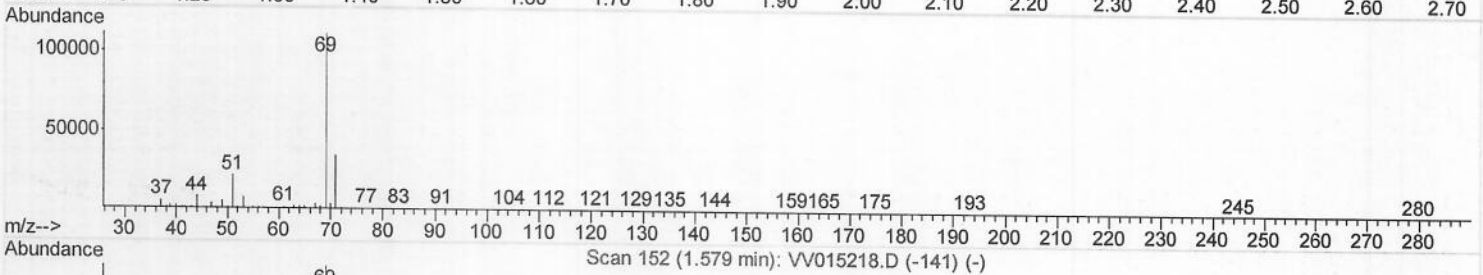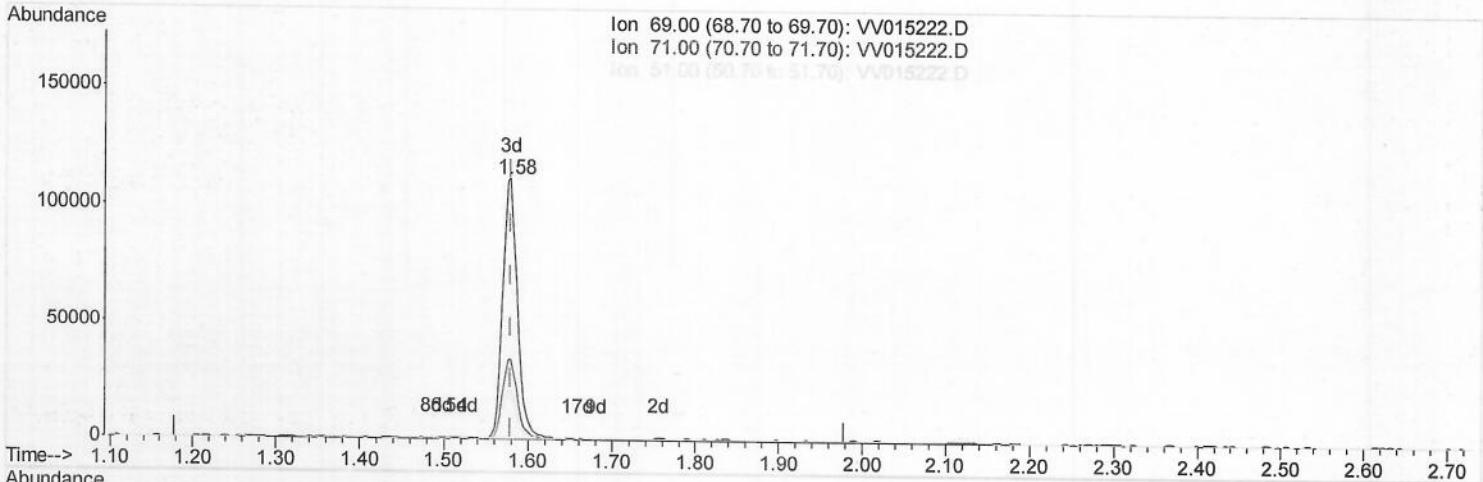

(7) Chloroethane-d5 (S)

1.579min (-0.000) 47.58ug/L m

response 135530

Ion	Exp%	Act%
69.00	100	100
71.00	32.80	0.05#
51.00	29.70	0.04#
0.00	0.00	0.00

SY
 03/31/2020

Quantitation Report (QT Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015222.D
 Acq On : 28 Mar 2020 03:56
 Operator : SY/MD
 Sample : L1985-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTL8

Manual Integrations
 APPROVED

apatel
 3/31/2020 9:22:44 AM

Quant Time: Mar 28 06:21:23 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 28 05:21:13 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	654961	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	617948	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	265042	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.31	65	134787	50.72	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 101.44%			
7) Chloroethane-d5	1.58	69	135530m7	47.58	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 95.16%			
11) 1,1-Dichloroethene-d2	2.12	63	218145	32.83	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 65.66%			
21) 2-Butanone-d5	3.94	46	209766	66.63	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 66.63%			
24) Chloroform-d	4.38	84	274019	39.53	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 79.06%			
26) 1,2-Dichloroethane-d4	5.06	65	181198	40.11	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 80.22%			
32) Benzene-d6	5.08	84	516863	47.50	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 95.00%			
36) 1,2-Dichloropropane-d6	6.10	67	170293	41.79	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 83.58%			
41) Toluene-d8	7.34	98	467027	48.71	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 97.42%			
43) trans-1,3-Dichloropropene-	7.64	79	84818	38.95	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 77.90%			
47) 2-Hexanone-d5	8.12	63	164945	70.12	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 70.12%			
57) 1,1,2,2-Tetrachloroethane-	10.24	84	253619	35.33	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 70.66%			
64) 1,2-Dichlorobenzene-d4	11.65	152	180931	40.02	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 80.04%			

Target Compounds

(#) = qualifier out of range (m) = manual integration (+) = signals summed

SY
 03/31/2020

Quantitation Report (QT Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015222.D
 Acq On : 28 Mar 2020 03:56
 Operator : SY/MD
 Sample : L1985-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTL8

Manual Integrations
 APPROVED

apatel
 3/31/2020 9:22:44 AM

Quant Time: Mar 28 06:21:23 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 28 05:21:13 2020
 Response via : Initial Calibration

