

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015255.D
 Acq On : 28 Mar 2020 18:54
 Operator : SY/MD
 Sample : L1975-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTH2

Manual Integrations
 APPROVED

apatel
 3/31/2020 9:24:49 AM

Quant Time: Mar 30 02:16:37 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Mar 30 02:13:00 2020
 Response via : Initial Calibration

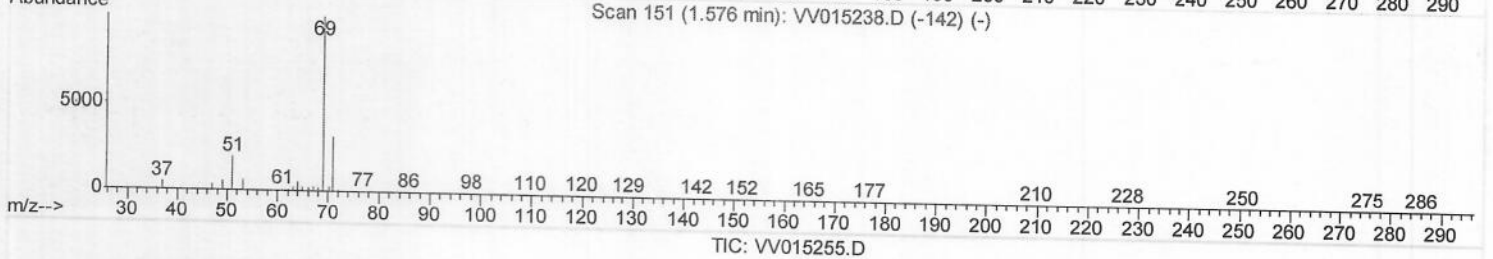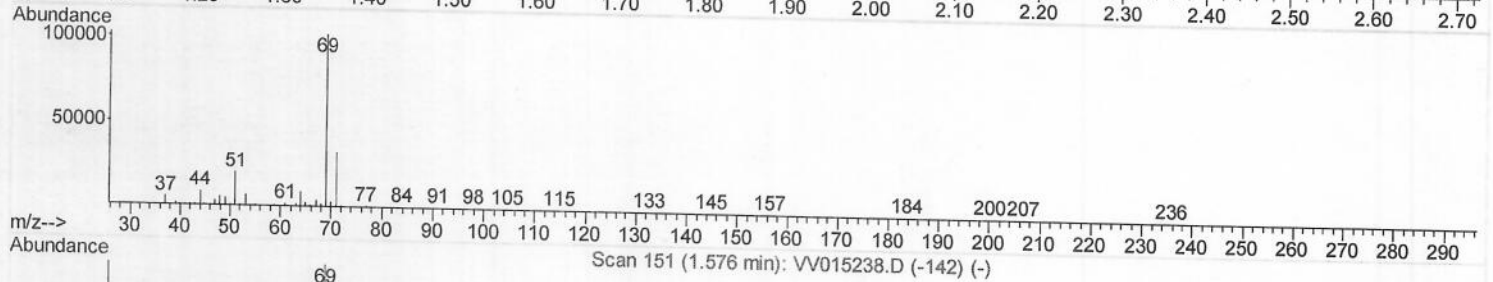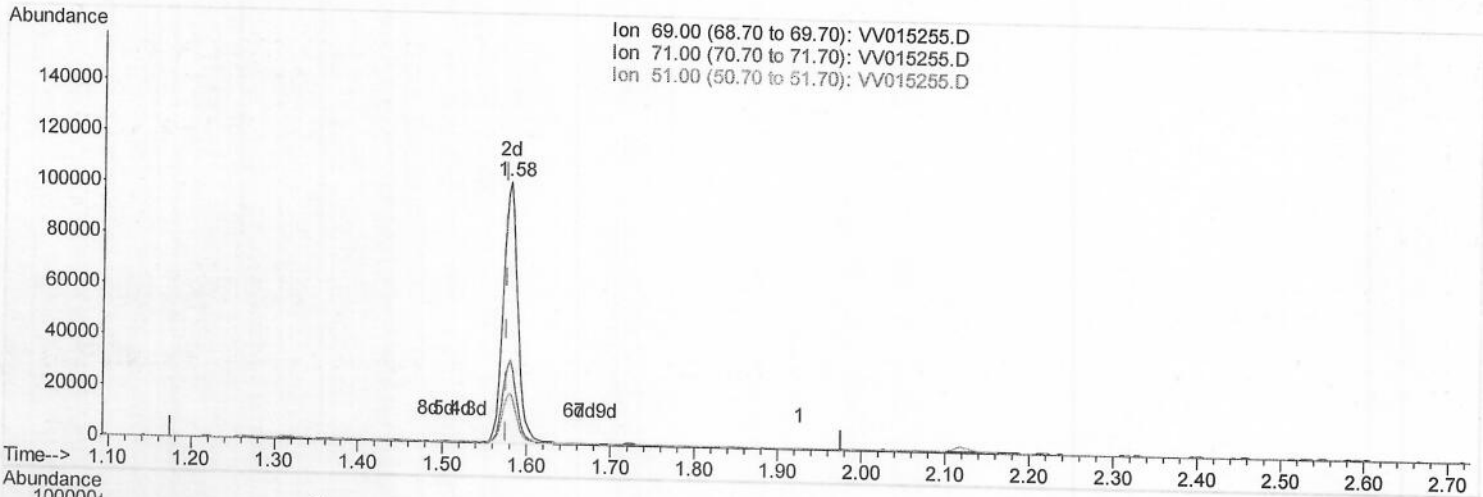

(7) Chloroethane-d5 (S)

1.579min (+0.003) 49.64ug/L m

response 121604

Ion	Exp%	Act%
69.00	100	100
71.00	32.80	0.09#
51.00	29.70	0.05#
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015255.D
 Acq On : 28 Mar 2020 18:54
 Operator : SY/MD
 Sample : L1975-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTH2

Manual Integrations
 APPROVED

apatel
 3/31/2020 9:24:49 AM

Quant Time: Mar 30 04:41:54 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Mar 30 02:13:00 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	563284	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	530452	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	223258	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.32	65	119286	52.19	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	104.38%		
7) Chloroethane-d5	1.58	69	121604m	49.64	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	99.28%		
11) 1,1-Dichloroethene-d2	2.12	63	188215	32.93	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	65.86%		
21) 2-Butanone-d5	3.93	46	196389	72.54	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	72.54%		
24) Chloroform-d	4.38	84	253340	42.50	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	85.00%		
26) 1,2-Dichloroethane-d4	5.06	65	173740	44.72	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.44%		
32) Benzene-d6	5.08	84	465202	49.81	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	99.62%		
36) 1,2-Dichloropropane-d6	6.10	67	161158	46.07	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	92.14%		
41) Toluene-d8	7.34	98	419795	51.00	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	102.00%		
43) trans-1,3-Dichloropropene-	7.64	79	74533	39.87	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	79.74%		
47) 2-Hexanone-d5	8.12	63	161285	79.88	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	79.88%		
57) 1,1,2,2-Tetrachloroethane-	10.24	84	240853	39.09	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	78.18%		
64) 1,2-Dichlorobenzene-d4	11.65	152	162945	42.79	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	85.58%		
Target Compounds						
5) Vinyl chloride	1.32	62	6792	1.355	ug/L #	44
20) cis-1,2-Dichloroethene	3.95	96	5762	1.329	ug/L #	82

(#) = qualifier out of range (m) = manual integration (+) = signals summed

SY
 03/31/2020

Quantitation Report (QT Reviewed)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015255.D
 Acq On : 28 Mar 2020 18:54
 Operator : SY/MD
 Sample : L1975-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTH2

Manual Integrations
 APPROVED

apatel
 3/31/2020 9:24:49 AM

Quant Time: Mar 30 04:41:54 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Mar 30 02:13:00 2020
 Response via : Initial Calibration

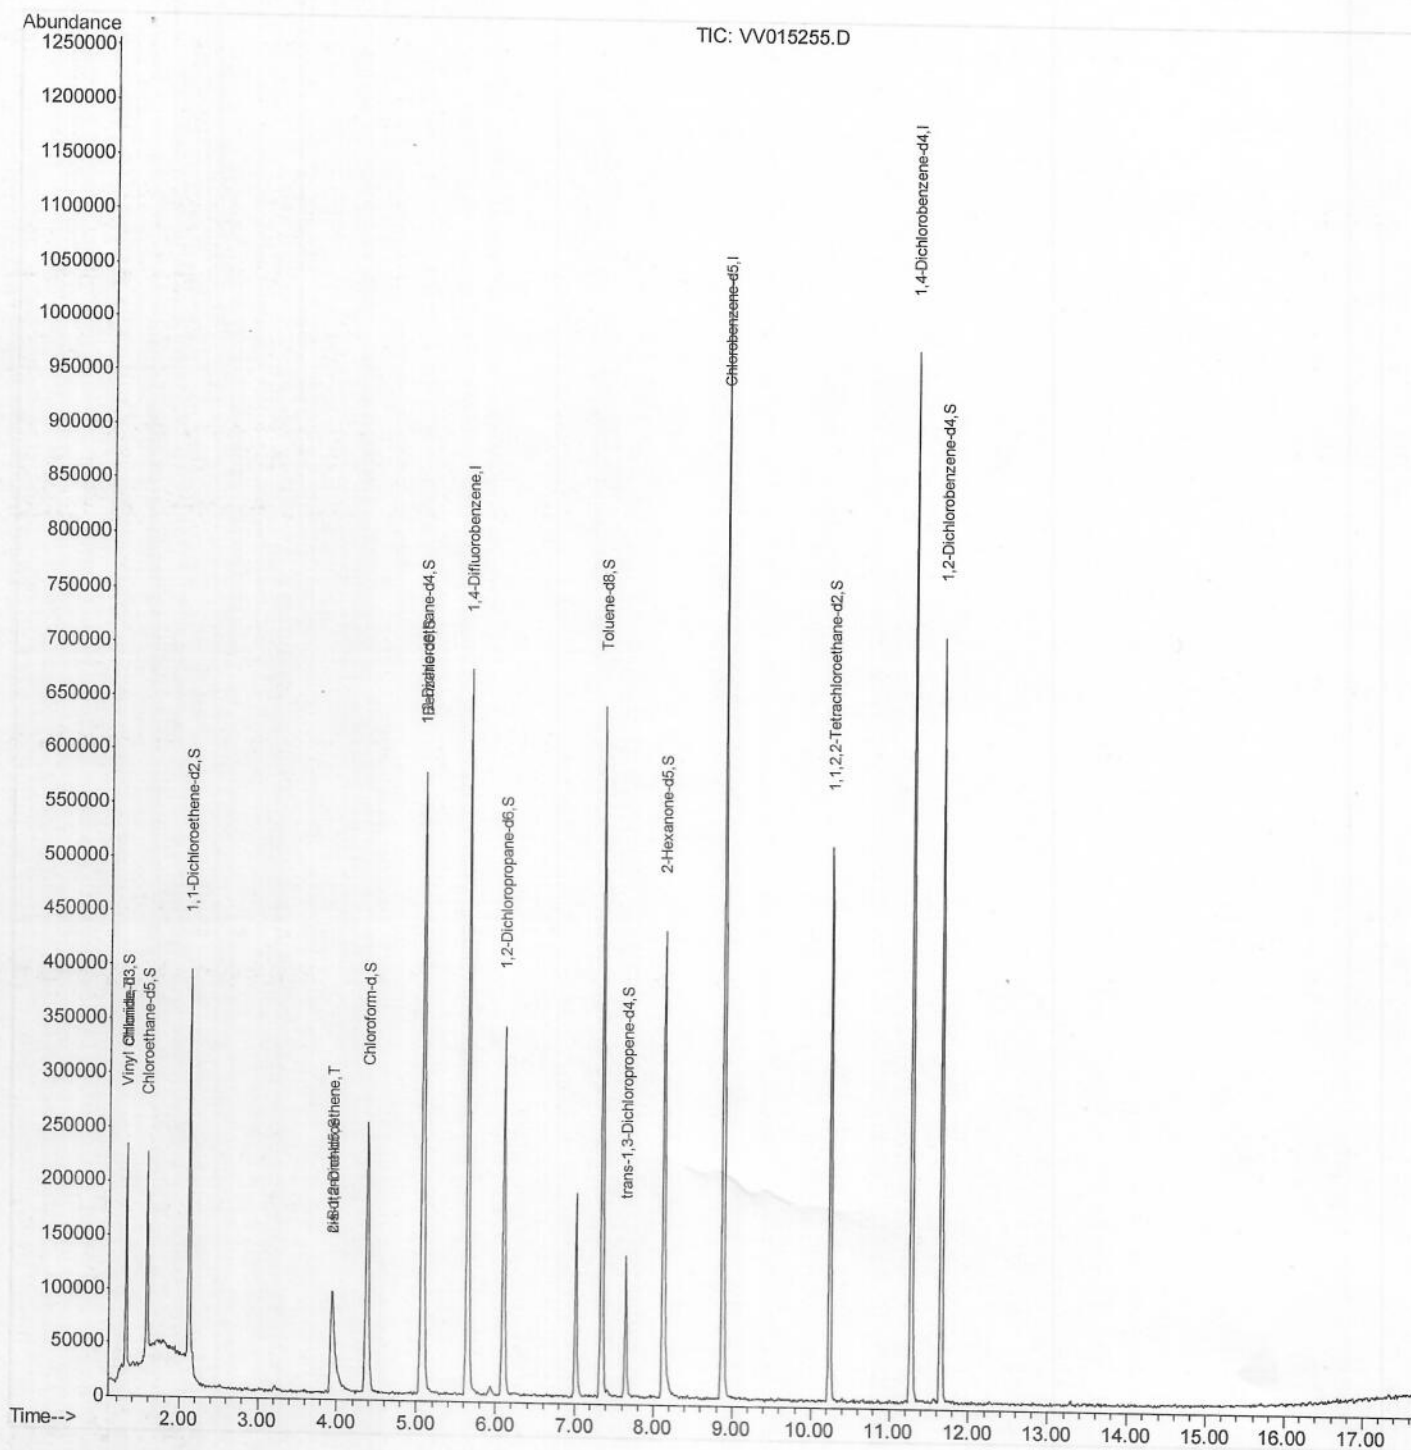

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015255.D
 Acq On : 28 Mar 2020 18:54
 Operator : SY/MD
 Sample : L1975-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTH2

Manual Integrations
 APPROVED

apatel
 3/31/2020 9:24:49 AM

Quant Time: Mar 30 02:16:37 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Mar 30 02:13:00 2020
 Response via : Initial Calibration

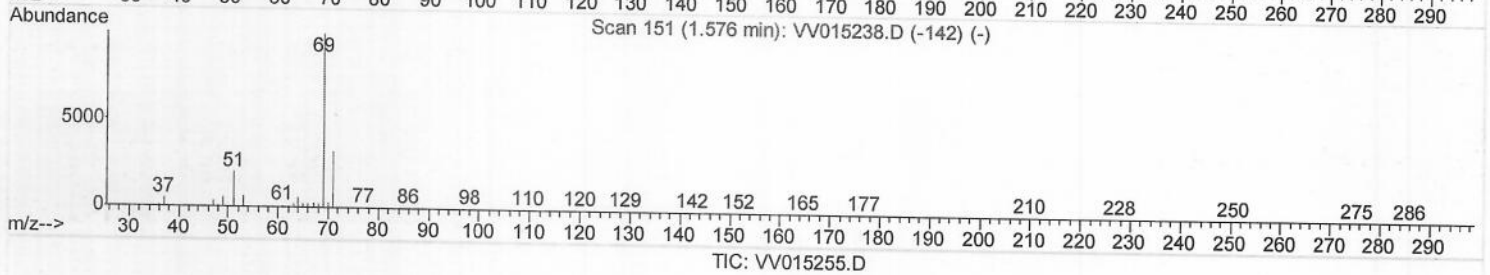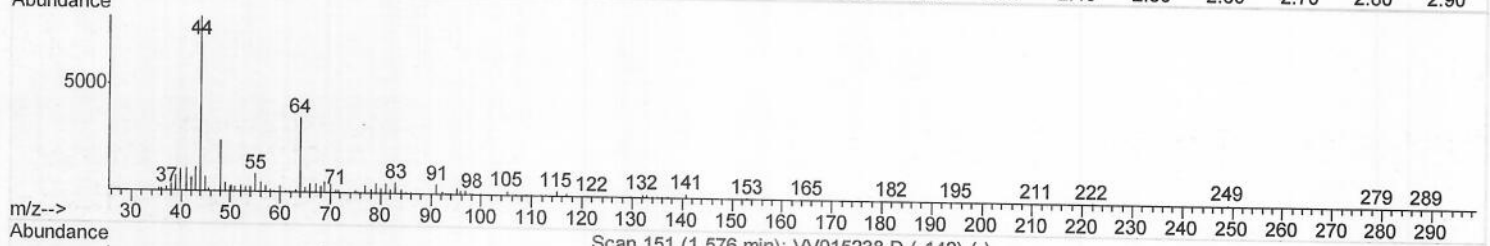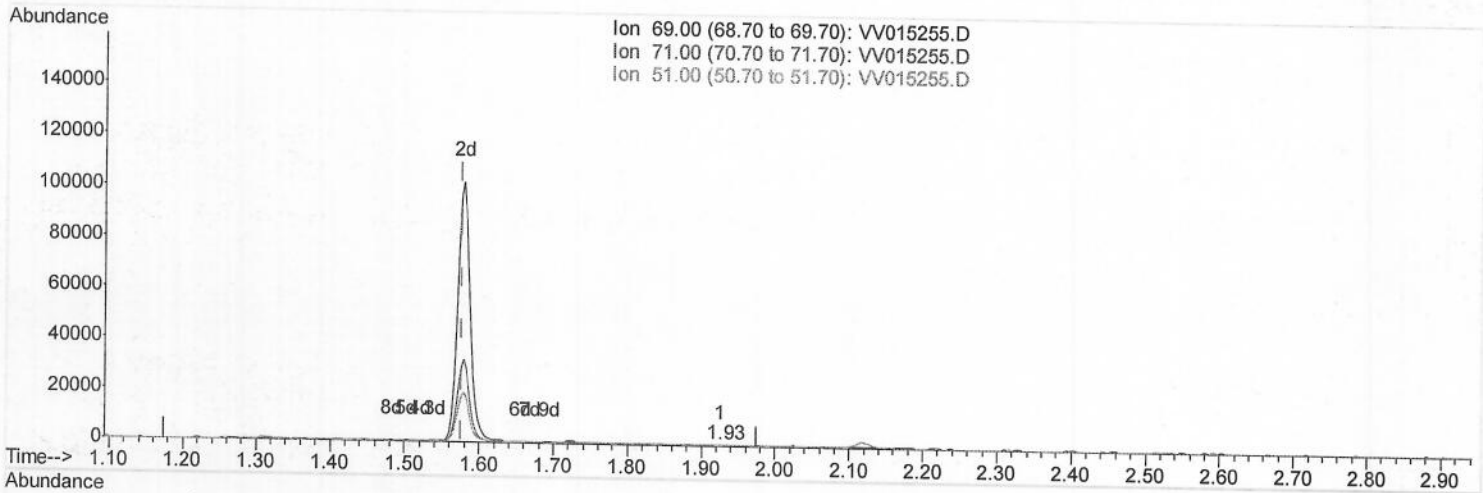

(7) Chloroethane-d5 (S)
 1.926min (+0.350) 0.11ug/L
 response 270

Ion	Exp%	Act%
69.00	100	100
71.00	32.80	41.48
51.00	29.70	21.11
0.00	0.00	0.00