

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015221.D
 Acq On : 28 Mar 2020 03:32
 Operator : SY/MD
 Sample : L2005-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DN1

Quant Time: Mar 28 06:11:06 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 28 05:21:13 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	665054	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	630683	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	266972	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	134533	49.86	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	99.72%
7) Chloroethane-d5	1.58	69	131245	45.37	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	90.74%
11) 1,1-Dichloroethene-d2	2.12	63	219426	32.52	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	65.04%
21) 2-Butanone-d5	3.94	46	208160	65.12	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	65.12%
24) Chloroform-d	4.38	84	275654	39.16	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	78.32%
26) 1,2-Dichloroethane-d4	5.06	65	181064	39.47	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	78.94%
32) Benzene-d6	5.08	84	512520	46.15	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.30%
36) 1,2-Dichloropropane-d6	6.09	67	168783	40.58	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	81.16%
41) Toluene-d8	7.34	98	466761	47.70	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.40%
43) trans-1,3-Dichloropropene-	7.64	79	86980	39.13	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	78.26%
47) 2-Hexanone-d5	8.12	63	167012	69.57	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	69.57%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	255269	34.84	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	69.68%
64) 1,2-Dichlorobenzene-d4	11.65	152	181999	39.96	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	79.92%#


Target Compounds				Ovalue
13) Acetone	2.22	43	11968	6.413 ug/L # 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032720\
Data File : VV015221.D
Acq On : 28 Mar 2020 03:32
Operator : SY/MD
Sample : L2005-09
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DN1

Quant Time: Mar 28 06:11:06 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 28 05:21:13 2020
Response via : Initial Calibration

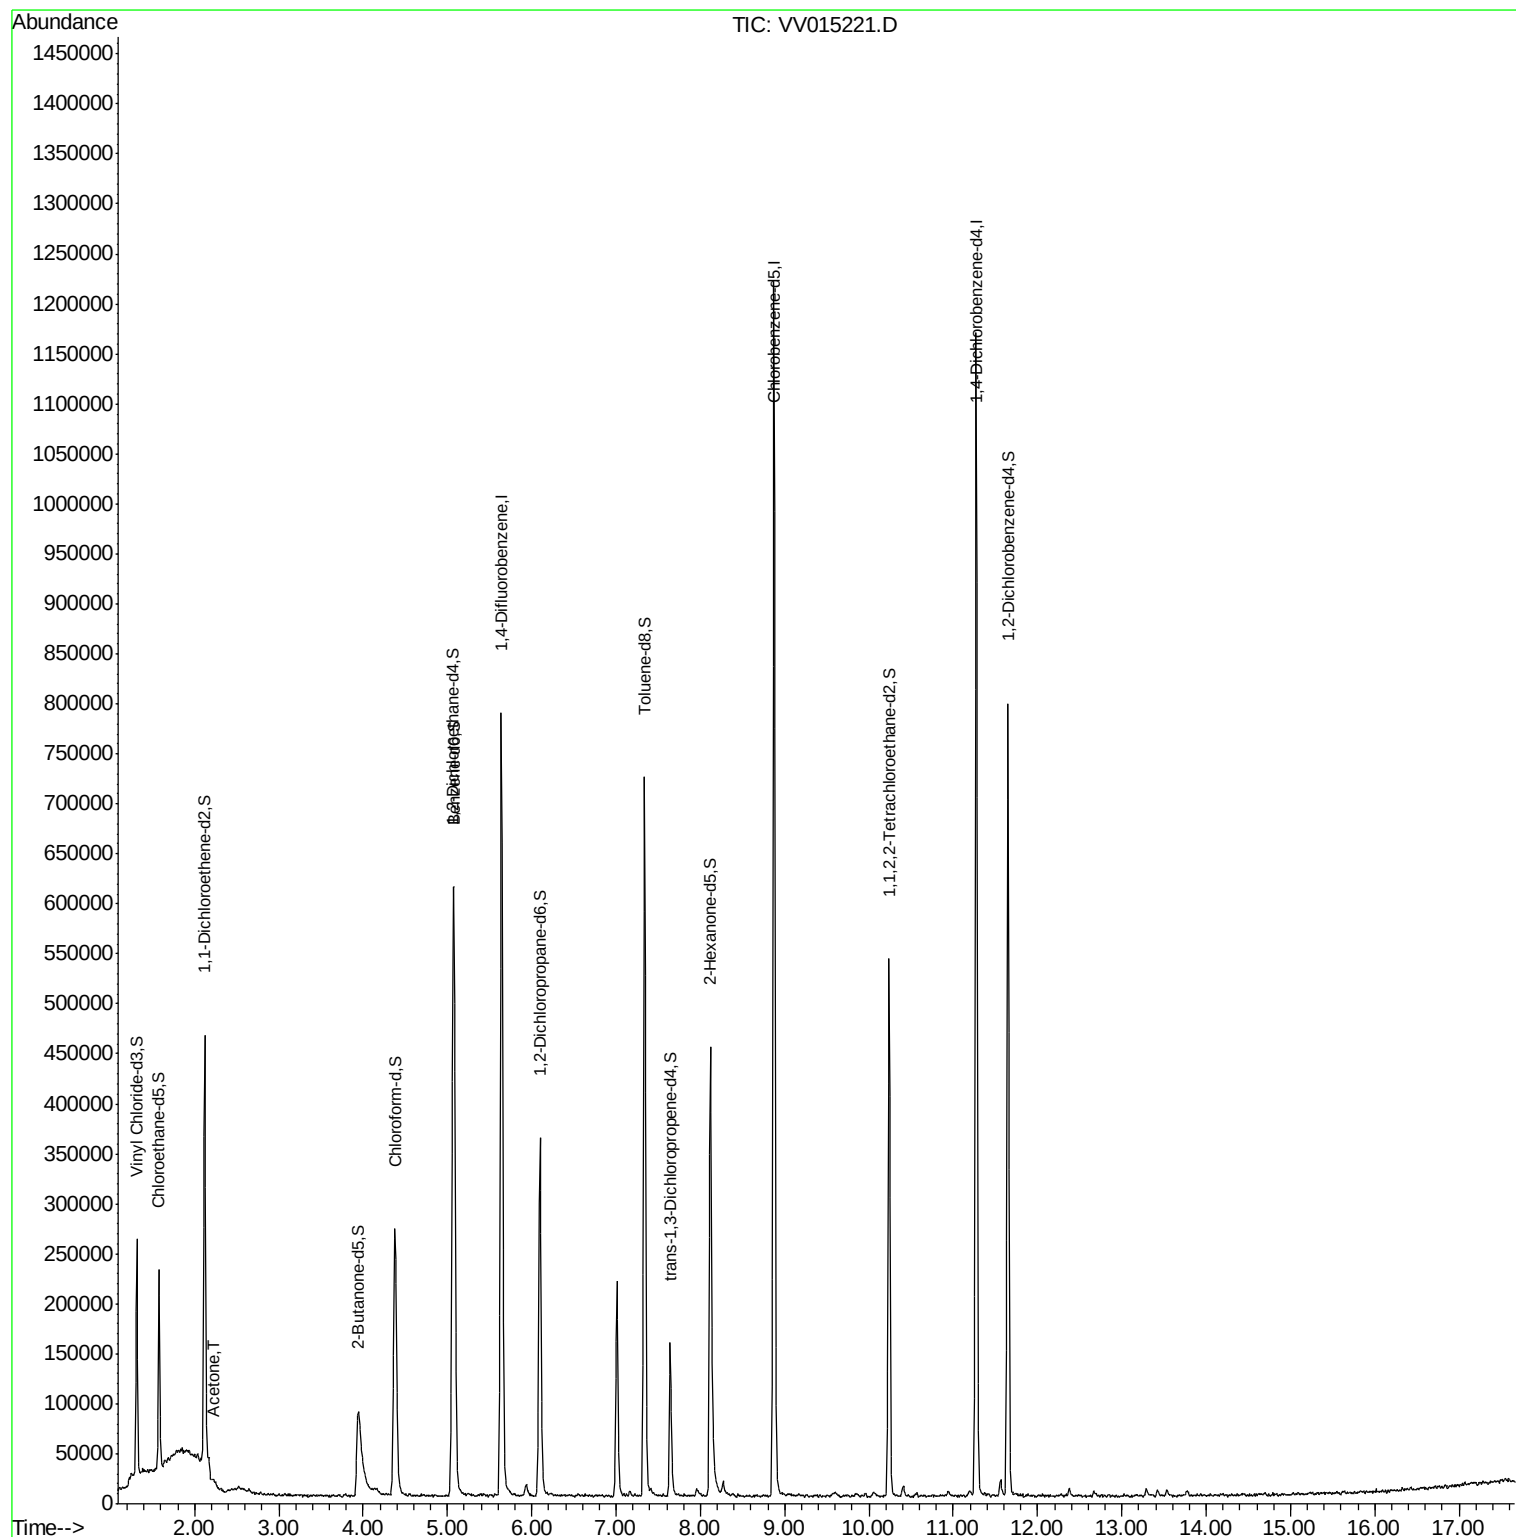

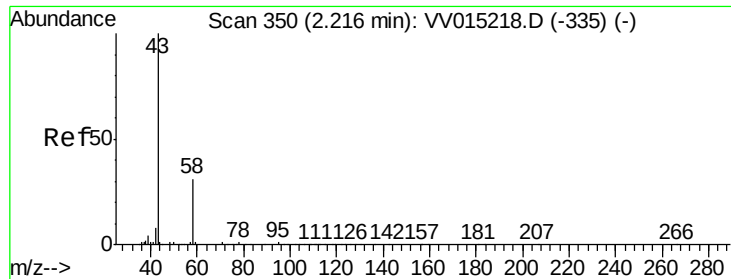

#13

Acetone

Concen: 6.413 ug/L

RT: 2.22 min Scan# 351

Delta R.T. 0.00 min

Lab File: VV015221.D

Acq: 28 Mar 2020 03:32

Instrument :
MSVOA_V
ClientSampleId :
C0DN1

Tot Ion: 43 Resp: 11968

Ion Ratio Lower Upper

43 100

58 15.1 0.0 0.0#

