

Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV032720\
 Data File : VV015219.D
 Acq On : 28 Mar 2020 02:19
 Operator : SY/MD
 Sample : VV0327WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK95

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	64	69	81	rVB	203522	207382	11.74%	1.303%
2	1.576	146	151	164	rVB	203750	235750	13.35%	1.481%
3	2.119	314	320	332	rVB	359452	492139	27.87%	3.093%
4	2.945	575	577	581	rVB4	2412	1061	0.06%	0.007%
5	3.023	598	601	606	rBV6	3523	2898	0.16%	0.018%
6	3.145	636	639	642	rBV4	3338	2676	0.15%	0.017%
7	3.550	763	765	767	rBV2	1751	1068	0.06%	0.007%
8	3.663	797	800	802	rBV4	1713	1101	0.06%	0.007%
9	3.753	826	828	835	rVB7	3296	3438	0.19%	0.022%
10	3.936	869	885	920	rBV	129942	577574	32.71%	3.629%
11	4.376	1007	1022	1045	rBV	311449	766787	43.42%	4.818%
12	4.576	1076	1084	1088	rBV	3635	5125	0.29%	0.032%
13	4.659	1107	1110	1112	rBV4	1854	1174	0.07%	0.007%
14	4.769	1142	1144	1148	rBV5	1712	1007	0.06%	0.006%
15	4.894	1179	1183	1184	rBV4	1751	1055	0.06%	0.007%
16	4.984	1209	1211	1214	rBV4	1426	911	0.05%	0.006%
17	5.071	1222	1238	1265	rBV2	675411	1710436	96.86%	10.748%
18	5.640	1399	1415	1438	rBV	714057	1411652	79.94%	8.871%
19	5.875	1486	1488	1491	rBV3	2170	1347	0.08%	0.008%
20	6.093	1543	1556	1583	rBV2	426364	884819	50.11%	5.560%
21	6.296	1617	1619	1620	rBV2	1945	782	0.04%	0.005%
22	6.357	1633	1638	1641	rBV7	1447	1297	0.07%	0.008%
23	6.482	1674	1677	1679	rVB4	1372	885	0.05%	0.006%
24	6.534	1690	1693	1695	rBV3	1868	1266	0.07%	0.008%
25	6.617	1716	1719	1721	rBV3	2184	1247	0.07%	0.008%
26	6.849	1786	1791	1796	rBV9	2063	2465	0.14%	0.015%
27	7.006	1830	1840	1857	rVV	251736	446394	25.28%	2.805%
28	7.257	1915	1918	1922	rBV5	3898	3398	0.19%	0.021%
29	7.338	1931	1943	1962	rBV	713424	1220374	69.11%	7.669%
30	7.643	2026	2038	2061	rBV	190636	323235	18.30%	2.031%
31	7.830	2091	2096	2098	rBV5	1530	1429	0.08%	0.009%
32	7.865	2104	2107	2116	rVB5	2864	3899	0.22%	0.025%
33	7.939	2128	2130	2133	rBV3	1605	946	0.05%	0.006%
34	7.994	2143	2147	2151	rBV6	5239	5934	0.34%	0.037%

Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV032720\
 Data File : VV015219.D
 Acq On : 28 Mar 2020 02:19
 Operator : SY/MD
 Sample : VV0327WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK95

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

35	8.058	2164	2167	2169	rBV4	1863	991	0.06%	0.006%
36	8.116	2173	2185	2211	rBV2	668857	1350434	76.48%	8.486%
37	8.440	2284	2286	2292	rBV6	2410	2478	0.14%	0.016%
38	8.675	2356	2359	2363	rVB5	1946	1371	0.08%	0.009%
39	8.704	2366	2368	2374	rVB8	1911	1394	0.08%	0.009%
40	8.736	2374	2378	2381	rBV5	1579	1371	0.08%	0.009%
41	8.874	2403	2421	2443	rBV	1101731	1765840	100.00%	11.096%
42	9.257	2537	2540	2542	rBV4	2335	1330	0.08%	0.008%
43	9.338	2562	2565	2568	rBV5	2006	1349	0.08%	0.008%
44	9.456	2599	2602	2604	rBV4	2310	1445	0.08%	0.009%
45	9.489	2609	2612	2615	rVV4	2572	1747	0.10%	0.011%
46	9.508	2615	2618	2621	rVB4	1400	959	0.05%	0.006%
47	9.572	2628	2638	2642	rBV8	6400	11052	0.63%	0.069%
48	9.736	2685	2689	2692	rBV5	1690	1154	0.07%	0.007%
49	9.801	2706	2709	2710	rBV3	1315	868	0.05%	0.005%
50	9.952	2748	2756	2757	rBV8	6829	5924	0.34%	0.037%
51	10.238	2833	2845	2865	rBV	734835	1172684	66.41%	7.369%
52	10.482	2918	2921	2926	rBV6	1297	1461	0.08%	0.009%
53	10.501	2926	2927	2932	rBV5	1757	1439	0.08%	0.009%
54	10.643	2968	2971	2975	rBV4	1826	1468	0.08%	0.009%
55	11.016	3083	3087	3090	rVB5	2024	1777	0.10%	0.011%
56	11.035	3090	3093	3096	rBV4	1645	1339	0.08%	0.008%
57	11.090	3106	3110	3117	rVB8	2564	2694	0.15%	0.017%
58	11.125	3117	3121	3123	rBV5	1691	1179	0.07%	0.007%
59	11.164	3131	3133	3135	rBV3	2153	1215	0.07%	0.008%
60	11.273	3156	3167	3190	rVB	1065363	1639668	92.85%	10.304%
61	11.453	3218	3223	3226	rBV7	2434	2428	0.14%	0.015%
62	11.585	3261	3264	3267	rBV3	1379	1011	0.06%	0.006%
63	11.649	3271	3284	3300	rVV	956090	1509258	85.47%	9.484%
64	11.858	3346	3349	3355	rBV8	1750	1618	0.09%	0.010%
65	11.923	3366	3369	3372	rBV5	997	830	0.05%	0.005%
66	11.945	3375	3376	3379	rVB3	1461	766	0.04%	0.005%
67	12.058	3409	3411	3415	rVB4	1912	937	0.05%	0.006%
68	12.093	3418	3422	3426	rVV7	1682	1153	0.07%	0.007%
69	12.125	3429	3432	3433	rBV3	1940	1110	0.06%	0.007%
70	12.193	3445	3453	3457	rBV8	2268	2776	0.16%	0.017%
71	12.225	3461	3463	3465	rBV3	1167	833	0.05%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV032720\
 Data File : VV015219.D
 Acq On : 28 Mar 2020 02:19
 Operator : SY/MD
 Sample : VV0327WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK95

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

72	12.328	3491	3495	3498	rBV6	1853	1375	0.08%	0.009%
73	12.347	3498	3501	3506	rBV6	2758	2228	0.13%	0.014%
74	12.386	3511	3513	3521	rBV8	2805	2486	0.14%	0.016%
75	12.456	3528	3535	3540	rBV9	2630	3695	0.21%	0.023%
76	12.524	3554	3556	3562	rBV7	2494	2455	0.14%	0.015%
77	12.620	3583	3586	3588	rBV4	2625	1689	0.10%	0.011%
78	12.672	3596	3602	3609	rVB5	14866	21122	1.20%	0.133%
79	12.900	3670	3673	3676	rBV5	2026	1620	0.09%	0.010%
80	12.929	3680	3682	3687	rVB6	2604	2127	0.12%	0.013%
81	12.964	3687	3693	3697	rBV8	2647	3040	0.17%	0.019%
82	12.987	3697	3700	3705	rVB5	1483	1084	0.06%	0.007%
83	13.029	3711	3713	3716	rBV3	2160	1292	0.07%	0.008%
84	13.080	3726	3729	3733	rVB6	2572	1756	0.10%	0.011%
85	13.148	3744	3750	3755	rBV8	2287	2593	0.15%	0.016%
86	13.199	3762	3766	3770	rBV6	2398	2099	0.12%	0.013%
87	13.231	3773	3776	3781	rBV6	2137	2318	0.13%	0.015%
88	13.360	3812	3816	3817	rBV4	2285	1079	0.06%	0.007%
89	13.694	3918	3920	3924	rVB4	1682	1052	0.06%	0.007%
90	13.720	3924	3928	3930	rBV4	2732	1939	0.11%	0.012%
91	13.768	3937	3943	3952	rVB5	16371	25019	1.42%	0.157%
92	13.958	4000	4002	4006	rVB4	1953	1342	0.08%	0.008%
93	13.980	4006	4009	4010	rBV3	1848	1023	0.06%	0.006%
94	14.064	4033	4035	4037	rBV3	1595	864	0.05%	0.005%
95	14.151	4059	4062	4064	rBV3	1914	1178	0.07%	0.007%
96	14.222	4081	4084	4085	rBV3	1796	1192	0.07%	0.007%
97	14.376	4130	4132	4134	rBV3	2314	1066	0.06%	0.007%
98	14.498	4166	4170	4174	rBV6	2607	2765	0.16%	0.017%
99	14.537	4180	4182	4183	rBV2	1763	793	0.04%	0.005%
100	15.051	4340	4342	4344	rBV3	1927	897	0.05%	0.006%


Sum of corrected areas: 15913490

Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV032720\
Data File : VV015219.D
Acq On : 28 Mar 2020 02:19
Operator : SY/MD
Sample : VV0327WBL01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
VBLK95

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

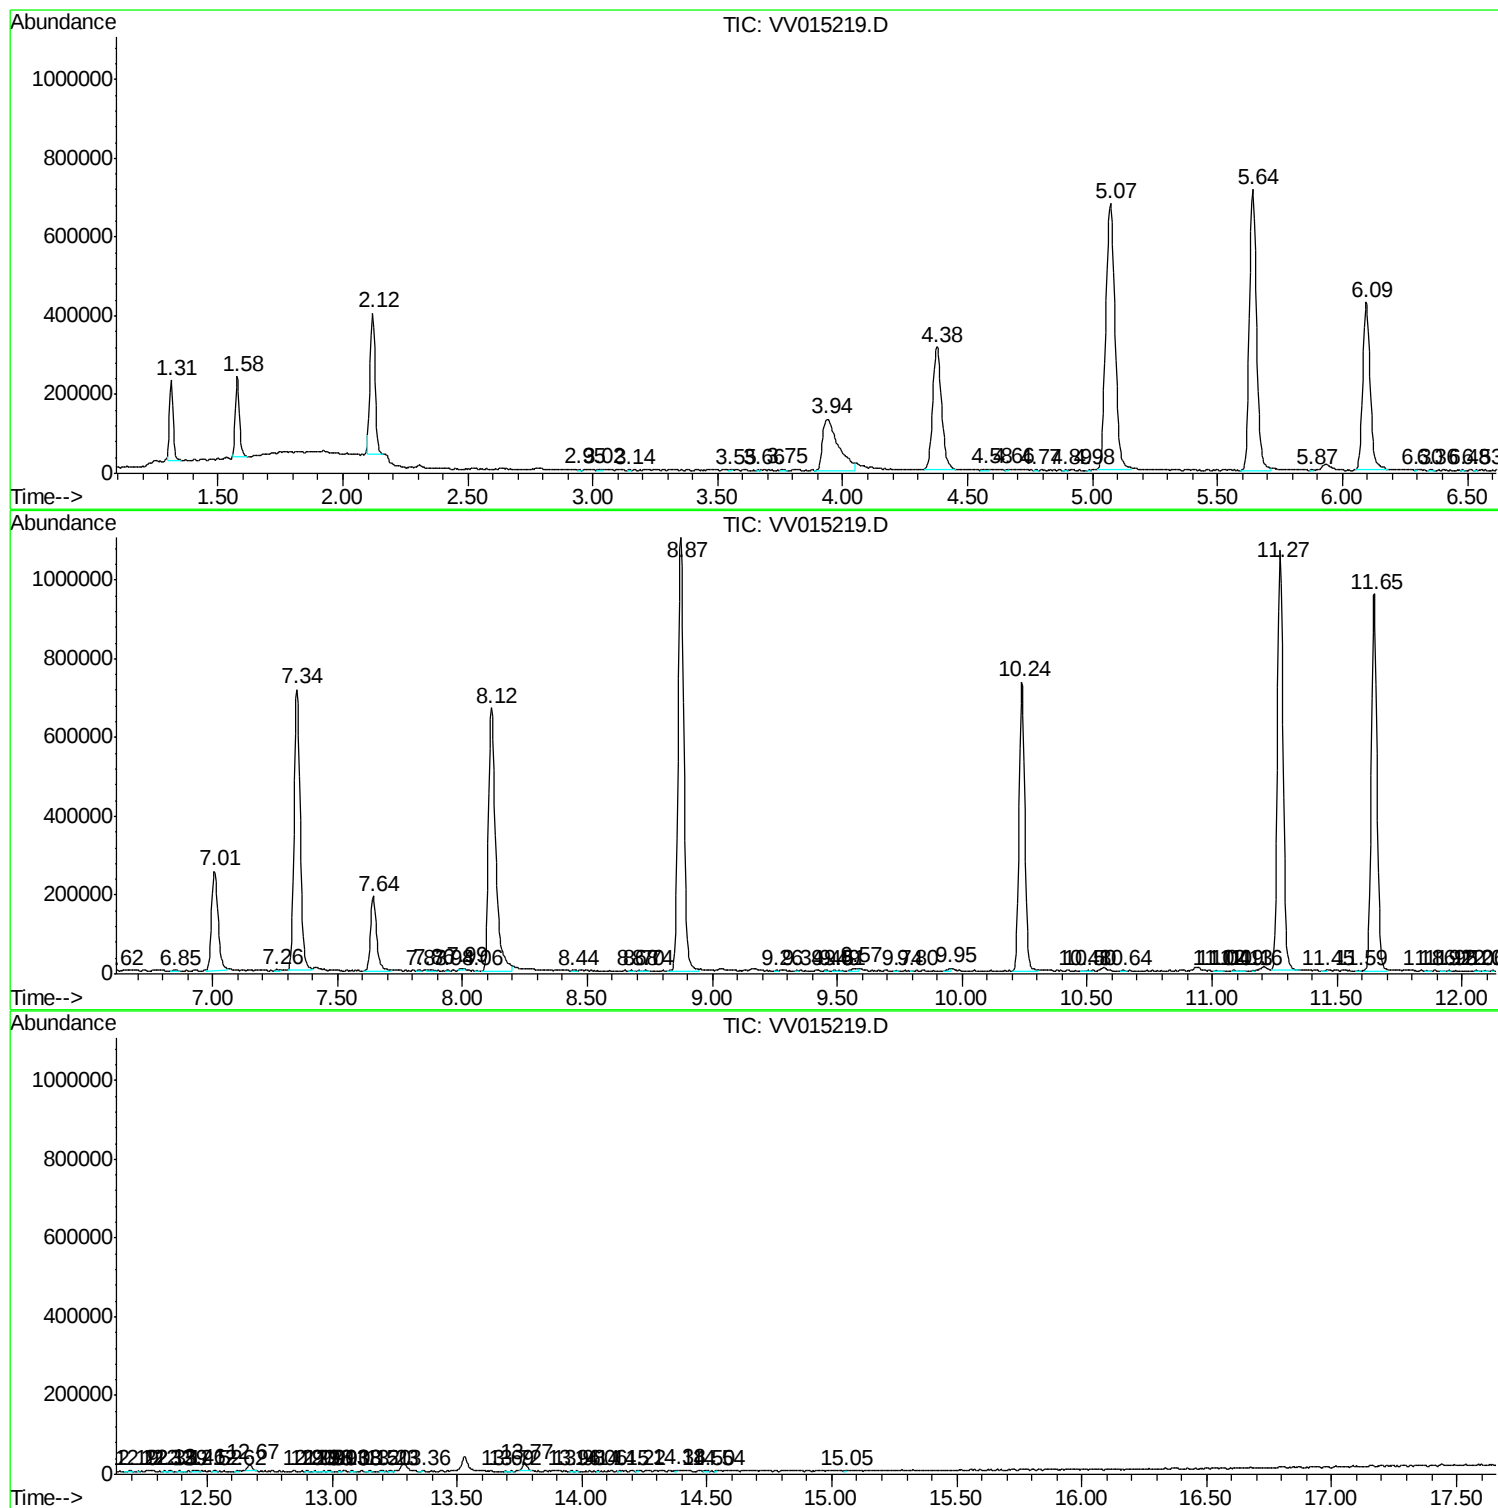

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032720\
Data File : VV015219.D
Acq On : 28 Mar 2020 02:19
Operator : SY/MD
Sample : VV0327WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK95

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032720\
Data File : VV015219.D
Acq On : 28 Mar 2020 02:19
Operator : SY/MD
Sample : VV0327WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK95

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc