

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015220.D
 Acq On : 28 Mar 2020 03:07
 Operator : SY/MD
 Sample : L2003-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EL6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	64	69	80	rVB	222071	228561	12.34%	1.586%
2	1.576	146	151	163	rVB	193876	224275	12.11%	1.556%
3	2.119	313	320	342	rVB	438342	675238	36.47%	4.685%
4	2.910	564	566	569	rBV3	2471	1635	0.09%	0.011%
5	3.074	613	617	619	rBV5	2168	1926	0.10%	0.013%
6	3.283	679	682	685	rBV5	2226	1782	0.10%	0.012%
7	3.380	708	712	713	rBV4	1594	1056	0.06%	0.007%
8	3.489	745	746	748	rBV2	1362	653	0.04%	0.005%
9	3.662	798	800	802	rBV3	910	561	0.03%	0.004%
10	3.759	824	830	833	rBV8	2081	2498	0.13%	0.017%
11	3.939	875	886	915	rBV2	87509	353238	19.08%	2.451%
12	4.376	1010	1022	1044	rVB	262886	638494	34.49%	4.430%
13	4.666	1110	1112	1114	rBV3	2028	1102	0.06%	0.008%
14	4.698	1118	1122	1124	rBV4	3273	2222	0.12%	0.015%
15	4.833	1162	1164	1166	rBV3	1624	750	0.04%	0.005%
16	4.936	1193	1196	1198	rBV4	1607	760	0.04%	0.005%
17	4.949	1198	1200	1201	rBV2	1609	681	0.04%	0.005%
18	5.071	1221	1238	1264	rBV2	612808	1542402	83.31%	10.702%
19	5.640	1403	1415	1440	rBV	746774	1473034	79.56%	10.220%
20	6.093	1544	1556	1584	rVB2	358764	735940	39.75%	5.106%
21	6.508	1683	1685	1688	rBV3	1544	1126	0.06%	0.008%
22	6.608	1715	1716	1717	rBV	1807	642	0.03%	0.004%
23	6.698	1739	1744	1746	rBV6	2868	2512	0.14%	0.017%
24	6.723	1750	1752	1756	rVB4	1233	748	0.04%	0.005%
25	6.778	1767	1769	1770	rBV2	1221	442	0.02%	0.003%
26	6.839	1786	1788	1794	rVB7	3166	2761	0.15%	0.019%
27	6.945	1819	1821	1823	rBV3	1187	438	0.02%	0.003%
28	7.006	1830	1840	1865	rVB	210729	379636	20.50%	2.634%
29	7.338	1932	1943	1963	rBV	711123	1233088	66.60%	8.556%
30	7.643	2028	2038	2056	rBV	147874	255198	13.78%	1.771%
31	7.842	2097	2100	2102	rBV4	1502	758	0.04%	0.005%
32	8.116	2175	2185	2219	rBV2	438436	916447	49.50%	6.359%
33	8.646	2347	2350	2352	rVB4	1708	759	0.04%	0.005%
34	8.874	2408	2421	2443	rBV	1147711	1851482	100.00%	12.846%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015220.D
 Acq On : 28 Mar 2020 03:07
 Operator : SY/MD
 Sample : L2003-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EL6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

35	9.141	2502	2504	2506	rBV3	1863	916	0.05%	0.006%
36	9.334	2560	2564	2567	rBV4	1698	1543	0.08%	0.011%
37	9.360	2570	2572	2574	rBV3	1558	820	0.04%	0.006%
38	9.399	2580	2584	2587	rBV5	1722	1516	0.08%	0.011%
39	9.450	2597	2600	2603	rVB5	1722	1047	0.06%	0.007%
40	9.485	2603	2611	2613	rBV8	2437	2815	0.15%	0.020%
41	9.524	2621	2623	2624	rBV2	737	269	0.01%	0.002%
42	9.563	2626	2635	2636	rBV9	3229	3429	0.19%	0.024%
43	9.829	2715	2718	2719	rBV3	4053	2228	0.12%	0.015%
44	9.891	2735	2737	2740	rBV4	1645	918	0.05%	0.006%
45	10.009	2770	2774	2775	rBV4	1558	1001	0.05%	0.007%
46	10.055	2783	2788	2792	rBV7	4226	5916	0.32%	0.041%
47	10.238	2835	2845	2862	rVB	533883	833105	45.00%	5.780%
48	10.360	2880	2883	2885	rBV4	1679	1122	0.06%	0.008%
49	10.530	2933	2936	2938	rBV4	1917	967	0.05%	0.007%
50	10.556	2938	2944	2945	rBV6	3809	3466	0.19%	0.024%
51	10.627	2964	2966	2970	rBV4	1459	1160	0.06%	0.008%
52	10.784	3011	3015	3018	rBV6	2121	1946	0.11%	0.014%
53	11.087	3105	3109	3111	rBV4	2533	1849	0.10%	0.013%
54	11.157	3128	3131	3132	rBV3	2482	1111	0.06%	0.008%
55	11.273	3155	3167	3183	rBV	1100556	1712351	92.49%	11.881%
56	11.559	3249	3256	3267	rBV4	12900	22746	1.23%	0.158%
57	11.649	3272	3284	3304	rVB	770480	1214730	65.61%	8.428%
58	11.897	3359	3361	3362	rBV2	634	301	0.02%	0.002%
59	11.913	3364	3366	3369	rVB3	2049	1263	0.07%	0.009%
60	11.987	3387	3389	3390	rBV2	1180	566	0.03%	0.004%
61	12.222	3460	3462	3463	rBV2	1427	526	0.03%	0.004%
62	12.370	3504	3508	3516	rBV8	7108	10460	0.56%	0.073%
63	12.514	3550	3553	3555	rVB4	1515	786	0.04%	0.005%
64	12.585	3572	3575	3577	rBV3	999	602	0.03%	0.004%
65	12.598	3577	3579	3582	rVV3	1698	1199	0.06%	0.008%
66	12.630	3586	3589	3591	rBV4	1834	1017	0.05%	0.007%
67	12.672	3595	3602	3614	rBV4	5977	11478	0.62%	0.080%
68	12.794	3639	3640	3641	rBV	945	327	0.02%	0.002%
69	12.897	3669	3672	3673	rBV3	2306	992	0.05%	0.007%
70	12.961	3690	3692	3693	rBV2	1447	609	0.03%	0.004%
71	13.029	3709	3713	3716	rBV5	2356	2205	0.12%	0.015%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
Data File : VV015220.D
Acq On : 28 Mar 2020 03:07
Operator : SY/MD
Sample : L2003-06
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EL6

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Title : VOC Analysis

72	13.286	3785	3793	3803	rBV5	9306	16585	0.90%	0.115%
73	13.427	3831	3837	3841	rBV9	5390	7209	0.39%	0.050%
74	13.993	4011	4013	4015	rBV3	1611	687	0.04%	0.005%
75	14.173	4066	4069	4072	rBV4	2173	1861	0.10%	0.013%
76	14.260	4092	4096	4099	rBV6	2495	2163	0.12%	0.015%
77	14.906	4295	4297	4301	rBV4	2706	2073	0.11%	0.014%


Sum of corrected areas: 14412725

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032720\
Data File : VV015220.D
Acq On : 28 Mar 2020 03:07
Operator : SY/MD
Sample : L2003-06
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EL6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

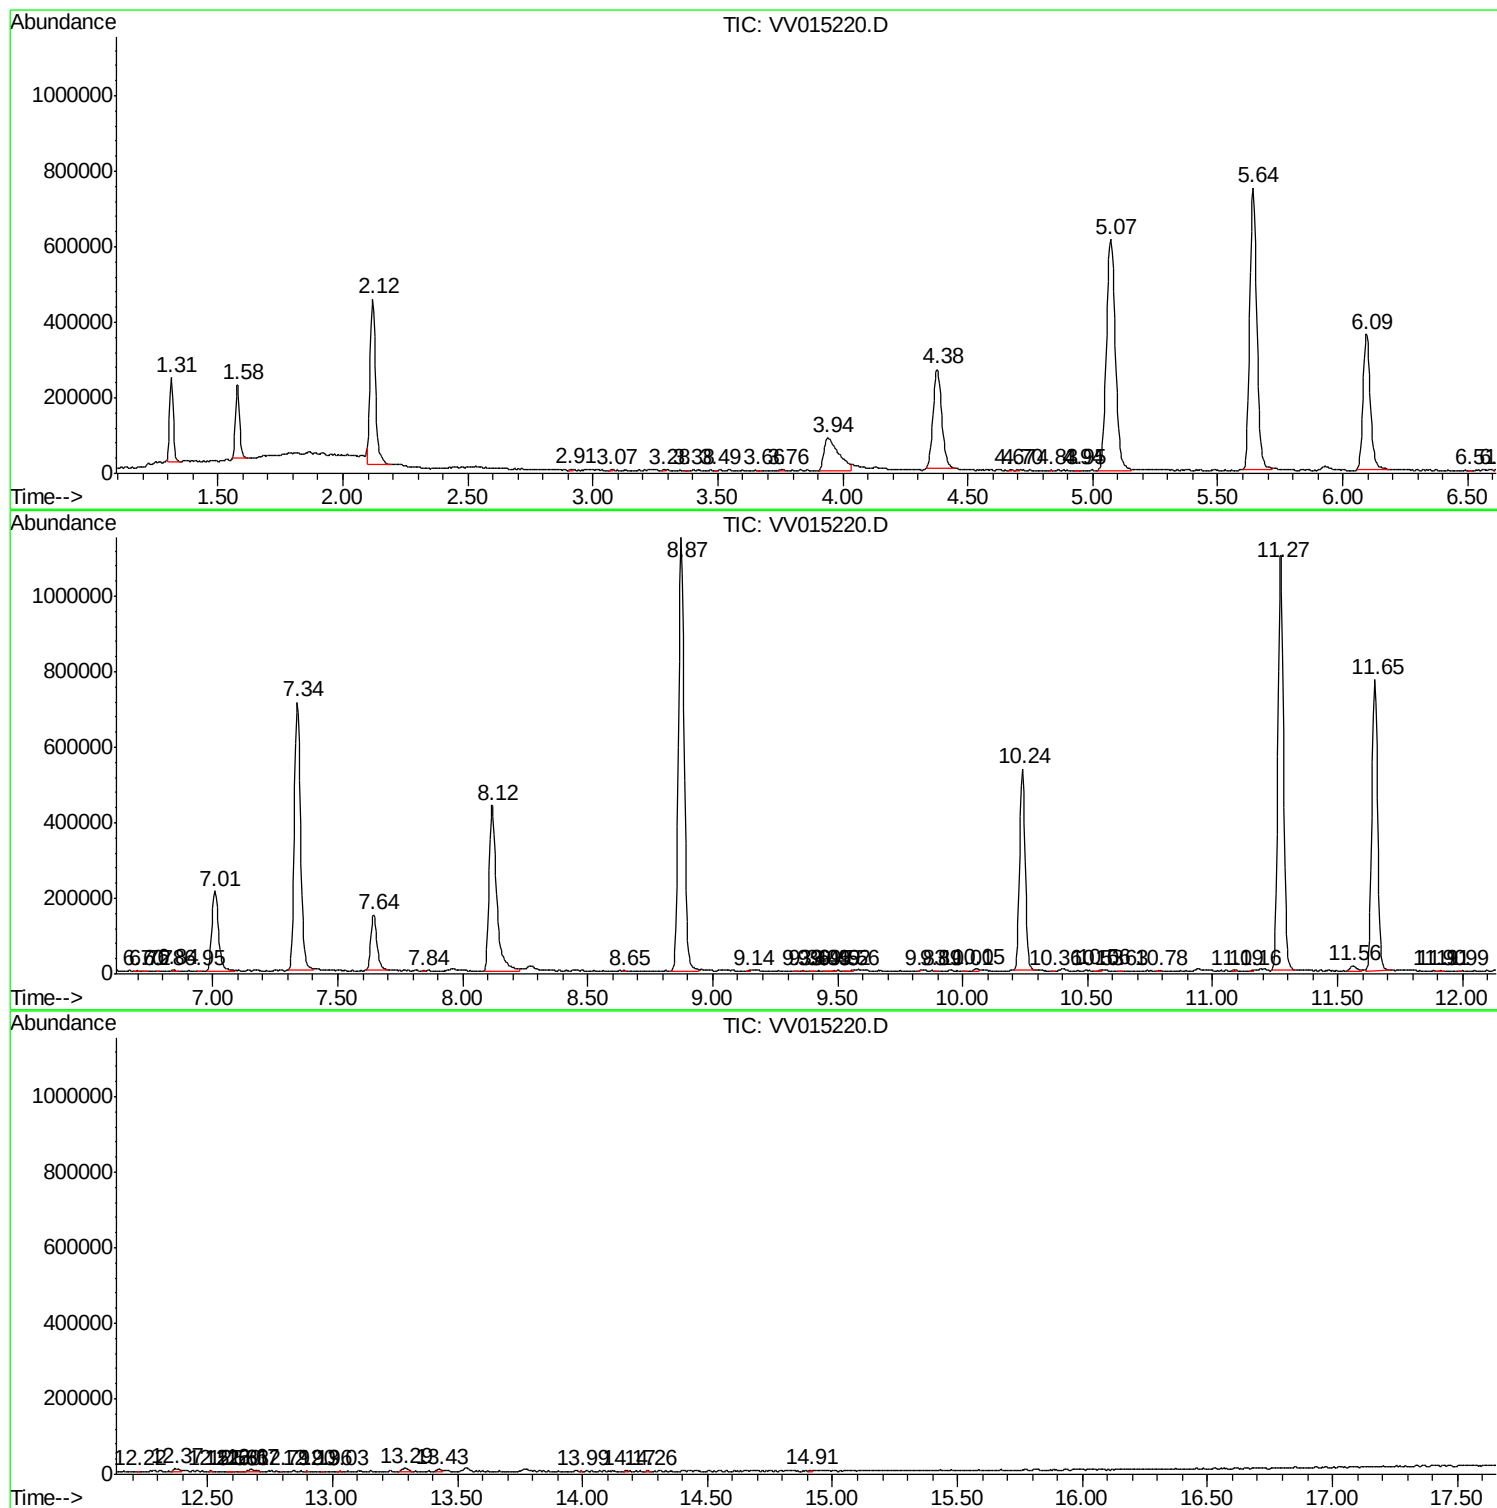

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032720\
Data File : VV015220.D
Acq On : 28 Mar 2020 03:07
Operator : SY/MD
Sample : L2003-06
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0EL6

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032720\
Data File : VV015220.D
Acq On : 28 Mar 2020 03:07
Operator : SY/MD
Sample : L2003-06
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0EL6

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc