

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015221.D
 Acq On : 28 Mar 2020 03:32
 Operator : SY/MD
 Sample : L2005-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DN1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	65	70	81	rVB	233657	228641	11.65%	1.551%
2	1.579	147	152	164	rVB	196101	226749	11.55%	1.538%
3	2.119	314	320	333	rVB	423035	585421	29.83%	3.970%
4	3.135	632	636	638	rBV4	2599	1737	0.09%	0.012%
5	3.293	681	685	686	rBV3	2127	1544	0.08%	0.010%
6	3.360	702	706	708	rBV5	2109	2096	0.11%	0.014%
7	3.447	728	733	735	rBV5	1562	1418	0.07%	0.010%
8	3.605	780	782	785	rVB4	1612	711	0.04%	0.005%
9	3.624	785	788	790	rBV4	1695	1091	0.06%	0.007%
10	3.772	831	834	838	rBV5	2026	1888	0.10%	0.013%
11	3.862	858	862	865	rBV5	2416	1949	0.10%	0.013%
12	3.942	876	887	928	rBV	82532	356758	18.18%	2.419%
13	4.376	1011	1022	1048	rVB	264527	661803	33.72%	4.488%
14	4.605	1091	1093	1097	rVB4	1701	874	0.04%	0.006%
15	4.843	1163	1167	1168	rBV4	1518	1175	0.06%	0.008%
16	4.974	1206	1208	1210	rBV3	1450	769	0.04%	0.005%
17	5.074	1222	1239	1270	rBV2	608952	1552795	79.12%	10.531%
18	5.386	1334	1336	1338	rBV3	1654	668	0.03%	0.005%
19	5.640	1402	1415	1439	rBV	782200	1563199	79.65%	10.601%
20	6.096	1544	1557	1580	rBV2	355794	730384	37.22%	4.953%
21	6.418	1655	1657	1659	rVB3	1713	760	0.04%	0.005%
22	6.630	1721	1723	1726	rVB3	2412	988	0.05%	0.007%
23	6.736	1754	1756	1758	rBV3	1393	657	0.03%	0.004%
24	6.781	1768	1770	1774	rBV5	1360	1047	0.05%	0.007%
25	6.942	1817	1820	1821	rBV3	1847	860	0.04%	0.006%
26	7.010	1826	1841	1859	rVV2	216069	394886	20.12%	2.678%
27	7.093	1863	1867	1871	rBV6	3003	2429	0.12%	0.016%
28	7.273	1922	1923	1928	rBV5	1342	813	0.04%	0.006%
29	7.338	1931	1943	1962	rBV	718818	1238915	63.13%	8.402%
30	7.643	2028	2038	2056	rBV	152983	260509	13.27%	1.767%
31	7.916	2120	2123	2125	rVB5	1715	883	0.04%	0.006%
32	7.955	2129	2135	2138	rBV6	7116	8369	0.43%	0.057%
33	8.119	2175	2186	2221	rBV2	447541	932211	47.50%	6.322%
34	8.444	2283	2287	2292	rBV8	2746	2814	0.14%	0.019%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015221.D
 Acq On : 28 Mar 2020 03:32
 Operator : SY/MD
 Sample : L2005-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DN1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

35	8.617	2338	2341	2343	rBV4	1327	889	0.05%	0.006%
36	8.649	2348	2351	2352	rBV3	1686	898	0.05%	0.006%
37	8.768	2386	2388	2392	rVB5	1424	1018	0.05%	0.007%
38	8.817	2399	2403	2405	rBV4	1516	1134	0.06%	0.008%
39	8.874	2407	2421	2443	rVV	1215122	1962492	100.00%	13.309%
40	9.251	2533	2538	2539	rBV4	2330	1891	0.10%	0.013%
41	9.334	2563	2564	2567	rBV3	1401	872	0.04%	0.006%
42	9.421	2584	2591	2594	rBV8	3052	3168	0.16%	0.021%
43	9.543	2626	2629	2632	rBV5	2036	1502	0.08%	0.010%
44	9.665	2664	2667	2670	rVB5	1306	783	0.04%	0.005%
45	9.784	2701	2704	2705	rBV2	1399	814	0.04%	0.006%
46	9.794	2705	2707	2710	rVV4	2047	1089	0.06%	0.007%
47	9.839	2717	2721	2723	rBV4	3035	2352	0.12%	0.016%
48	9.903	2738	2741	2743	rBV4	1399	1014	0.05%	0.007%
49	9.948	2752	2755	2759	rBV5	2649	2804	0.14%	0.019%
50	10.055	2776	2788	2793	rBV5	5606	10807	0.55%	0.073%
51	10.145	2813	2816	2818	rBV4	1352	854	0.04%	0.006%
52	10.180	2823	2827	2831	rBV6	2189	2307	0.12%	0.016%
53	10.238	2834	2845	2861	rVB	536667	848225	43.22%	5.752%
54	10.508	2924	2929	2930	rBV5	1356	679	0.03%	0.005%
55	10.534	2935	2937	2940	rBV4	1891	954	0.05%	0.006%
56	10.550	2940	2942	2944	rBV3	2846	1616	0.08%	0.011%
57	10.688	2981	2985	2987	rBV4	1491	1268	0.06%	0.009%
58	10.775	3009	3012	3014	rBV4	2120	1157	0.06%	0.008%
59	11.016	3085	3087	3091	rVB5	1548	931	0.05%	0.006%
60	11.042	3093	3095	3097	rVB3	1599	592	0.03%	0.004%
61	11.058	3097	3100	3104	rVB6	1640	1082	0.06%	0.007%
62	11.080	3104	3107	3108	rBV3	1926	1082	0.06%	0.007%
63	11.148	3126	3128	3130	rBV3	1417	861	0.04%	0.006%
64	11.273	3155	3167	3187	rBV	1162258	1812287	92.35%	12.290%
65	11.466	3220	3227	3229	rBV8	2678	2871	0.15%	0.019%
66	11.649	3272	3284	3299	rBV	791011	1230643	62.71%	8.346%
67	11.791	3326	3328	3331	rBV3	1806	963	0.05%	0.007%
68	11.823	3336	3338	3341	rVB3	3164	1568	0.08%	0.011%
69	11.855	3343	3348	3349	rBV5	1580	1384	0.07%	0.009%
70	11.868	3349	3352	3355	rBV5	2224	1415	0.07%	0.010%
71	11.990	3388	3390	3392	rBV4	1254	636	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015221.D
 Acq On : 28 Mar 2020 03:32
 Operator : SY/MD
 Sample : L2005-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DN1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

72	12.009	3392	3396	3400	rVV7	2050	2203	0.11%	0.015%
73	12.061	3409	3412	3415	rBV5	2702	1593	0.08%	0.011%
74	12.093	3418	3422	3425	rBV6	2756	2449	0.12%	0.017%
75	12.148	3436	3439	3441	rBV4	1626	1227	0.06%	0.008%
76	12.225	3462	3463	3466	rBV3	1399	796	0.04%	0.005%
77	12.328	3490	3495	3496	rBV5	1536	1368	0.07%	0.009%
78	12.476	3539	3541	3543	rBV3	1714	1049	0.05%	0.007%
79	12.517	3551	3554	3556	rBV4	1821	1041	0.05%	0.007%
80	12.543	3559	3562	3564	rBV4	1169	813	0.04%	0.006%
81	12.595	3572	3578	3580	rBV6	1812	1827	0.09%	0.012%
82	12.669	3593	3601	3602	rBV7	7164	6887	0.35%	0.047%
83	12.749	3625	3626	3628	rBV2	1471	719	0.04%	0.005%
84	12.833	3648	3652	3657	rBV8	1941	2597	0.13%	0.018%
85	12.958	3688	3691	3694	rBV4	1595	965	0.05%	0.007%
86	13.025	3708	3712	3717	rVB7	2703	2054	0.10%	0.014%
87	13.115	3738	3740	3743	rVB4	2021	1005	0.05%	0.007%
88	13.132	3743	3745	3748	rBV3	1150	818	0.04%	0.006%
89	13.260	3783	3785	3786	rBV2	1313	747	0.04%	0.005%
90	13.289	3788	3794	3805	rVV2	7347	12863	0.66%	0.087%
91	13.421	3828	3835	3846	rBV2	7639	14216	0.72%	0.096%
92	13.607	3890	3893	3898	rBV6	1581	1598	0.08%	0.011%
93	13.662	3907	3910	3913	rBV4	1765	1284	0.07%	0.009%
94	13.894	3979	3982	3984	rBV4	2460	1232	0.06%	0.008%
95	14.096	4042	4045	4046	rBV3	1800	1126	0.06%	0.008%
96	14.173	4063	4069	4072	rBV8	2578	3358	0.17%	0.023%
97	14.296	4104	4107	4109	rBV4	2520	1752	0.09%	0.012%
98	14.350	4123	4124	4128	rBV4	1603	842	0.04%	0.006%
99	14.479	4162	4164	4166	rBV3	2075	1256	0.06%	0.009%
100	14.556	4185	4188	4190	rBV3	1724	1168	0.06%	0.008%


Sum of corrected areas: 14745566

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032720\
Data File : VV015221.D
Acq On : 28 Mar 2020 03:32
Operator : SY/MD
Sample : L2005-09
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DN1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

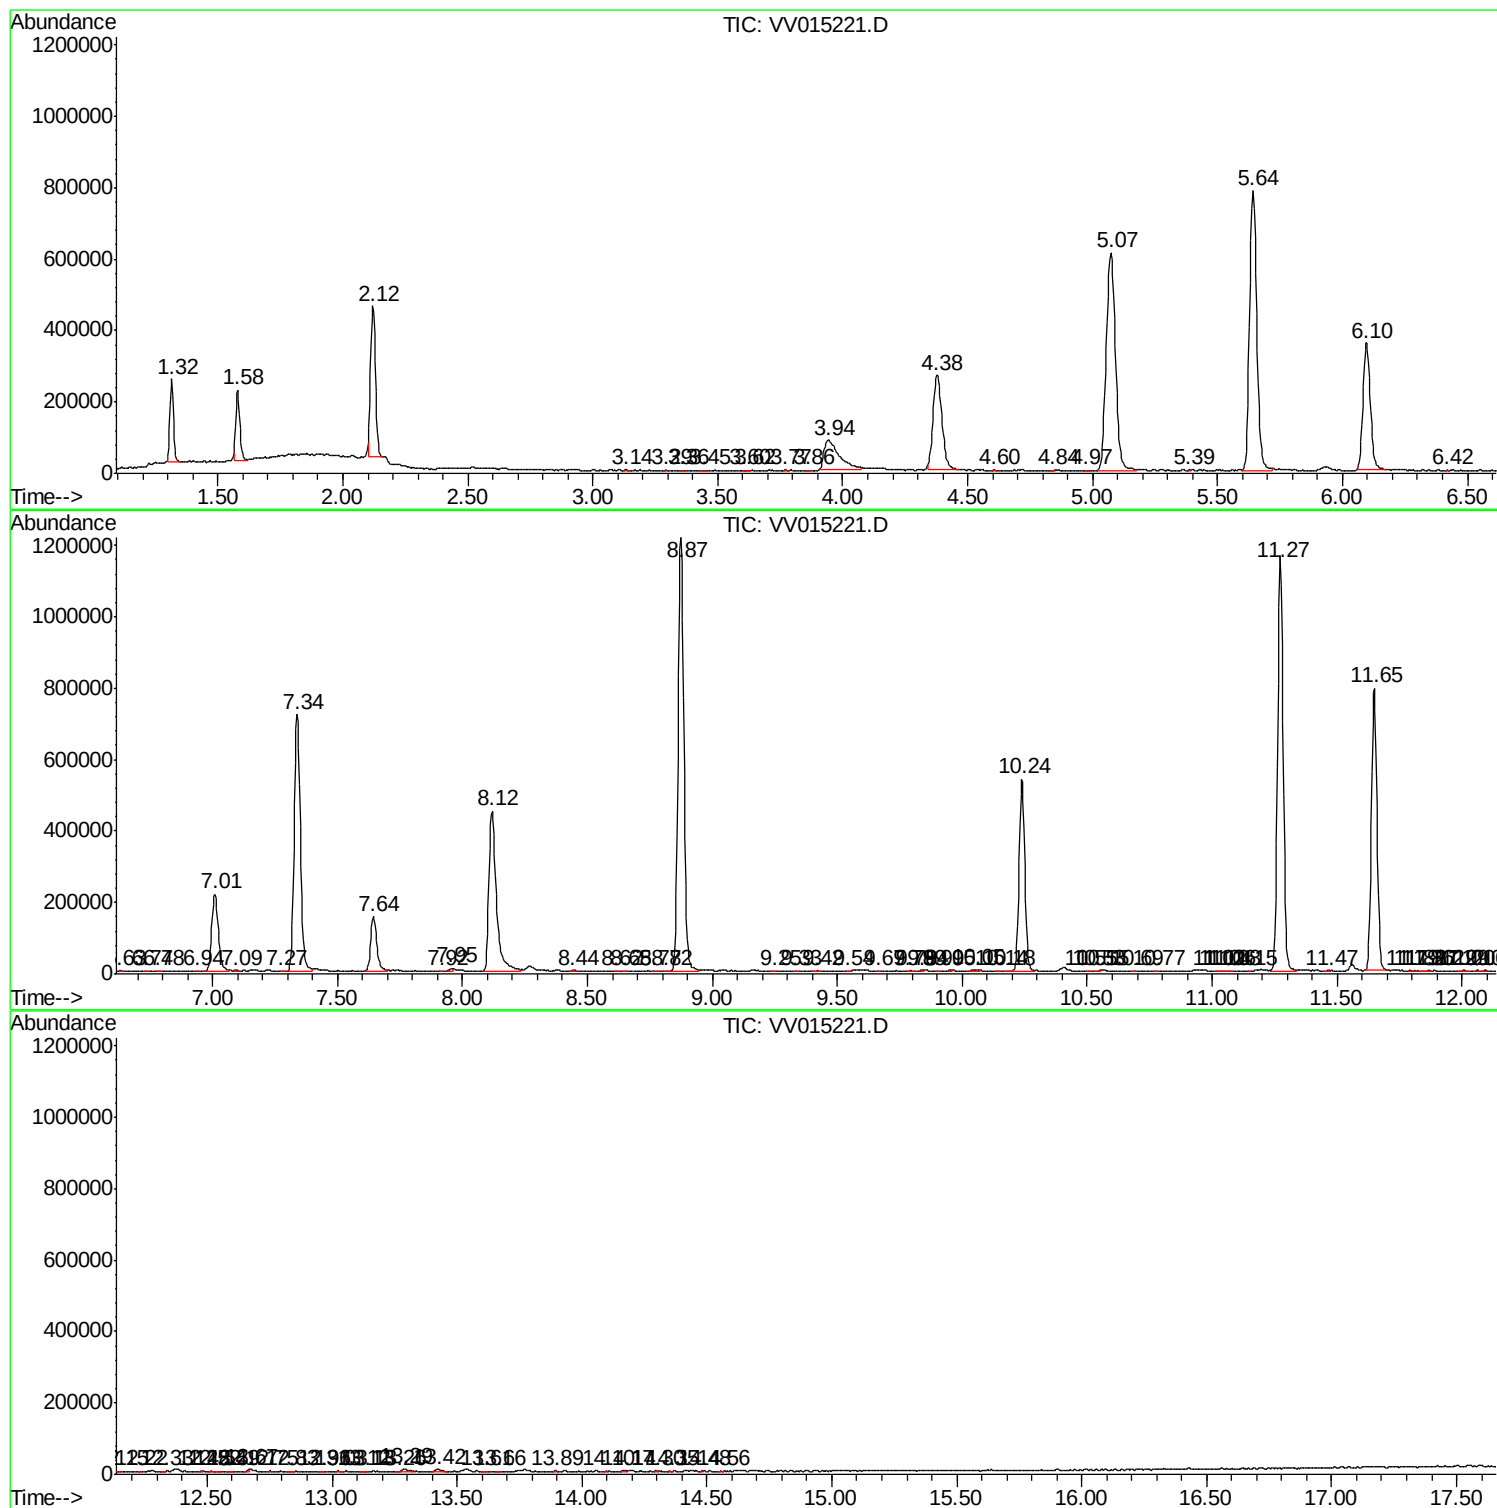

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032720\
Data File : VV015221.D
Acq On : 28 Mar 2020 03:32
Operator : SY/MD
Sample : L2005-09
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0DN1

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032720\
Data File : VV015221.D
Acq On : 28 Mar 2020 03:32
Operator : SY/MD
Sample : L2005-09
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0DN1

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
