

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015223.D
 Acq On : 28 Mar 2020 04:20
 Operator : SY/MD
 Sample : L1985-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTL5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	64	69	83	rVB	220620	228761	11.98%	1.556%
2	1.576	146	151	162	rVB	198380	230223	12.05%	1.566%
3	2.119	313	320	337	rVB	436880	660461	34.58%	4.493%
4	3.042	605	607	612	rBV6	2533	2573	0.13%	0.018%
5	3.145	635	639	644	rVB7	2493	2564	0.13%	0.017%
6	3.393	713	716	720	rBV5	2110	1610	0.08%	0.011%
7	3.457	731	736	738	rBV4	2988	2439	0.13%	0.017%
8	3.512	751	753	755	rBV3	1682	804	0.04%	0.005%
9	3.608	781	783	786	rBV4	1698	960	0.05%	0.007%
10	3.692	806	809	813	rBV4	2148	1662	0.09%	0.011%
11	3.762	829	831	833	rVB3	1910	831	0.04%	0.006%
12	3.778	833	836	838	rBV4	1704	1156	0.06%	0.008%
13	3.875	864	866	869	rBV3	1452	1046	0.05%	0.007%
14	3.939	874	886	909	rBV	87909	364282	19.07%	2.478%
15	4.376	1009	1022	1044	rVB	264367	645842	33.81%	4.393%
16	4.846	1166	1168	1171	rVV3	1611	1149	0.06%	0.008%
17	4.904	1184	1186	1188	rBV3	1252	804	0.04%	0.005%
18	4.962	1201	1204	1206	rVV4	1468	1043	0.05%	0.007%
19	5.071	1223	1238	1264	rBV2	615193	1522127	79.69%	10.354%
20	5.640	1402	1415	1444	rBV	771794	1550063	81.16%	10.544%
21	5.820	1466	1471	1473	rBV6	2220	1751	0.09%	0.012%
22	6.039	1537	1539	1542	rBV3	1160	946	0.05%	0.006%
23	6.093	1543	1556	1579	rVV2	365226	742704	38.89%	5.052%
24	6.364	1638	1640	1646	rVB7	2617	2457	0.13%	0.017%
25	6.434	1659	1662	1664	rBV3	1893	1120	0.06%	0.008%
26	6.743	1756	1758	1764	rVB7	2098	1504	0.08%	0.010%
27	6.836	1783	1787	1789	rBV5	1557	1215	0.06%	0.008%
28	6.942	1818	1820	1823	rVV3	1576	836	0.04%	0.006%
29	7.010	1830	1841	1860	rBV	213423	387375	20.28%	2.635%
30	7.187	1890	1896	1898	rBV7	2380	1968	0.10%	0.013%
31	7.264	1912	1920	1931	rBV3	10891	19517	1.02%	0.133%
32	7.338	1931	1943	1960	rBV	701219	1216971	63.72%	8.279%
33	7.643	2024	2038	2054	rBV	149704	262229	13.73%	1.784%
34	7.830	2094	2096	2097	rBV2	1819	825	0.04%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015223.D
 Acq On : 28 Mar 2020 04:20
 Operator : SY/MD
 Sample : L1985-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTL5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

35	7.872	2107	2109	2116	rVB7	2950	1993	0.10%	0.014%
36	7.900	2116	2118	2121	rBV4	1627	1280	0.07%	0.009%
37	8.045	2159	2163	2167	rVB6	2414	1708	0.09%	0.012%
38	8.116	2175	2185	2216	rBV3	447767	932719	48.83%	6.345%
39	8.595	2331	2334	2337	rBV4	2201	1231	0.06%	0.008%
40	8.823	2401	2405	2408	rBV6	2188	1494	0.08%	0.010%
41	8.875	2408	2421	2448	rBV	1176100	1909985	100.00%	12.993%
42	9.370	2573	2575	2578	rVB3	2113	1088	0.06%	0.007%
43	9.460	2600	2603	2604	rBV3	1404	830	0.04%	0.006%
44	9.624	2652	2654	2657	rBV3	1796	1286	0.07%	0.009%
45	9.704	2675	2679	2681	rBV5	2122	1571	0.08%	0.011%
46	9.752	2689	2694	2702	rBV5	2631	3597	0.19%	0.024%
47	9.904	2738	2741	2747	rBV8	2138	2538	0.13%	0.017%
48	10.238	2831	2845	2861	rBV	535450	857039	44.87%	5.830%
49	10.396	2889	2894	2895	rBV5	4002	3068	0.16%	0.021%
50	10.473	2915	2918	2920	rVV4	1662	991	0.05%	0.007%
51	10.521	2930	2933	2936	rBV5	2268	1857	0.10%	0.013%
52	10.540	2936	2939	2942	rVV4	2531	2121	0.11%	0.014%
53	10.559	2942	2945	2953	rVB9	3429	4544	0.24%	0.031%
54	10.630	2959	2967	2969	rBV9	1813	2348	0.12%	0.016%
55	10.762	3005	3008	3010	rBV4	2097	1442	0.08%	0.010%
56	10.987	3074	3078	3081	rVB6	2395	1760	0.09%	0.012%
57	11.035	3089	3093	3096	rBV6	1462	1352	0.07%	0.009%
58	11.119	3117	3119	3124	rVB5	2003	1455	0.08%	0.010%
59	11.141	3124	3126	3130	rVB5	2200	1008	0.05%	0.007%
60	11.183	3132	3139	3142	rBV8	4043	5101	0.27%	0.035%
61	11.273	3155	3167	3185	rBV	1123409	1745133	91.37%	11.871%
62	11.518	3240	3243	3246	rBV5	2197	1480	0.08%	0.010%
63	11.559	3246	3256	3270	rVV2	30470	57005	2.98%	0.388%
64	11.649	3272	3284	3302	rVV	786501	1220735	63.91%	8.304%
65	11.897	3356	3361	3364	rBV7	2690	3175	0.17%	0.022%
66	12.013	3393	3397	3398	rBV4	2479	1894	0.10%	0.013%
67	12.100	3420	3424	3427	rVB6	2048	1505	0.08%	0.010%
68	12.138	3433	3436	3441	rBV6	2477	2106	0.11%	0.014%
69	12.190	3450	3452	3458	rVB7	1646	1426	0.07%	0.010%
70	12.270	3472	3477	3483	rBV10	3225	3906	0.20%	0.027%
71	12.440	3528	3530	3532	rBV3	1770	981	0.05%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015223.D
 Acq On : 28 Mar 2020 04:20
 Operator : SY/MD
 Sample : L1985-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTL5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

72	12.527	3554	3557	3559	rBV4	1791	995	0.05%	0.007%
73	12.553	3562	3565	3567	rBV4	1713	1230	0.06%	0.008%
74	12.649	3592	3595	3597	rBV3	2820	1915	0.10%	0.013%
75	12.704	3607	3612	3615	rBV7	2530	2252	0.12%	0.015%
76	12.804	3639	3643	3647	rVB7	2020	1555	0.08%	0.011%
77	12.894	3667	3671	3673	rBV5	1567	1173	0.06%	0.008%
78	13.006	3703	3706	3707	rBV3	1460	956	0.05%	0.007%
79	13.074	3724	3727	3729	rBV3	2181	1357	0.07%	0.009%
80	13.167	3753	3756	3762	rVB7	2228	1993	0.10%	0.014%
81	13.273	3786	3789	3790	rBV3	2106	1195	0.06%	0.008%
82	13.347	3809	3812	3817	rVB7	1773	1537	0.08%	0.010%
83	13.373	3817	3820	3824	rBV6	1269	1101	0.06%	0.007%
84	13.392	3824	3826	3830	rVV5	2134	1463	0.08%	0.010%
85	13.431	3836	3838	3842	rBV4	1342	1003	0.05%	0.007%
86	13.482	3852	3854	3859	rVB5	2061	1843	0.10%	0.013%
87	13.534	3859	3870	3878	rBV5	6779	14441	0.76%	0.098%
88	13.611	3890	3894	3896	rBV4	2166	1759	0.09%	0.012%
89	13.829	3960	3962	3965	rBV5	1287	831	0.04%	0.006%
90	13.865	3968	3973	3975	rBV5	2080	1676	0.09%	0.011%
91	13.932	3991	3994	3995	rBV3	1700	845	0.04%	0.006%
92	13.987	4007	4011	4014	rBV6	1699	1444	0.08%	0.010%
93	14.148	4058	4061	4062	rBV3	1442	888	0.05%	0.006%
94	14.415	4141	4144	4145	rBV3	2004	1162	0.06%	0.008%
95	14.466	4157	4160	4165	rBV6	2537	2211	0.12%	0.015%
96	14.492	4165	4168	4169	rBV4	1700	826	0.04%	0.006%
97	14.569	4190	4192	4197	rVB5	2579	1652	0.09%	0.011%
98	14.598	4198	4201	4204	rVV5	2227	1580	0.08%	0.011%
99	14.743	4244	4246	4250	rBV4	2607	1808	0.09%	0.012%
100	14.839	4273	4276	4277	rBV3	1842	1117	0.06%	0.008%


Sum of corrected areas: 14700378

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032720\
Data File : VV015223.D
Acq On : 28 Mar 2020 04:20
Operator : SY/MD
Sample : L1985-01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTL5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

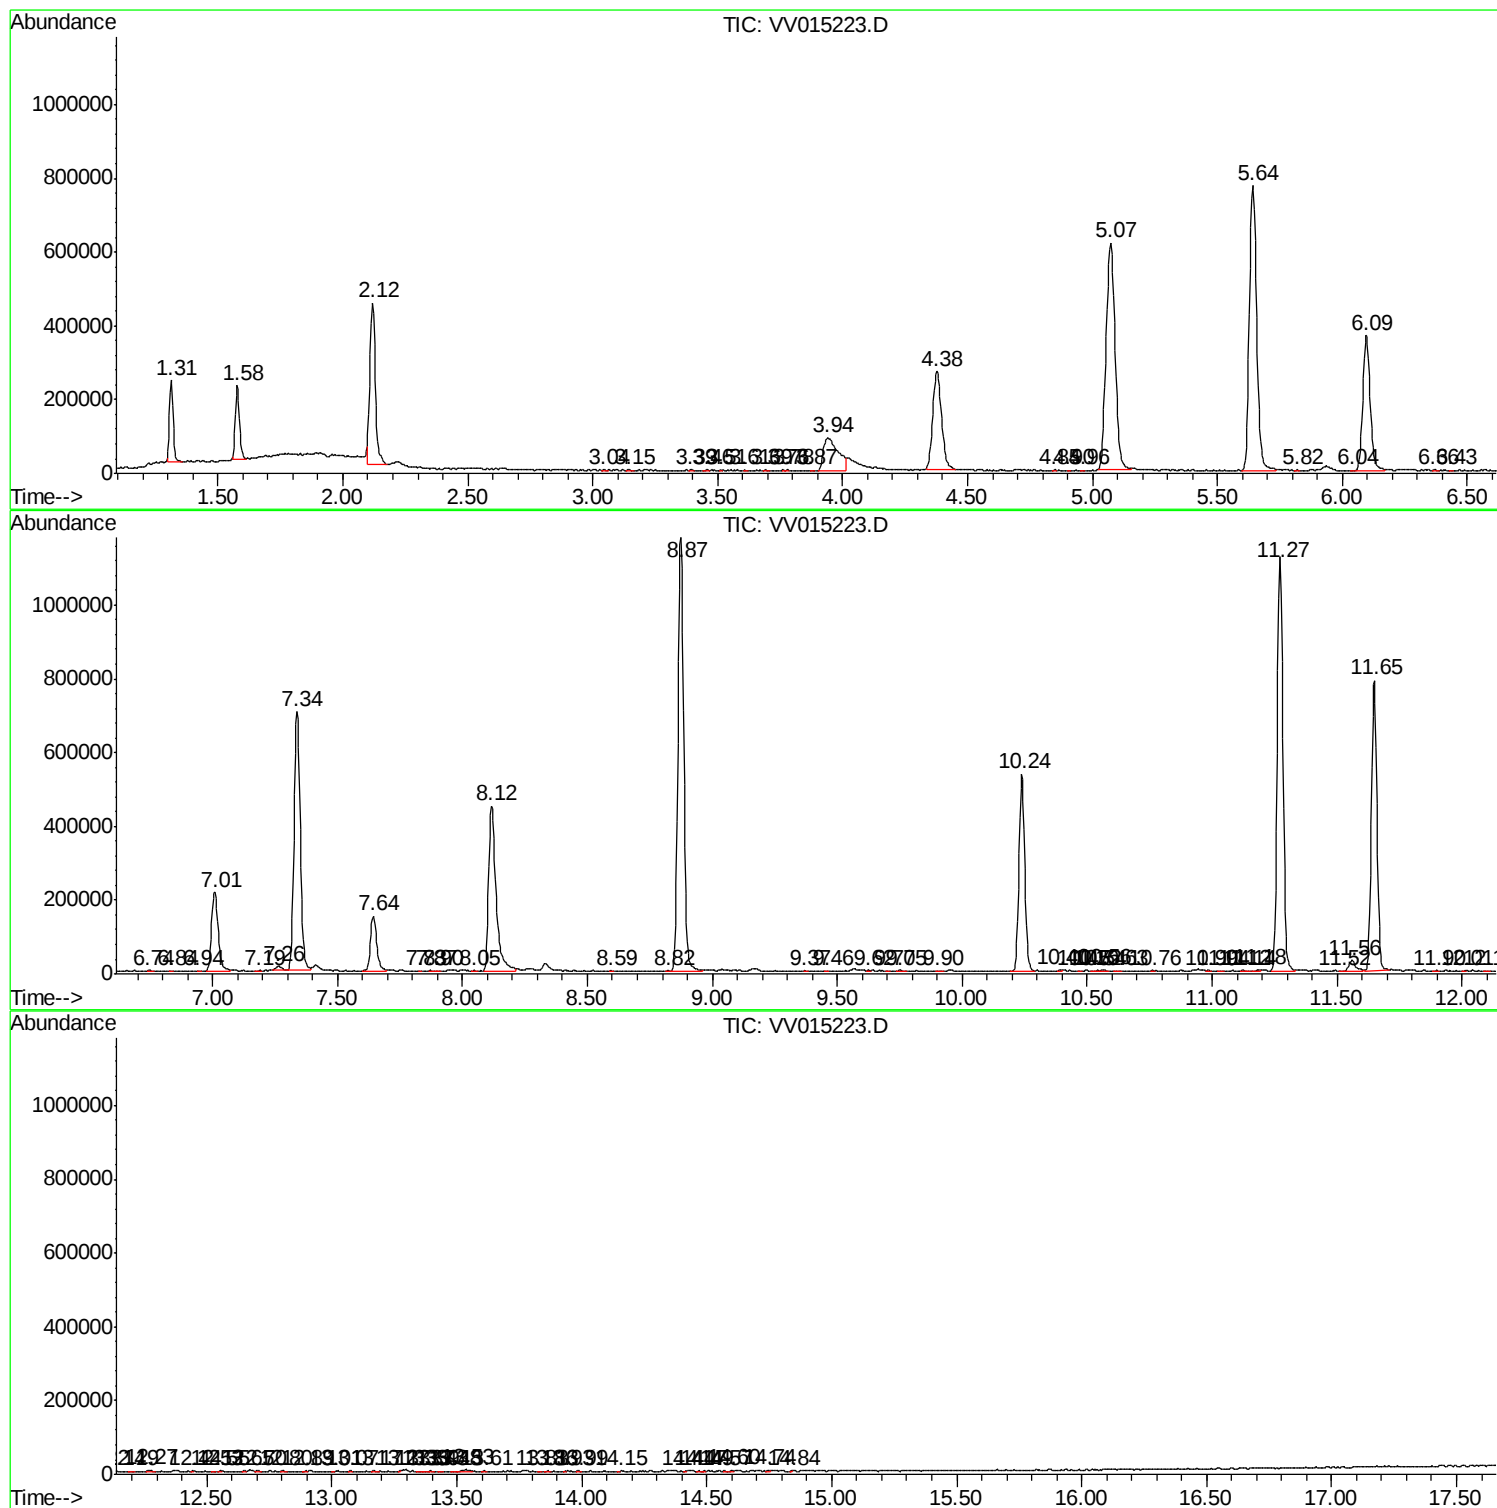

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV032720\
Data File : VV015223.D
Acq On : 28 Mar 2020 04:20
Operator : SY/MD
Sample : L1985-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTL5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032720\
Data File : VV015223.D
Acq On : 28 Mar 2020 04:20
Operator : SY/MD
Sample : L1985-01
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
ETTL5

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc