

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015227.D
 Acq On : 28 Mar 2020 05:57
 Operator : SY/MD
 Sample : L2003-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EK4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	81	rVB	246320	244487	10.40%	1.443%
2	1.579	146	152	167	rVB	211161	246822	10.50%	1.456%
3	2.119	313	320	331	rVB	438481	617221	26.27%	3.642%
4	3.363	705	707	710	rVB4	1336	501	0.02%	0.003%
5	3.383	710	713	717	rBV6	1506	1248	0.05%	0.007%
6	3.444	730	732	733	rBV	1564	608	0.03%	0.004%
7	3.521	754	756	758	rBV3	1927	1057	0.04%	0.006%
8	3.537	759	761	765	rVB5	3087	2260	0.10%	0.013%
9	3.605	778	782	783	rBV4	1214	780	0.03%	0.005%
10	3.675	798	804	805	rBV4	3065	2422	0.10%	0.014%
11	3.756	827	829	832	rBV3	2027	1277	0.05%	0.008%
12	3.814	845	847	850	rBV4	1854	1320	0.06%	0.008%
13	3.949	875	889	935	rBV3	96296	554321	23.59%	3.271%
14	4.376	1009	1022	1048	rVB	275571	694482	29.55%	4.098%
15	4.685	1114	1118	1120	rBV5	2732	2306	0.10%	0.014%
16	4.833	1162	1164	1166	rBV2	1672	829	0.04%	0.005%
17	5.074	1223	1239	1273	rVB2	653358	1655407	70.45%	9.767%
18	5.408	1340	1343	1345	rBV4	1730	1244	0.05%	0.007%
19	5.643	1400	1416	1437	rBV	758198	1516605	64.54%	8.948%
20	6.096	1544	1557	1579	rBV	385492	775977	33.02%	4.578%
21	6.379	1641	1645	1647	rBV4	2155	1622	0.07%	0.010%
22	6.424	1656	1659	1660	rBV2	1575	861	0.04%	0.005%
23	6.614	1716	1718	1719	rBV2	2599	996	0.04%	0.006%
24	6.897	1802	1806	1807	rBV4	1841	1059	0.05%	0.006%
25	6.923	1812	1814	1818	rVB5	2607	1639	0.07%	0.010%
26	6.961	1821	1826	1828	rBV5	2558	2447	0.10%	0.014%
27	7.010	1831	1841	1860	rVB	222167	396156	16.86%	2.337%
28	7.338	1930	1943	1967	rBV	764347	1325351	56.40%	7.820%
29	7.572	2012	2016	2019	rBV5	3304	2897	0.12%	0.017%
30	7.643	2028	2038	2056	rBV	159536	273198	11.63%	1.612%
31	7.842	2097	2100	2103	rBV5	1936	1303	0.06%	0.008%
32	7.878	2108	2111	2112	rBV3	1717	812	0.03%	0.005%
33	7.936	2127	2129	2130	rBV2	1251	610	0.03%	0.004%
34	8.116	2171	2185	2217	rBV2	471030	989336	42.10%	5.837%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015227.D
 Acq On : 28 Mar 2020 05:57
 Operator : SY/MD
 Sample : L2003-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EK4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

35	8.440	2281	2286	2288	rBV6	2639	2077	0.09%	0.012%
36	8.611	2335	2339	2342	rVB3	1751	1356	0.06%	0.008%
37	8.653	2342	2352	2354	rBV9	2806	3919	0.17%	0.023%
38	8.755	2382	2384	2387	rBV3	2631	1733	0.07%	0.010%
39	8.772	2387	2389	2392	rVV4	1365	820	0.03%	0.005%
40	8.874	2409	2421	2451	rBV2	1183231	2349827	100.00%	13.865%
41	9.312	2555	2557	2559	rBV3	1578	883	0.04%	0.005%
42	9.473	2605	2607	2608	rBV2	1841	594	0.03%	0.004%
43	9.611	2648	2650	2653	rBV4	938	528	0.02%	0.003%
44	9.685	2671	2673	2674	rBV2	1515	734	0.03%	0.004%
45	9.727	2680	2686	2691	rVB7	2798	3086	0.13%	0.018%
46	9.755	2692	2695	2696	rBV3	1271	641	0.03%	0.004%
47	9.800	2706	2709	2711	rBV3	1894	1043	0.04%	0.006%
48	9.829	2713	2718	2722	rBV8	1865	1866	0.08%	0.011%
49	9.881	2730	2734	2735	rBV3	1065	662	0.03%	0.004%
50	9.929	2746	2749	2752	rBV5	882	659	0.03%	0.004%
51	9.945	2752	2754	2755	rBV2	832	256	0.01%	0.002%
52	10.013	2773	2775	2776	rBV2	1058	361	0.02%	0.002%
53	10.087	2795	2798	2800	rBV3	1864	1265	0.05%	0.007%
54	10.109	2803	2805	2806	rBV2	1382	496	0.02%	0.003%
55	10.238	2830	2845	2863	rBV	571860	901477	38.36%	5.319%
56	10.331	2873	2874	2878	rBV4	1411	574	0.02%	0.003%
57	10.399	2893	2895	2896	rBV2	2920	1323	0.06%	0.008%
58	10.472	2916	2918	2922	rVB4	2041	1189	0.05%	0.007%
59	10.604	2957	2959	2961	rBV3	1523	781	0.03%	0.005%
60	10.620	2961	2964	2965	rBV3	1584	898	0.04%	0.005%
61	10.730	2995	2998	3003	rBV6	2167	1928	0.08%	0.011%
62	10.845	3032	3034	3039	rBV6	1475	918	0.04%	0.005%
63	10.900	3049	3051	3052	rBV2	1079	416	0.02%	0.002%
64	11.032	3090	3092	3094	rBV3	1515	659	0.03%	0.004%
65	11.054	3094	3099	3101	rBV5	2146	2113	0.09%	0.012%
66	11.144	3125	3127	3130	rBV4	2687	1594	0.07%	0.009%
67	11.206	3140	3146	3155	rVB3	40460	58971	2.51%	0.348%
68	11.273	3156	3167	3190	rVB2	1167479	2241769	95.40%	13.227%
69	11.649	3273	3284	3311	rVB3	874433	1697911	72.26%	10.018%
70	11.926	3367	3370	3373	rBV4	1699	1039	0.04%	0.006%
71	12.003	3391	3394	3397	rVB4	3460	2225	0.09%	0.013%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015227.D
 Acq On : 28 Mar 2020 05:57
 Operator : SY/MD
 Sample : L2003-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EK4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

72	12.022	3397	3400	3402	rBV4	1714	1151	0.05%	0.007%
73	12.061	3410	3412	3414	rBV3	2644	1694	0.07%	0.010%
74	12.128	3430	3433	3435	rBV3	2301	1572	0.07%	0.009%
75	12.254	3467	3472	3473	rBV5	3185	1989	0.08%	0.012%
76	12.498	3546	3548	3550	rBV2	1494	747	0.03%	0.004%
77	12.530	3555	3558	3562	rBV5	2012	1434	0.06%	0.008%
78	12.595	3576	3578	3579	rBV2	1303	718	0.03%	0.004%
79	12.865	3659	3662	3665	rVB5	1620	1134	0.05%	0.007%
80	12.968	3690	3694	3696	rBV4	2041	1883	0.08%	0.011%
81	12.996	3701	3703	3708	rVV6	2168	1475	0.06%	0.009%
82	13.029	3711	3713	3717	rBV5	1536	916	0.04%	0.005%
83	13.241	3774	3779	3780	rBV5	2651	2315	0.10%	0.014%
84	13.286	3783	3793	3807	rVV	151599	243251	10.35%	1.435%
85	13.437	3836	3840	3843	rBV4	2050	1954	0.08%	0.012%
86	13.476	3850	3852	3855	rBV3	3096	1682	0.07%	0.010%
87	13.771	3937	3944	3958	rVB2	44138	71581	3.05%	0.422%
88	13.897	3981	3983	3987	rBV4	2212	1271	0.05%	0.007%
89	14.652	4216	4218	4221	rBV4	2415	1674	0.07%	0.010%
90	14.672	4221	4224	4227	rVV5	2578	2007	0.09%	0.012%


Sum of corrected areas: 16948500

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032720\
Data File : VV015227.D
Acq On : 28 Mar 2020 05:57
Operator : SY/MD
Sample : L2003-03
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EK4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

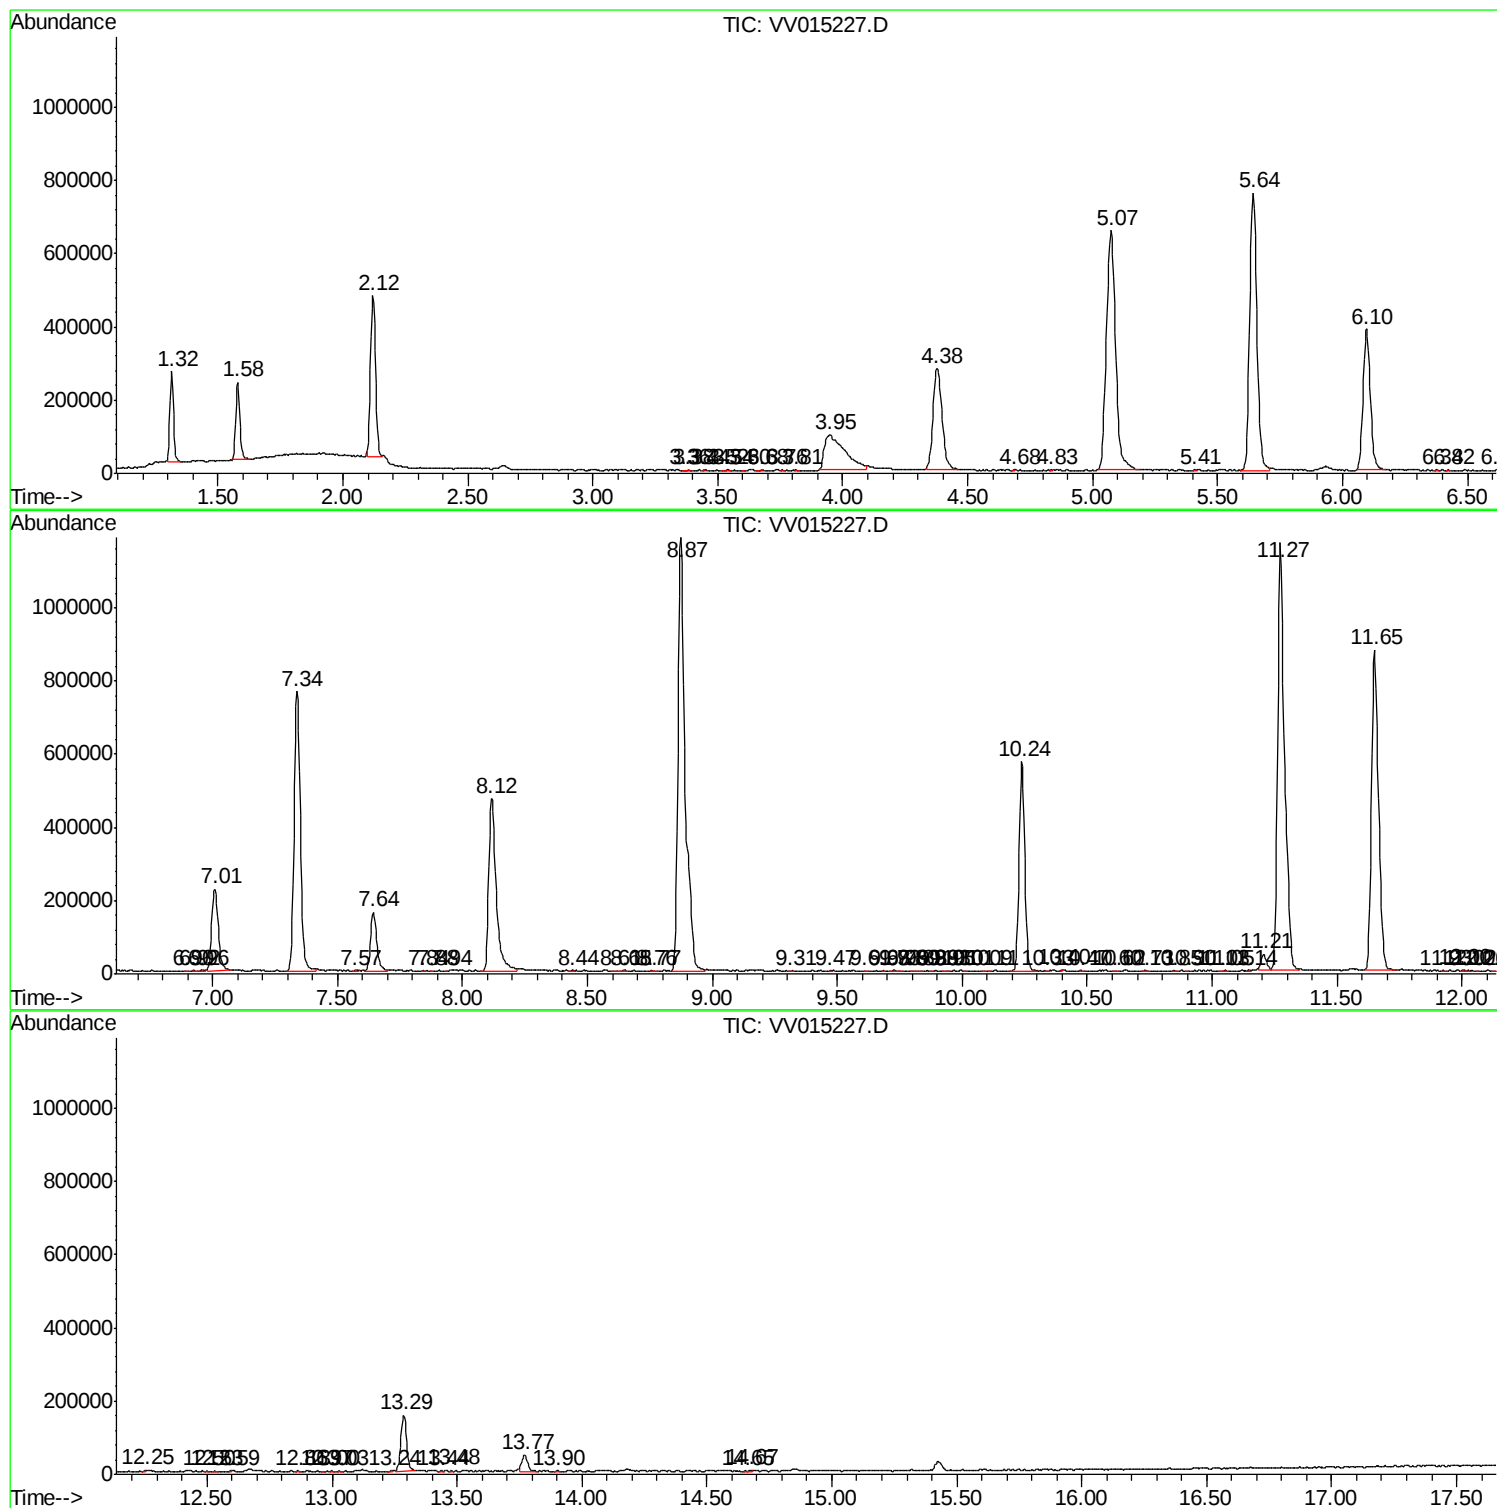

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV032720\
Data File : VV015227.D
Acq On : 28 Mar 2020 05:57
Operator : SY/MD
Sample : L2003-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EK4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV032720\
Data File : VV015227.D
Acq On : 28 Mar 2020 05:57
Operator : SY/MD
Sample : L2003-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EK4

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc