

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015228.D
 Acq On : 28 Mar 2020 06:21
 Operator : SY/MD
 Sample : L2003-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EK5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	65	70	77	rVB	233561	220636	10.42%	1.389%
2	1.579	147	152	165	rVB	211429	244921	11.57%	1.542%
3	2.119	313	320	331	rVB	443818	614943	29.04%	3.872%
4	3.158	641	643	645	rBV3	1988	1021	0.05%	0.006%
5	3.492	744	747	748	rBV3	2354	1312	0.06%	0.008%
6	3.598	774	780	782	rBV7	1396	1482	0.07%	0.009%
7	3.691	803	809	812	rBV8	2599	3210	0.15%	0.020%
8	3.708	812	814	815	rBV2	1339	497	0.02%	0.003%
9	3.753	825	828	831	rBV4	2351	1480	0.07%	0.009%
10	3.942	876	887	924	rBV3	94548	465135	21.97%	2.928%
11	4.380	1010	1023	1046	rVB	275375	685355	32.37%	4.315%
12	4.820	1158	1160	1163	rBV4	1568	943	0.04%	0.006%
13	5.074	1222	1239	1266	rBV2	652012	1651533	78.00%	10.398%
14	5.640	1401	1415	1441	rBV	756170	1525766	72.06%	9.606%
15	5.875	1485	1488	1490	rBV4	1969	1430	0.07%	0.009%
16	5.923	1496	1503	1505	rBV8	9295	10613	0.50%	0.067%
17	6.096	1543	1557	1583	rBV	386282	786036	37.12%	4.949%
18	6.341	1630	1633	1636	rBV4	2337	1758	0.08%	0.011%
19	6.695	1742	1743	1744	rBV	1371	496	0.02%	0.003%
20	6.801	1774	1776	1779	rBV3	1227	675	0.03%	0.004%
21	6.839	1785	1788	1790	rBV4	1331	946	0.04%	0.006%
22	6.887	1800	1803	1808	rBV6	2860	2455	0.12%	0.015%
23	6.965	1824	1827	1828	rBV3	1497	884	0.04%	0.006%
24	7.010	1830	1841	1861	rVV	219187	401729	18.97%	2.529%
25	7.244	1911	1914	1916	rBV4	1834	1053	0.05%	0.007%
26	7.257	1916	1918	1920	rBV3	1808	1194	0.06%	0.008%
27	7.277	1922	1924	1927	rBV4	1406	761	0.04%	0.005%
28	7.338	1931	1943	1961	rBV	750825	1295851	61.20%	8.159%
29	7.524	1997	2001	2003	rBV4	1597	1307	0.06%	0.008%
30	7.643	2029	2038	2059	rVB2	154701	261648	12.36%	1.647%
31	7.768	2075	2077	2081	rBV5	1148	729	0.03%	0.005%
32	7.810	2087	2090	2095	rVB7	1587	1275	0.06%	0.008%
33	7.855	2103	2104	2106	rBV2	1157	473	0.02%	0.003%
34	7.894	2113	2116	2123	rBV8	2009	2086	0.10%	0.013%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015228.D
 Acq On : 28 Mar 2020 06:21
 Operator : SY/MD
 Sample : L2003-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EK5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

35	8.029	2155	2158	2160	rBV4	1284	1042	0.05%	0.007%
36	8.116	2175	2185	2217	rBV2	461470	975316	46.06%	6.141%
37	8.485	2297	2300	2303	rBV5	2653	1821	0.09%	0.011%
38	8.556	2320	2322	2326	rVB5	1654	1079	0.05%	0.007%
39	8.585	2326	2331	2336	rBV8	2893	3246	0.15%	0.020%
40	8.688	2358	2363	2366	rBV6	1796	1939	0.09%	0.012%
41	8.794	2393	2396	2397	rBV3	1801	814	0.04%	0.005%
42	8.875	2409	2421	2446	rBV	1176183	2117290	100.00%	13.330%
43	9.296	2549	2552	2554	rBV4	1528	824	0.04%	0.005%
44	9.312	2554	2557	2560	rBV3	1855	1346	0.06%	0.008%
45	9.350	2566	2569	2571	rBV4	1037	735	0.03%	0.005%
46	9.624	2652	2654	2656	rBV3	1257	786	0.04%	0.005%
47	9.691	2672	2675	2676	rBV2	1449	657	0.03%	0.004%
48	9.701	2676	2678	2679	rVB2	1611	559	0.03%	0.004%
49	9.752	2692	2694	2696	rBV3	1927	1125	0.05%	0.007%
50	9.794	2704	2707	2709	rBV4	1567	833	0.04%	0.005%
51	9.804	2709	2710	2711	rBV	1001	245	0.01%	0.002%
52	9.862	2726	2728	2730	rBV3	1304	874	0.04%	0.006%
53	9.897	2736	2739	2744	rBV7	2861	3311	0.16%	0.021%
54	9.926	2746	2748	2752	rVB5	1575	1054	0.05%	0.007%
55	10.026	2775	2779	2780	rBV4	1907	1231	0.06%	0.008%
56	10.048	2785	2786	2787	rBV	917	266	0.01%	0.002%
57	10.161	2820	2821	2825	rVB4	1944	1036	0.05%	0.007%
58	10.180	2825	2827	2830	rVB3	1766	1003	0.05%	0.006%
59	10.238	2833	2845	2866	rBV	572350	897468	42.39%	5.650%
60	10.386	2889	2891	2892	rBV2	2166	883	0.04%	0.006%
61	10.489	2920	2923	2928	rBV6	2014	1514	0.07%	0.010%
62	10.559	2943	2945	2947	rBV3	2058	1026	0.05%	0.006%
63	10.646	2968	2972	2974	rBV5	2657	1965	0.09%	0.012%
64	10.826	3027	3028	3030	rBV2	1222	566	0.03%	0.004%
65	11.055	3096	3099	3103	rBV5	1753	1202	0.06%	0.008%
66	11.074	3103	3105	3108	rBV4	1740	1040	0.05%	0.007%
67	11.209	3140	3147	3156	rVB4	22254	31718	1.50%	0.200%
68	11.273	3156	3167	3186	rBV2	1118441	1979234	93.48%	12.461%
69	11.649	3272	3284	3307	rBV2	857868	1504196	71.04%	9.470%
70	11.984	3385	3388	3390	rBV4	1943	1076	0.05%	0.007%
71	12.103	3423	3425	3427	rVB3	1472	511	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015228.D
 Acq On : 28 Mar 2020 06:21
 Operator : SY/MD
 Sample : L2003-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EK5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

72	12.119	3427	3430	3432	rBV4	2061	1127	0.05%	0.007%
73	12.196	3452	3454	3456	rVB3	2912	1096	0.05%	0.007%
74	12.231	3462	3465	3467	rBV4	1222	721	0.03%	0.005%
75	12.241	3467	3468	3471	rVV3	1161	617	0.03%	0.004%
76	12.537	3558	3560	3561	rBV2	1623	538	0.03%	0.003%
77	12.746	3623	3625	3626	rBV2	1205	433	0.02%	0.003%
78	12.826	3647	3650	3651	rBV3	1171	811	0.04%	0.005%
79	12.858	3655	3660	3662	rBV5	1856	1735	0.08%	0.011%
80	12.907	3672	3675	3679	rBV6	2670	2131	0.10%	0.013%
81	13.003	3703	3705	3708	rVB4	1879	844	0.04%	0.005%
82	13.170	3753	3757	3760	rBV5	1992	1961	0.09%	0.012%
83	13.215	3767	3771	3774	rBV4	2587	1961	0.09%	0.012%
84	13.286	3784	3793	3805	rBV3	82611	129994	6.14%	0.818%
85	13.411	3830	3832	3836	rBV5	1464	874	0.04%	0.006%
86	13.495	3855	3858	3861	rVB5	2276	1357	0.06%	0.009%
87	13.514	3861	3864	3865	rBV3	1602	849	0.04%	0.005%
88	13.890	3980	3981	3985	rBV4	1427	818	0.04%	0.005%
89	14.151	4060	4062	4064	rBV3	2110	1015	0.05%	0.006%
90	14.553	4184	4187	4190	rBV4	3318	1714	0.08%	0.011%


Sum of corrected areas: 15883060

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032720\
Data File : VV015228.D
Acq On : 28 Mar 2020 06:21
Operator : SY/MD
Sample : L2003-04
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EK5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

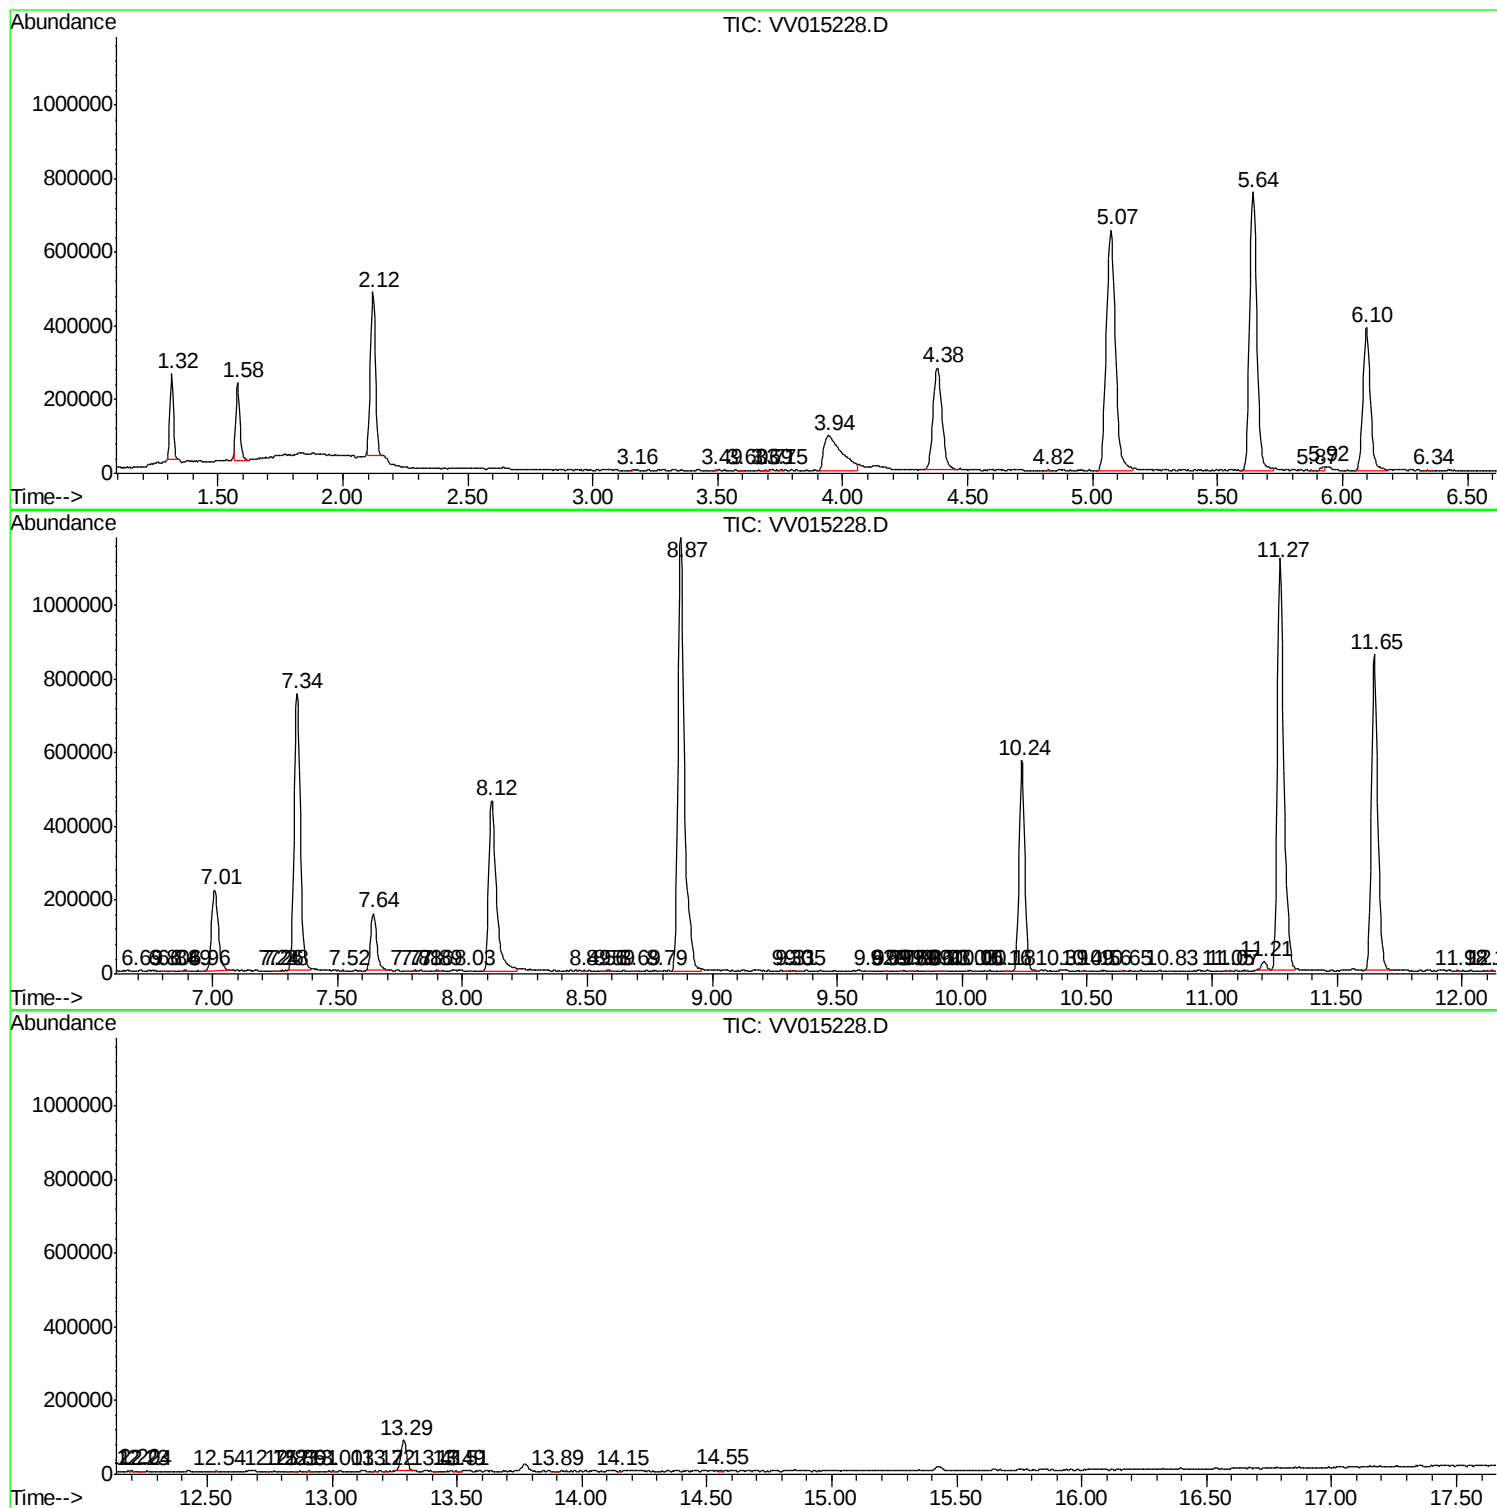

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV032720\
Data File : VV015228.D
Acq On : 28 Mar 2020 06:21
Operator : SY/MD
Sample : L2003-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EK5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032720\
Data File : VV015228.D
Acq On : 28 Mar 2020 06:21
Operator : SY/MD
Sample : L2003-04
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0EK5

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc