

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015230.D
 Acq On : 28 Mar 2020 07:10
 Operator : SY/MD
 Sample : L1976-19
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTK4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	64	69	80	rVB	243986	238429	11.88%	1.553%
2	1.576	146	151	164	rVB	206638	238653	11.89%	1.554%
3	2.119	313	320	343	rVB	439455	688667	34.30%	4.485%
4	3.332	695	697	698	rBV2	1250	413	0.02%	0.003%
5	3.470	738	740	742	rBV3	1381	839	0.04%	0.005%
6	3.936	872	885	921	rBV	98571	404639	20.15%	2.635%
7	4.376	1010	1022	1047	rVB	281600	688032	34.27%	4.480%
8	4.589	1085	1088	1092	rVB5	3562	2141	0.11%	0.014%
9	4.740	1133	1135	1137	rBV3	2315	1072	0.05%	0.007%
10	4.759	1137	1141	1144	rBV5	1034	839	0.04%	0.005%
11	4.778	1144	1147	1150	rBV5	2393	1651	0.08%	0.011%
12	4.833	1161	1164	1167	rBV5	3407	2531	0.13%	0.016%
13	4.923	1190	1192	1198	rVB7	2657	2064	0.10%	0.013%
14	4.952	1198	1201	1204	rBV4	1700	1569	0.08%	0.010%
15	5.071	1218	1238	1268	rBV2	644662	1647268	82.05%	10.727%
16	5.415	1341	1345	1347	rBV5	1285	1197	0.06%	0.008%
17	5.640	1403	1415	1434	rBV	769282	1507390	75.08%	9.816%
18	6.093	1540	1556	1581	rBV	387239	791352	39.42%	5.153%
19	6.360	1635	1639	1641	rBV4	3003	2279	0.11%	0.015%
20	6.396	1648	1650	1654	rBV4	1620	1094	0.05%	0.007%
21	6.531	1688	1692	1694	rBV5	1357	1310	0.07%	0.009%
22	6.653	1726	1730	1732	rBV4	2052	1597	0.08%	0.010%
23	6.814	1778	1780	1783	rVB4	2837	1600	0.08%	0.010%
24	6.830	1783	1785	1787	rBV3	1328	748	0.04%	0.005%
25	6.865	1795	1796	1798	rBV2	1168	538	0.03%	0.004%
26	7.007	1827	1840	1857	rBV	222034	405809	20.21%	2.643%
27	7.196	1896	1899	1902	rBV4	2595	2081	0.10%	0.014%
28	7.338	1931	1943	1965	rBV	738827	1286122	64.06%	8.375%
29	7.560	2009	2012	2014	rBV3	1996	1406	0.07%	0.009%
30	7.643	2028	2038	2059	rBV	158244	268868	13.39%	1.751%
31	7.814	2089	2091	2093	rBV3	1567	647	0.03%	0.004%
32	7.862	2104	2106	2108	rBV3	1473	760	0.04%	0.005%
33	8.116	2175	2185	2210	rBV2	451409	921974	45.92%	6.004%
34	8.441	2282	2286	2287	rBV4	1134	860	0.04%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015230.D
 Acq On : 28 Mar 2020 07:10
 Operator : SY/MD
 Sample : L1976-19
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTK4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

35	8.553	2318	2321	2323	rBV4	1608	1034	0.05%	0.007%
36	8.614	2338	2340	2344	rBV5	1430	1237	0.06%	0.008%
37	8.704	2366	2368	2371	rVB3	1337	813	0.04%	0.005%
38	8.720	2371	2373	2378	rBV6	2119	2314	0.12%	0.015%
39	8.875	2409	2421	2449	rBV	1151289	2007681	100.00%	13.074%
40	9.148	2502	2506	2508	rBV4	1582	1338	0.07%	0.009%
41	9.318	2556	2559	2562	rBV4	1543	1403	0.07%	0.009%
42	9.437	2594	2596	2597	rBV2	1490	427	0.02%	0.003%
43	9.466	2602	2605	2609	rBV5	1849	1489	0.07%	0.010%
44	9.511	2617	2619	2622	rBV4	1311	761	0.04%	0.005%
45	9.534	2622	2626	2628	rBV4	2245	1875	0.09%	0.012%
46	9.640	2656	2659	2663	rVB6	2451	1486	0.07%	0.010%
47	9.672	2667	2669	2670	rBV2	1154	398	0.02%	0.003%
48	9.717	2678	2683	2688	rVB7	2755	2665	0.13%	0.017%
49	9.743	2688	2691	2693	rBV4	971	566	0.03%	0.004%
50	9.785	2701	2704	2706	rBV4	2410	1458	0.07%	0.009%
51	9.810	2710	2712	2713	rBV2	1192	507	0.03%	0.003%
52	9.958	2756	2758	2763	rVB5	2770	1840	0.09%	0.012%
53	9.984	2763	2766	2767	rBV3	1273	700	0.03%	0.005%
54	10.048	2784	2786	2788	rBV3	1781	809	0.04%	0.005%
55	10.093	2798	2800	2802	rVB3	836	247	0.01%	0.002%
56	10.106	2802	2804	2808	rVB5	1998	1337	0.07%	0.009%
57	10.125	2808	2810	2812	rBV3	1278	671	0.03%	0.004%
58	10.180	2823	2827	2829	rBV4	1160	872	0.04%	0.006%
59	10.196	2829	2832	2833	rBV3	1428	694	0.03%	0.005%
60	10.238	2833	2845	2859	rBV	555532	879664	43.81%	5.728%
61	10.363	2882	2884	2886	rBV3	1558	746	0.04%	0.005%
62	10.463	2913	2915	2916	rBV2	1420	699	0.03%	0.005%
63	10.505	2924	2928	2931	rVB5	3039	2354	0.12%	0.015%
64	10.521	2931	2933	2936	rBV3	1325	878	0.04%	0.006%
65	10.550	2939	2942	2944	rBV4	1696	932	0.05%	0.006%
66	10.588	2950	2954	2956	rVB4	1595	1161	0.06%	0.008%
67	10.637	2967	2969	2971	rBV3	1123	520	0.03%	0.003%
68	10.669	2977	2979	2982	rVB3	2235	1086	0.05%	0.007%
69	10.704	2987	2990	2992	rBV3	1662	1112	0.06%	0.007%
70	10.752	3002	3005	3009	rBV5	1962	1359	0.07%	0.009%
71	10.772	3009	3011	3013	rBV3	1082	459	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015230.D
 Acq On : 28 Mar 2020 07:10
 Operator : SY/MD
 Sample : L1976-19
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTK4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

72	10.788	3013	3016	3021	rVB7	2334	1216	0.06%	0.008%
73	10.814	3021	3024	3025	rBV3	1242	720	0.04%	0.005%
74	10.862	3037	3039	3040	rBV2	1164	355	0.02%	0.002%
75	11.035	3091	3093	3095	rBV2	1206	743	0.04%	0.005%
76	11.068	3102	3103	3107	rVB4	1511	545	0.03%	0.004%
77	11.093	3107	3111	3112	rBV4	2361	1909	0.10%	0.012%
78	11.125	3118	3121	3124	rVB5	3647	2195	0.11%	0.014%
79	11.145	3124	3127	3128	rBV2	1528	778	0.04%	0.005%
80	11.209	3138	3147	3153	rBV4	12819	20325	1.01%	0.132%
81	11.273	3155	3167	3188	rVV	1127279	1851997	92.25%	12.060%
82	11.650	3273	3284	3303	rVB	810626	1348103	67.15%	8.779%
83	11.842	3341	3344	3349	rVB6	3617	2921	0.15%	0.019%
84	11.865	3349	3351	3352	rBV2	1373	522	0.03%	0.003%
85	11.939	3372	3374	3379	rBV5	1573	1427	0.07%	0.009%
86	11.965	3379	3382	3385	rBV5	1546	1106	0.06%	0.007%
87	12.077	3413	3417	3420	rVB5	1229	979	0.05%	0.006%
88	12.096	3420	3423	3425	rBV4	2248	1379	0.07%	0.009%
89	12.132	3431	3434	3440	rBV7	2800	2144	0.11%	0.014%
90	12.257	3465	3473	3476	rBV10	1471	2352	0.12%	0.015%
91	12.367	3503	3507	3508	rBV3	1356	853	0.04%	0.006%
92	12.508	3548	3551	3552	rBV3	1638	699	0.03%	0.005%
93	13.055	3718	3721	3724	rBV4	1889	1197	0.06%	0.008%
94	13.077	3725	3728	3729	rBV3	1834	889	0.04%	0.006%
95	13.289	3784	3794	3805	rBV2	39524	65569	3.27%	0.427%
96	13.354	3811	3814	3816	rVB3	2379	1170	0.06%	0.008%
97	14.042	4026	4028	4029	rBV2	1972	746	0.04%	0.005%
98	14.270	4095	4099	4100	rBV4	2405	1609	0.08%	0.010%


Sum of corrected areas: 15356479

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032720\
Data File : VV015230.D
Acq On : 28 Mar 2020 07:10
Operator : SY/MD
Sample : L1976-19
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTK4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

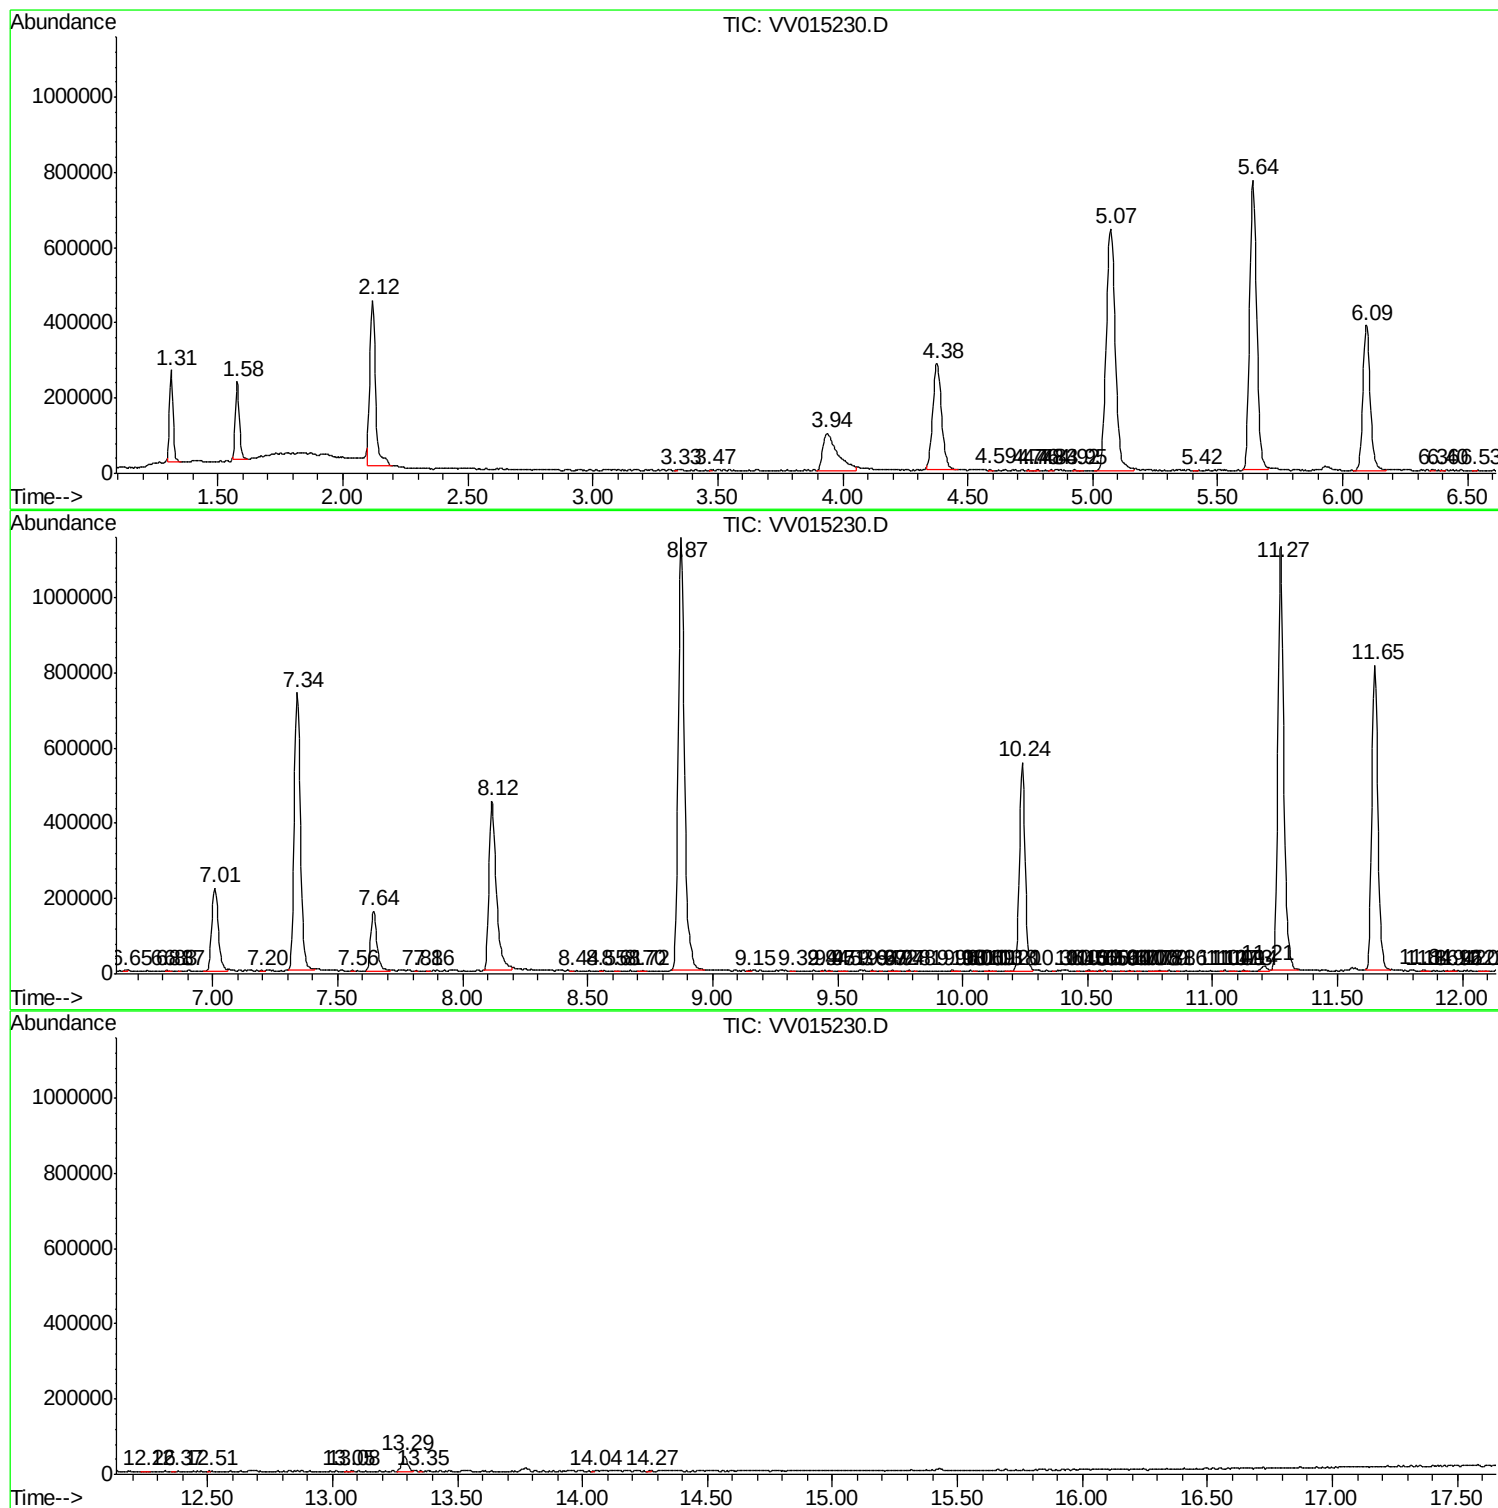

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV032720\
Data File : VV015230.D
Acq On : 28 Mar 2020 07:10
Operator : SY/MD
Sample : L1976-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTK4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032720\
Data File : VV015230.D
Acq On : 28 Mar 2020 07:10
Operator : SY/MD
Sample : L1976-19
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
ETTK4

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc