

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015232.D
 Acq On : 28 Mar 2020 07:58
 Operator : SY/MD
 Sample : L1976-21
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTK6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	64	69	78	rVB	218721	220248	2.79%	1.011%
2	2.119	314	320	330	rVB	374173	507078	6.43%	2.328%
3	3.267	674	677	685	rBV9	2590	3075	0.04%	0.014%
4	3.380	708	712	714	rBV3	2667	2299	0.03%	0.011%
5	3.605	778	782	784	rBV4	2241	1745	0.02%	0.008%
6	3.775	828	835	839	rVB8	3662	4189	0.05%	0.019%
7	3.936	870	885	921	rBV2	113688	442628	5.62%	2.032%
8	4.377	1009	1022	1045	rVB	260017	644652	8.18%	2.959%
9	4.766	1142	1143	1146	rBV3	1211	350	0.00%	0.002%
10	4.987	1209	1212	1214	rBV3	1222	741	0.01%	0.003%
11	5.071	1223	1238	1259	rBV3	597893	1502088	19.06%	6.895%
12	5.405	1338	1342	1345	rBV6	3360	2973	0.04%	0.014%
13	5.640	1400	1415	1442	rBV	702548	1412583	17.93%	6.485%
14	5.862	1478	1484	1485	rBV6	2035	2103	0.03%	0.010%
15	5.936	1491	1507	1535	rBV	4174618	7880252	100.00%	36.175%
16	6.093	1546	1556	1580	rVB	363569	722587	9.17%	3.317%
17	6.402	1649	1652	1654	rBV3	2076	1266	0.02%	0.006%
18	6.508	1683	1685	1686	rBV2	985	397	0.01%	0.002%
19	6.524	1686	1690	1692	rBV5	1895	1467	0.02%	0.007%
20	6.598	1709	1713	1714	rBV4	1890	1335	0.02%	0.006%
21	6.875	1795	1799	1802	rVB6	1477	1195	0.02%	0.005%
22	7.007	1830	1840	1855	rBV	205605	362079	4.59%	1.662%
23	7.338	1932	1943	1963	rBV	678045	1162462	14.75%	5.336%
24	7.643	2028	2038	2055	rBV	145628	251160	3.19%	1.153%
25	7.836	2096	2098	2099	rBV2	1355	443	0.01%	0.002%
26	8.000	2143	2149	2154	rBV9	4124	5134	0.07%	0.024%
27	8.116	2174	2185	2213	rBV	450029	909840	11.55%	4.177%
28	8.875	2406	2421	2444	rBV	1067090	1822447	23.13%	8.366%
29	9.473	2605	2607	2610	rBV4	1205	571	0.01%	0.003%
30	9.508	2615	2618	2625	rVB8	1910	1861	0.02%	0.009%
31	9.650	2659	2662	2665	rBV4	2301	1569	0.02%	0.007%
32	9.778	2699	2702	2705	rBV3	1291	735	0.01%	0.003%
33	9.798	2705	2708	2710	rVV3	1485	647	0.01%	0.003%
34	9.817	2710	2714	2716	rBV4	2123	1410	0.02%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015232.D
 Acq On : 28 Mar 2020 07:58
 Operator : SY/MD
 Sample : L1976-21
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTK6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

35	9.916	2744	2745	2748	rBV3	1086	657	0.01%	0.003%
36	10.048	2784	2786	2789	rBV3	1799	1023	0.01%	0.005%
37	10.061	2789	2790	2791	rBV	1534	519	0.01%	0.002%
38	10.087	2796	2798	2803	rVB5	1881	1365	0.02%	0.006%
39	10.190	2826	2830	2832	rBV5	1438	875	0.01%	0.004%
40	10.238	2832	2845	2863	rBV	542046	857168	10.88%	3.935%
41	10.431	2903	2905	2906	rBV	1358	580	0.01%	0.003%
42	10.502	2925	2927	2928	rBV2	1171	392	0.00%	0.002%
43	10.659	2974	2976	2979	rBV3	1710	1200	0.02%	0.006%
44	10.714	2991	2993	2997	rVB5	1991	1175	0.01%	0.005%
45	10.743	2997	3002	3006	rBV7	2153	2375	0.03%	0.011%
46	10.823	3024	3027	3029	rBV4	1279	938	0.01%	0.004%
47	11.016	3085	3087	3093	rBV6	2883	2236	0.03%	0.010%
48	11.077	3104	3106	3110	rBV3	2257	1832	0.02%	0.008%
49	11.093	3110	3111	3114	rVB3	1085	394	0.00%	0.002%
50	11.119	3114	3119	3121	rBV4	2287	2029	0.03%	0.009%
51	11.177	3131	3137	3138	rBV6	1983	2016	0.03%	0.009%
52	11.209	3138	3147	3155	rVV9	9601	18091	0.23%	0.083%
53	11.273	3155	3167	3188	rVV	1050368	1706673	21.66%	7.835%
54	11.650	3271	3284	3304	rBV	778507	1279622	16.24%	5.874%
55	11.990	3388	3390	3391	rBV2	1261	394	0.00%	0.002%
56	12.042	3403	3406	3409	rBV5	1693	968	0.01%	0.004%
57	12.058	3409	3411	3412	rBV2	1059	295	0.00%	0.001%
58	12.138	3432	3436	3441	rBV8	3140	3500	0.04%	0.016%
59	12.186	3449	3451	3452	rBV2	1714	794	0.01%	0.004%
60	12.325	3491	3494	3496	rBV3	1680	1126	0.01%	0.005%
61	12.534	3555	3559	3560	rBV4	1504	1054	0.01%	0.005%
62	12.579	3570	3573	3574	rBV3	2290	1304	0.02%	0.006%
63	12.662	3596	3599	3601	rBV4	3634	2806	0.04%	0.013%
64	12.727	3615	3619	3620	rBV4	2471	1683	0.02%	0.008%
65	12.949	3686	3688	3690	rBV3	2003	1286	0.02%	0.006%
66	13.100	3732	3735	3736	rBV3	1564	710	0.01%	0.003%
67	13.122	3736	3742	3744	rVV6	2019	2114	0.03%	0.010%
68	13.434	3837	3839	3840	rBV2	1438	733	0.01%	0.003%
69	14.103	4039	4047	4048	rBV6	3102	3792	0.05%	0.017%
70	14.421	4144	4146	4148	rBV3	1694	1011	0.01%	0.005%
71	14.469	4158	4161	4164	rBV4	1516	1163	0.01%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
Data File : VV015232.D
Acq On : 28 Mar 2020 07:58
Operator : SY/MD
Sample : L1976-21
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTK6

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Title : VOC Analysis

72	14.900	4291	4295	4297	rBV5	3079	2432	0.03%	0.011%
----	--------	------	------	------	------	------	------	-------	--------


Sum of corrected areas: 21783934

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032720\
Data File : VV015232.D
Acq On : 28 Mar 2020 07:58
Operator : SY/MD
Sample : L1976-21
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTK6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

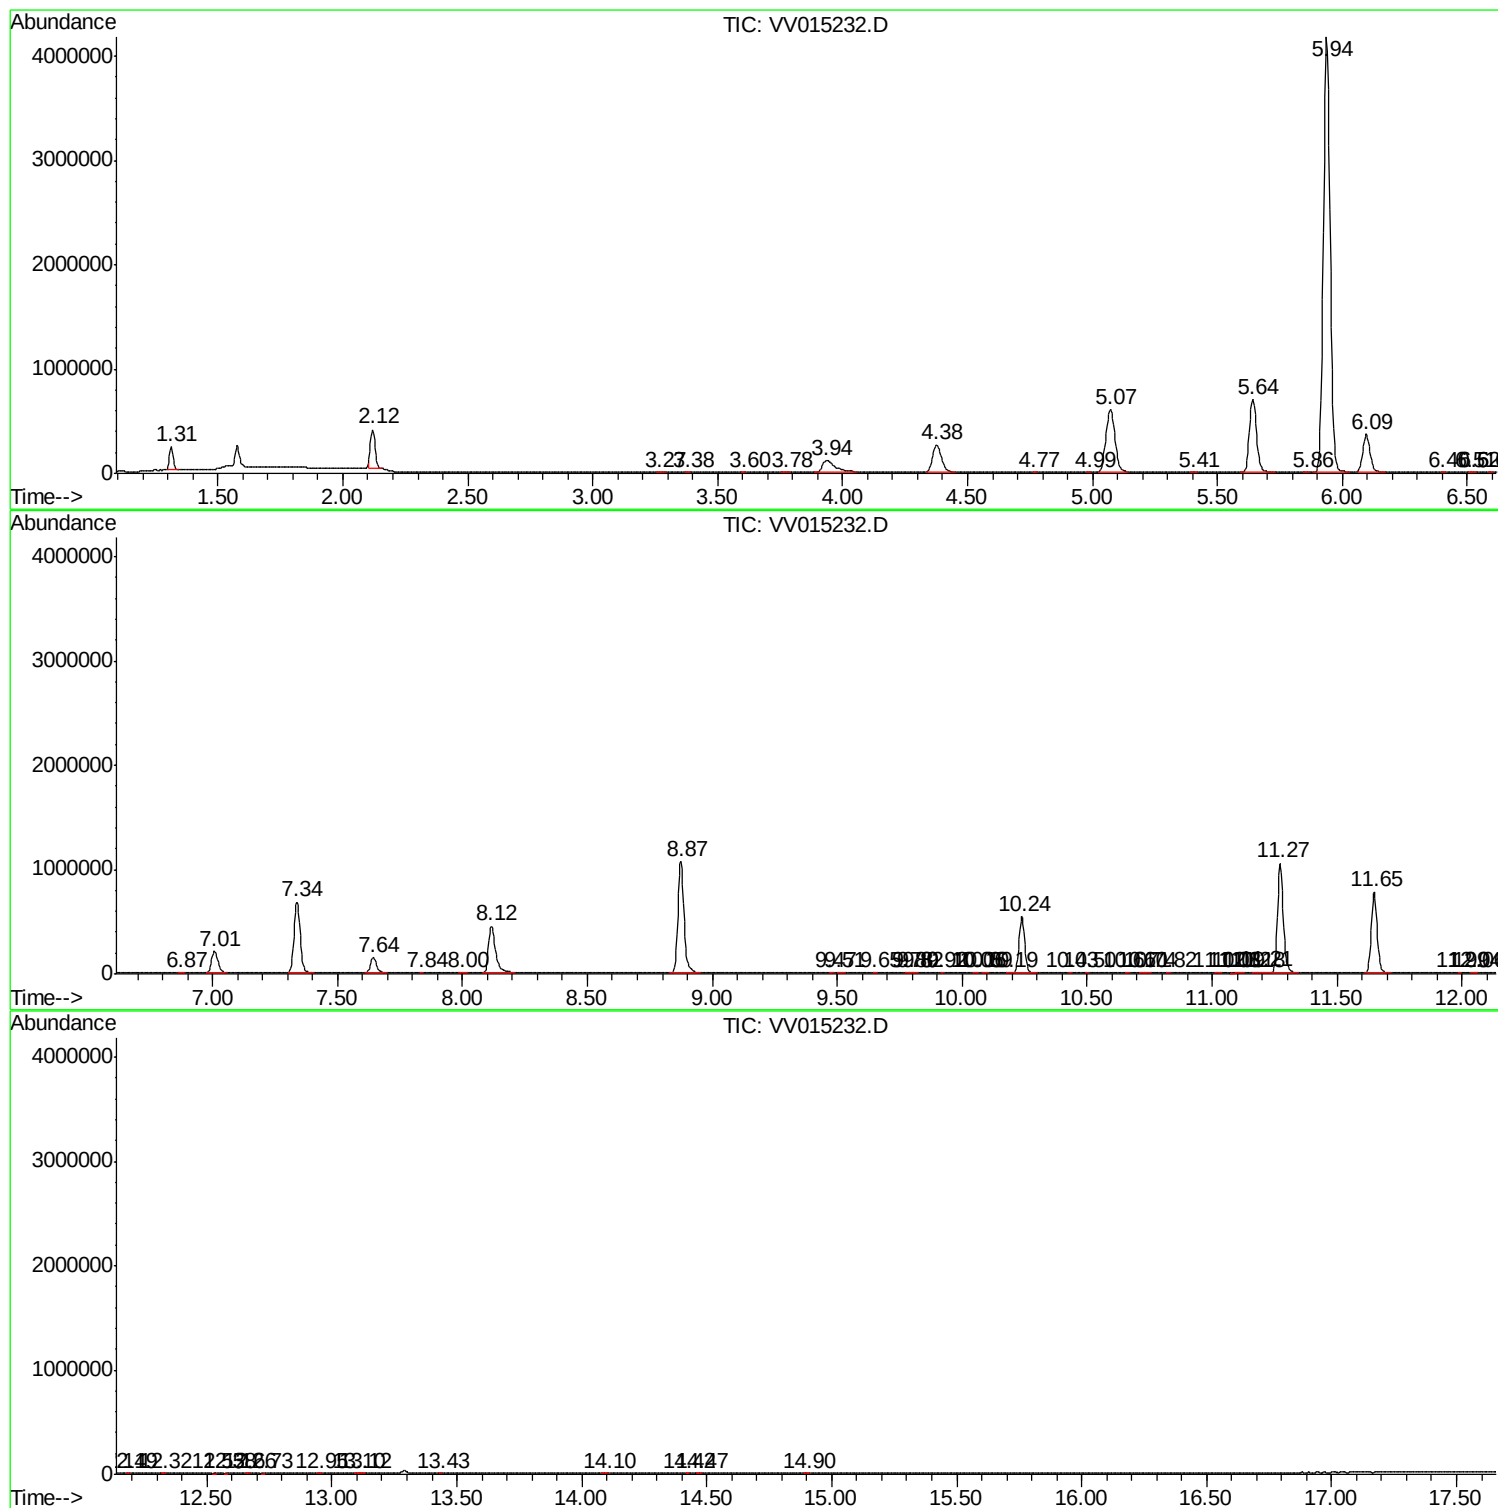

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV032720\
Data File : VV015232.D
Acq On : 28 Mar 2020 07:58
Operator : SY/MD
Sample : L1976-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTK6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032720\
Data File : VV015232.D
Acq On : 28 Mar 2020 07:58
Operator : SY/MD
Sample : L1976-21
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
ETTK6

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc