

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015234.D
 Acq On : 28 Mar 2020 08:47
 Operator : SY/MD
 Sample : L1976-23
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTL3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	64	71	85	rVB2	1317353	1381088	9.32%	3.931%
2	1.579	147	152	163	rVB	195843	223659	1.51%	0.637%
3	2.122	313	321	349	rVB2	540031	973193	6.57%	2.770%
4	3.373	706	710	712	rBV4	1688	1278	0.01%	0.004%
5	3.643	792	794	795	rBV2	1292	581	0.00%	0.002%
6	3.682	804	806	808	rBV3	1245	605	0.00%	0.002%
7	3.794	839	841	844	rVB3	2627	1279	0.01%	0.004%
8	3.823	847	850	852	rBV4	1655	1177	0.01%	0.003%
9	3.939	868	886	924	rBV	6105405	14822499	100.00%	42.189%
10	4.376	1010	1022	1042	rVB	268473	655219	4.42%	1.865%
11	4.708	1121	1125	1126	rBV4	1651	942	0.01%	0.003%
12	4.859	1169	1172	1175	rBV5	2978	2209	0.01%	0.006%
13	4.920	1187	1191	1192	rBV3	1655	1175	0.01%	0.003%
14	5.074	1222	1239	1268	rBV2	624459	1580139	10.66%	4.498%
15	5.643	1402	1416	1437	rBV2	740384	1470298	9.92%	4.185%
16	5.936	1493	1507	1533	rBV	2414597	4618857	31.16%	13.147%
17	6.097	1546	1557	1573	rVB	369179	727791	4.91%	2.072%
18	6.457	1667	1669	1672	rBV4	1575	894	0.01%	0.003%
19	6.576	1704	1706	1707	rBV2	1702	693	0.00%	0.002%
20	6.897	1802	1806	1808	rBV4	2365	1630	0.01%	0.005%
21	6.926	1813	1815	1817	rBV3	1666	918	0.01%	0.003%
22	7.010	1830	1841	1864	rBV	214281	377223	2.54%	1.074%
23	7.187	1893	1896	1900	rBV6	1977	1676	0.01%	0.005%
24	7.257	1915	1918	1920	rBV3	1780	1069	0.01%	0.003%
25	7.270	1920	1922	1924	rBV3	1610	791	0.01%	0.002%
26	7.338	1931	1943	1963	rBV	713974	1234348	8.33%	3.513%
27	7.643	2028	2038	2054	rBV	149478	254291	1.72%	0.724%
28	7.797	2084	2086	2087	rBV3	2066	703	0.00%	0.002%
29	7.855	2101	2104	2106	rBV4	2653	1755	0.01%	0.005%
30	7.897	2114	2117	2119	rBV3	2176	1301	0.01%	0.004%
31	7.942	2129	2131	2134	rBV4	2016	1654	0.01%	0.005%
32	8.116	2175	2185	2217	rBV2	463283	937018	6.32%	2.667%
33	8.344	2254	2256	2257	rBV2	1999	811	0.01%	0.002%
34	8.424	2279	2281	2283	rBV3	1503	730	0.00%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015234.D
 Acq On : 28 Mar 2020 08:47
 Operator : SY/MD
 Sample : L1976-23
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTL3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

35	8.650	2349	2351	2354	rBV4	1805	1370	0.01%	0.004%
36	8.678	2359	2360	2363	rVB3	1125	531	0.00%	0.002%
37	8.736	2375	2378	2381	rBV4	1284	724	0.00%	0.002%
38	8.768	2384	2388	2392	rBV8	2265	1745	0.01%	0.005%
39	8.791	2392	2395	2396	rBV2	1965	934	0.01%	0.003%
40	8.875	2409	2421	2446	rBV	1131666	1875049	12.65%	5.337%
41	9.270	2541	2544	2545	rBV3	2522	1120	0.01%	0.003%
42	9.309	2552	2556	2560	rBV6	2203	1839	0.01%	0.005%
43	9.328	2560	2562	2564	rBV3	1022	703	0.00%	0.002%
44	9.379	2575	2578	2581	rBV4	1837	1590	0.01%	0.005%
45	9.434	2589	2595	2596	rBV6	1952	1570	0.01%	0.004%
46	9.521	2617	2622	2624	rVB4	1808	1386	0.01%	0.004%
47	9.566	2633	2636	2637	rBV3	1845	1057	0.01%	0.003%
48	9.662	2664	2666	2668	rBV3	1863	949	0.01%	0.003%
49	9.701	2675	2678	2682	rVB4	2588	1878	0.01%	0.005%
50	9.723	2682	2685	2687	rBV3	1200	765	0.01%	0.002%
51	9.788	2700	2705	2706	rBV4	1889	1304	0.01%	0.004%
52	9.823	2711	2716	2718	rBV5	3013	2012	0.01%	0.006%
53	9.855	2723	2726	2727	rBV3	1378	787	0.01%	0.002%
54	9.923	2745	2747	2749	rBV3	1654	919	0.01%	0.003%
55	9.994	2767	2769	2774	rVB5	2990	2012	0.01%	0.006%
56	10.029	2774	2780	2781	rBV6	1928	1895	0.01%	0.005%
57	10.238	2833	2845	2861	rBV	568156	884721	5.97%	2.518%
58	10.469	2914	2917	2920	rBV4	1779	1022	0.01%	0.003%
59	10.666	2976	2978	2979	rBV2	1537	682	0.00%	0.002%
60	10.682	2982	2983	2985	rVV2	1545	823	0.01%	0.002%
61	10.714	2989	2993	2996	rVB5	2132	1514	0.01%	0.004%
62	10.730	2996	2998	3001	rBV3	1888	1289	0.01%	0.004%
63	10.849	3033	3035	3039	rVB4	2251	1228	0.01%	0.003%
64	10.875	3039	3043	3048	rBV7	2649	3471	0.02%	0.010%
65	10.965	3068	3071	3072	rBV2	1510	701	0.00%	0.002%
66	11.006	3082	3084	3090	rVB6	2138	1860	0.01%	0.005%
67	11.035	3091	3093	3096	rBV4	1662	833	0.01%	0.002%
68	11.125	3117	3121	3122	rBV5	1484	1140	0.01%	0.003%
69	11.273	3154	3167	3186	rBV	1086946	1707159	11.52%	4.859%
70	11.563	3248	3257	3268	rBV7	9304	16831	0.11%	0.048%
71	11.649	3272	3284	3301	rBV	793600	1255666	8.47%	3.574%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015234.D
 Acq On : 28 Mar 2020 08:47
 Operator : SY/MD
 Sample : L1976-23
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTL3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

72	11.862	3347	3350	3354	rVB5	1460	1058	0.01%	0.003%
73	12.029	3398	3402	3404	rBV4	1546	1269	0.01%	0.004%
74	12.051	3407	3409	3411	rBV3	1310	606	0.00%	0.002%
75	12.100	3422	3424	3425	rBV2	1721	726	0.00%	0.002%
76	12.193	3450	3453	3455	rBV4	1189	684	0.00%	0.002%
77	12.302	3485	3487	3489	rBV3	1591	783	0.01%	0.002%
78	12.363	3501	3506	3511	rBV9	2556	2880	0.02%	0.008%
79	12.437	3526	3529	3532	rBV3	1470	890	0.01%	0.003%
80	12.665	3593	3600	3601	rBV7	2449	3067	0.02%	0.009%
81	12.707	3610	3613	3615	rBV3	1558	1111	0.01%	0.003%
82	12.784	3633	3637	3643	rBV9	2775	2649	0.02%	0.008%
83	12.813	3643	3646	3651	rVV6	1854	1888	0.01%	0.005%
84	12.849	3655	3657	3662	rVB5	2238	1185	0.01%	0.003%
85	12.871	3662	3664	3666	rBV3	1219	554	0.00%	0.002%
86	13.093	3728	3733	3738	rBV7	2918	2765	0.02%	0.008%
87	13.125	3741	3743	3745	rBV3	1332	720	0.00%	0.002%
88	13.154	3749	3752	3754	rBV3	2086	1111	0.01%	0.003%
89	13.228	3774	3775	3782	rBV7	1476	1677	0.01%	0.005%
90	13.257	3782	3784	3785	rBV2	1868	787	0.01%	0.002%
91	13.289	3786	3794	3803	rVB6	17266	26263	0.18%	0.075%
92	13.659	3906	3909	3910	rBV3	1374	700	0.00%	0.002%
93	13.669	3910	3912	3913	rBV2	1360	576	0.00%	0.002%
94	13.772	3935	3944	3952	rBV2	5647	11194	0.08%	0.032%
95	13.820	3956	3959	3963	rBV5	1642	1590	0.01%	0.005%
96	14.222	4082	4084	4086	rBV3	1345	579	0.00%	0.002%
97	14.292	4103	4106	4108	rBV3	2972	1774	0.01%	0.005%
98	14.704	4232	4234	4235	rBV3	1631	627	0.00%	0.002%
99	14.849	4277	4279	4282	rVB4	3449	1592	0.01%	0.005%
100	14.910	4295	4298	4301	rBV3	2252	1348	0.01%	0.004%


Sum of corrected areas: 35133226

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032720\
Data File : VV015234.D
Acq On : 28 Mar 2020 08:47
Operator : SY/MD
Sample : L1976-23
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTL3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

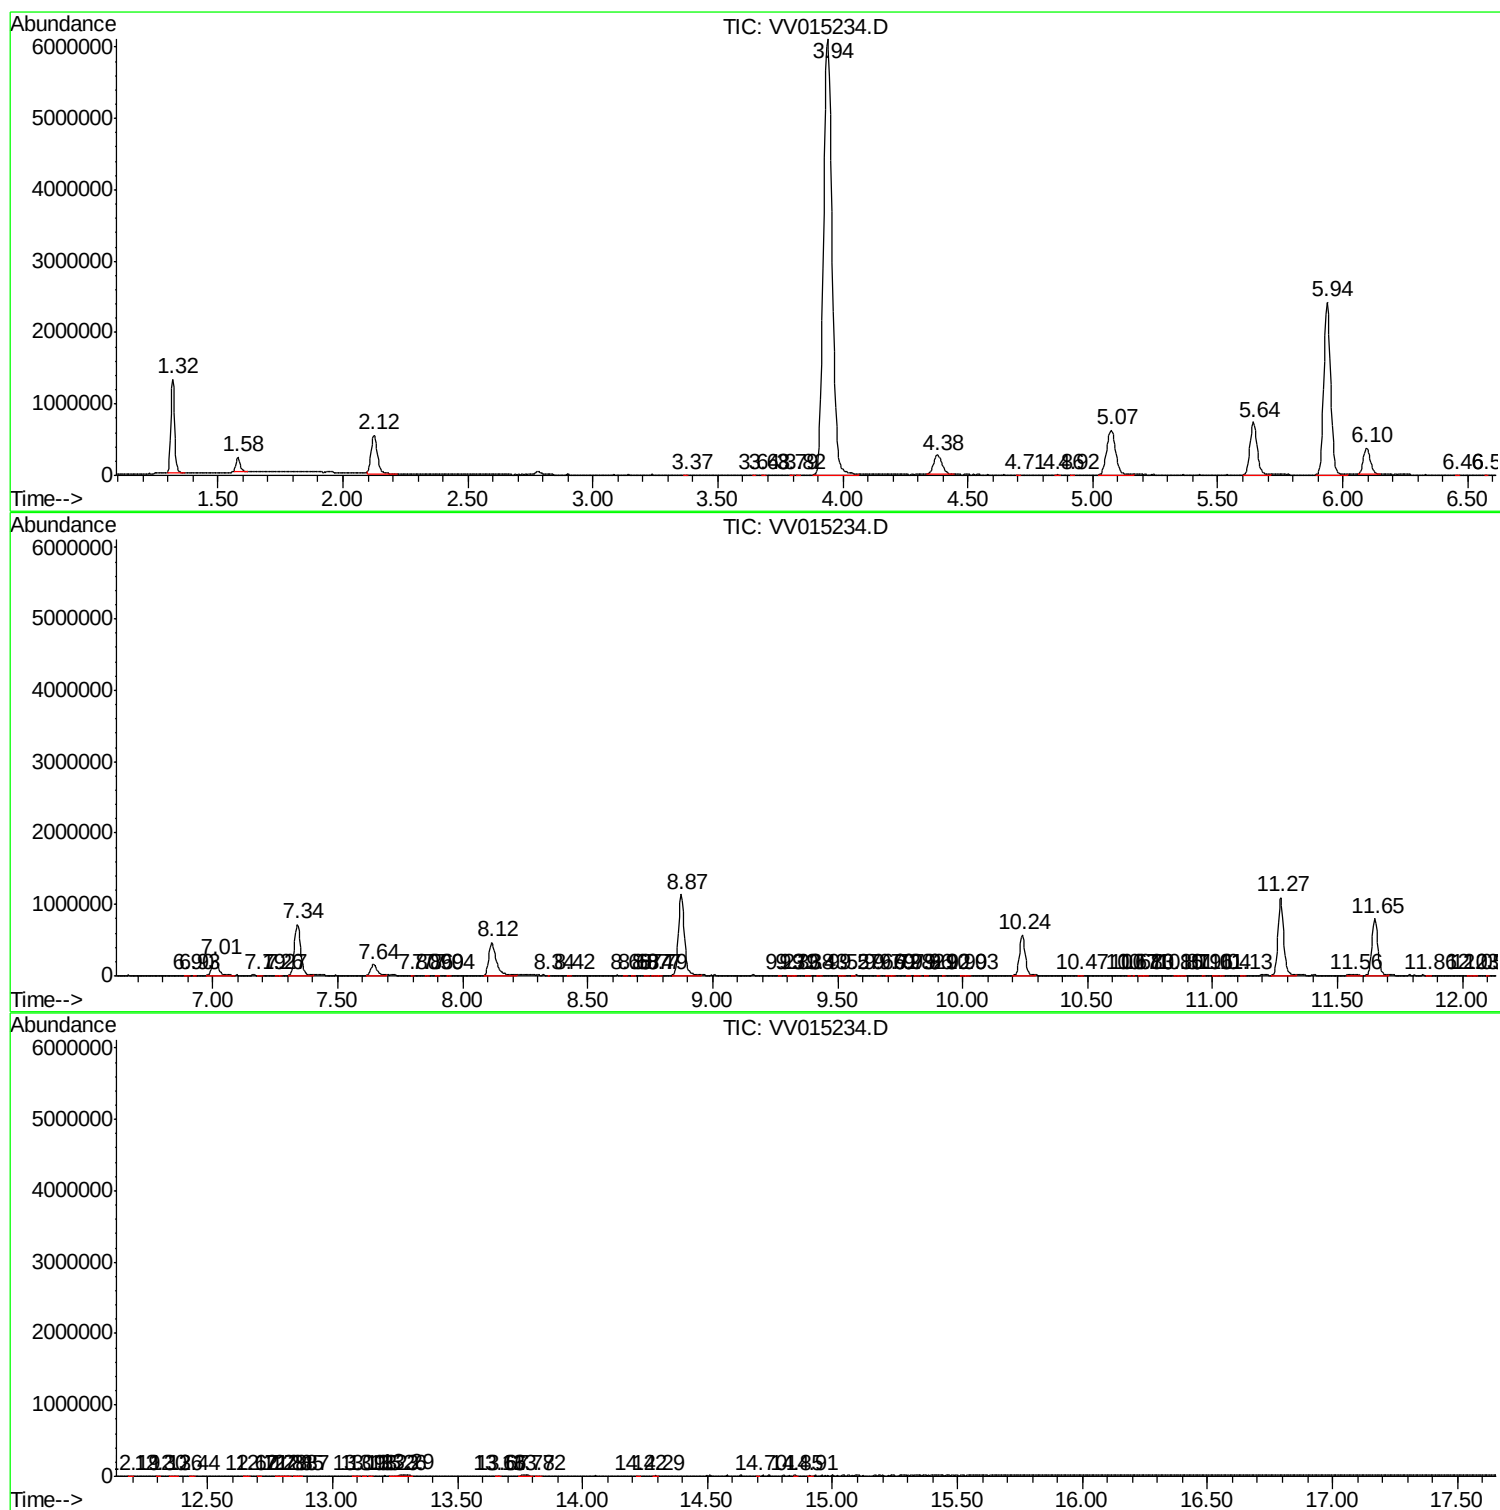

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV032720\
Data File : VV015234.D
Acq On : 28 Mar 2020 08:47
Operator : SY/MD
Sample : L1976-23
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTL3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032720\
Data File : VV015234.D
Acq On : 28 Mar 2020 08:47
Operator : SY/MD
Sample : L1976-23
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
ETTL3

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc