

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015237.D
 Acq On : 28 Mar 2020 10:00
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	64	69	82	rVB	237864	234634	12.56%	1.567%
2	1.576	146	151	160	rVB	200236	223409	11.96%	1.492%
3	2.119	313	320	333	rVB	434670	609816	32.64%	4.073%
4	3.161	641	644	646	rBV3	1939	1176	0.06%	0.008%
5	3.418	719	724	729	rBV9	2679	3062	0.16%	0.020%
6	3.598	777	780	782	rBV4	1749	1199	0.06%	0.008%
7	3.637	789	792	796	rVB5	2409	1227	0.07%	0.008%
8	3.682	802	806	807	rBV4	1877	1114	0.06%	0.007%
9	3.827	844	851	852	rBV7	2810	2559	0.14%	0.017%
10	3.884	865	869	871	rBV5	1794	1231	0.07%	0.008%
11	3.939	873	886	926	rBV2	100675	513463	27.48%	3.430%
12	4.376	1008	1022	1044	rVB	275096	669413	35.83%	4.471%
13	4.862	1170	1173	1174	rBV2	1597	1006	0.05%	0.007%
14	5.071	1219	1238	1267	rBV2	641942	1609198	86.12%	10.748%
15	5.460	1355	1359	1362	rBV5	1663	1448	0.08%	0.010%
16	5.569	1390	1393	1396	rBV5	3053	2539	0.14%	0.017%
17	5.640	1402	1415	1441	rBV	733058	1470970	78.72%	9.825%
18	5.936	1492	1507	1522	rBV	14481	37580	2.01%	0.251%
19	6.093	1542	1556	1580	rBV	378998	779199	41.70%	5.204%
20	6.306	1616	1622	1624	rBV7	2417	2795	0.15%	0.019%
21	6.357	1635	1638	1640	rBV4	2595	1764	0.09%	0.012%
22	6.733	1753	1755	1758	rBV4	1766	1157	0.06%	0.008%
23	6.762	1762	1764	1769	rVB5	2680	1662	0.09%	0.011%
24	6.788	1769	1772	1773	rBV3	1900	1071	0.06%	0.007%
25	7.010	1825	1841	1861	rBV2	210268	390573	20.90%	2.609%
26	7.241	1911	1913	1918	rBV6	1379	1095	0.06%	0.007%
27	7.293	1927	1929	1930	rBV2	1783	903	0.05%	0.006%
28	7.338	1930	1943	1962	rVV	736479	1276813	68.33%	8.528%
29	7.569	2013	2015	2017	rBV2	1786	960	0.05%	0.006%
30	7.643	2028	2038	2054	rBV2	146618	255825	13.69%	1.709%
31	7.781	2078	2081	2085	rBV5	1865	1477	0.08%	0.010%
32	7.875	2108	2110	2113	rBV3	1817	1187	0.06%	0.008%
33	8.116	2174	2185	2224	rBV2	468419	980986	52.50%	6.552%
34	8.531	2312	2314	2320	rBV6	1693	1842	0.10%	0.012%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015237.D
 Acq On : 28 Mar 2020 10:00
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

35	8.579	2327	2329	2332	rBV3	2098	971	0.05%	0.006%
36	8.675	2355	2359	2364	rBV6	2192	2644	0.14%	0.018%
37	8.813	2398	2402	2403	rBV4	1539	1033	0.06%	0.007%
38	8.875	2408	2421	2443	rBV	1130076	1868523	100.00%	12.480%
39	9.151	2500	2507	2508	rBV6	2647	2736	0.15%	0.018%
40	9.228	2529	2531	2534	rVB3	1928	1075	0.06%	0.007%
41	9.296	2549	2552	2554	rBV3	2356	1154	0.06%	0.008%
42	9.341	2562	2566	2570	rVB6	1955	1564	0.08%	0.010%
43	9.370	2570	2575	2578	rBV7	1874	2133	0.11%	0.014%
44	9.463	2600	2604	2607	rBV5	1259	1253	0.07%	0.008%
45	9.604	2644	2648	2652	rVB6	1648	1189	0.06%	0.008%
46	9.627	2652	2655	2657	rBV3	1547	985	0.05%	0.007%
47	9.701	2674	2678	2682	rBV6	1456	1599	0.09%	0.011%
48	9.743	2686	2691	2693	rBV5	1646	1408	0.08%	0.009%
49	9.791	2701	2706	2707	rBV5	2516	1846	0.10%	0.012%
50	9.952	2754	2756	2763	rVB8	3534	3443	0.18%	0.023%
51	10.003	2767	2772	2773	rBV5	2801	2408	0.13%	0.016%
52	10.061	2788	2790	2792	rBV3	1504	923	0.05%	0.006%
53	10.119	2805	2808	2810	rBV3	1678	1054	0.06%	0.007%
54	10.238	2833	2845	2866	rBV	554913	885410	47.39%	5.914%
55	10.408	2895	2898	2903	rBV7	1860	2145	0.11%	0.014%
56	10.547	2937	2941	2942	rBV3	1467	1071	0.06%	0.007%
57	10.595	2953	2956	2959	rBV5	2548	1567	0.08%	0.010%
58	10.711	2983	2992	2994	rBV8	3485	3237	0.17%	0.022%
59	10.730	2994	2998	3000	rBV5	2044	1384	0.07%	0.009%
60	10.762	3005	3008	3010	rBV4	2113	1203	0.06%	0.008%
61	10.791	3013	3017	3020	rVB6	1249	1013	0.05%	0.007%
62	10.846	3032	3034	3036	rBV3	1922	1045	0.06%	0.007%
63	10.936	3060	3062	3063	rBV2	2075	922	0.05%	0.006%
64	11.013	3082	3086	3089	rBV4	1632	1324	0.07%	0.009%
65	11.125	3119	3121	3125	rVB4	1479	951	0.05%	0.006%
66	11.174	3131	3136	3138	rBV5	2938	2547	0.14%	0.017%
67	11.273	3155	3167	3186	rBV	1115432	1733403	92.77%	11.578%
68	11.501	3236	3238	3241	rVB4	2090	1181	0.06%	0.008%
69	11.550	3250	3253	3256	rBV4	2185	1566	0.08%	0.010%
70	11.649	3272	3284	3300	rBV	797871	1277674	68.38%	8.534%
71	11.784	3323	3326	3329	rBV6	2087	1418	0.08%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015237.D
 Acq On : 28 Mar 2020 10:00
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

72	11.868	3348	3352	3354	rBV5	1540	1395	0.07%	0.009%
73	12.064	3406	3413	3415	rVV7	1958	2670	0.14%	0.018%
74	12.180	3444	3449	3452	rBV6	2272	1607	0.09%	0.011%
75	12.231	3461	3465	3470	rBV8	1831	2048	0.11%	0.014%
76	12.264	3470	3475	3477	rBV5	2458	2829	0.15%	0.019%
77	12.447	3528	3532	3536	rVB6	2422	2174	0.12%	0.015%
78	12.476	3536	3541	3543	rBV6	2365	1658	0.09%	0.011%
79	12.662	3594	3599	3601	rBV5	3457	2470	0.13%	0.016%
80	12.739	3621	3623	3626	rBV4	1757	1115	0.06%	0.007%
81	12.820	3646	3648	3653	rVB4	1838	1125	0.06%	0.008%
82	12.842	3653	3655	3660	rBV6	2098	1546	0.08%	0.010%
83	13.064	3722	3724	3727	rBV4	1543	1137	0.06%	0.008%
84	13.106	3735	3737	3738	rBV3	2587	1046	0.06%	0.007%
85	13.145	3745	3749	3752	rBV6	1976	1374	0.07%	0.009%
86	13.215	3768	3771	3773	rBV2	1987	975	0.05%	0.007%
87	13.286	3785	3793	3804	rBV8	12972	22415	1.20%	0.150%
88	13.344	3809	3811	3814	rBV2	1742	1279	0.07%	0.009%
89	13.431	3835	3838	3841	rBV5	1974	1320	0.07%	0.009%
90	13.633	3898	3901	3902	rBV3	2650	1437	0.08%	0.010%
91	13.730	3929	3931	3934	rVB4	1965	1056	0.06%	0.007%
92	13.752	3934	3938	3939	rBV4	2376	1659	0.09%	0.011%
93	13.884	3976	3979	3985	rBV8	2335	2606	0.14%	0.017%
94	13.971	4002	4006	4009	rBV5	2350	1991	0.11%	0.013%
95	14.061	4031	4034	4038	rBV5	2552	1912	0.10%	0.013%
96	14.379	4129	4133	4135	rBV5	2180	1804	0.10%	0.012%
97	14.726	4238	4241	4246	rBV7	2046	2032	0.11%	0.014%
98	14.897	4292	4294	4296	rBV3	1936	1026	0.05%	0.007%
99	15.196	4385	4387	4390	rBV4	1994	1354	0.07%	0.009%
100	15.421	4454	4457	4461	rBV6	3651	3414	0.18%	0.023%


Sum of corrected areas: 14971829

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032720\
Data File : VV015237.D
Acq On : 28 Mar 2020 10:00
Operator : SY/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

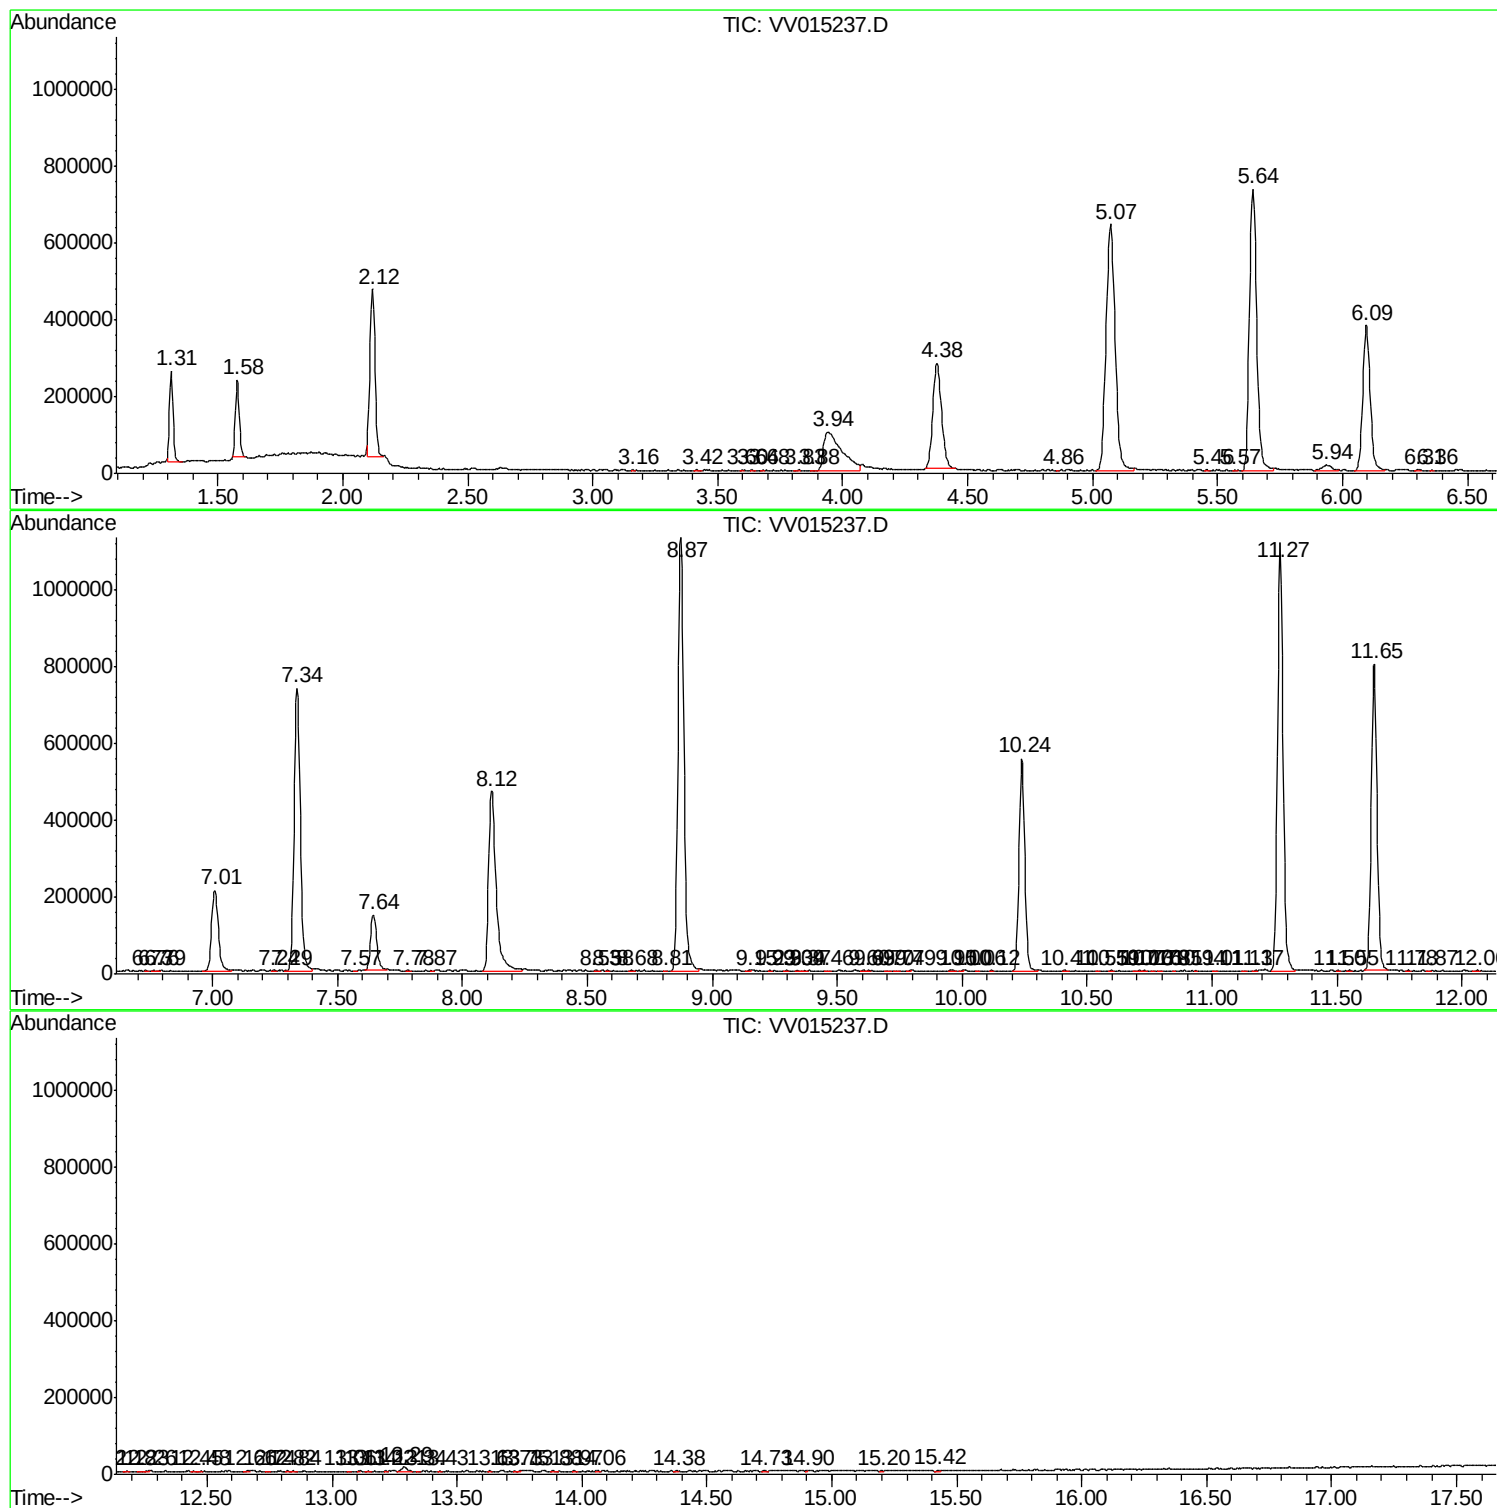

Data_Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV032720\
Data_File : VV015237.D
Acq_On : 28-Mar-2020 10:000
Operator : SY/MDD
Sample : VIBLKK
Misc : 5.0mL/MSVOA_V/WATERR
ALS_Vial : 1 Sample_Multiplier: 11

Instrument :
MSVOA_V
ClientSampleId :
VIBLK

Quant_Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.MM
Quant_Title : VOC_Analysis

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
