

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015240.D
 Acq On : 28 Mar 2020 12:17
 Operator : SY/MD
 Sample : L1975-09 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTH4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	65	70	81	rVB	203614	205602	10.84%	1.513%
2	1.579	146	152	163	rVB	179838	208619	11.00%	1.536%
3	2.119	314	320	331	rVB	380051	521570	27.49%	3.839%
4	2.949	575	578	581	rBV4	2220	1794	0.09%	0.013%
5	3.132	632	635	638	rVB4	2052	1218	0.06%	0.009%
6	3.502	748	750	755	rBV6	1319	874	0.05%	0.006%
7	3.807	843	845	848	rBV3	1407	557	0.03%	0.004%
8	3.885	865	869	873	rVB6	2249	2305	0.12%	0.017%
9	3.939	874	886	887	rBV2	80980	111910	5.90%	0.824%
10	4.380	1010	1023	1045	rVB2	245714	600721	31.66%	4.422%
11	4.795	1150	1152	1154	rBV3	1102	713	0.04%	0.005%
12	4.881	1175	1179	1181	rBV4	2667	1779	0.09%	0.013%
13	4.930	1189	1194	1195	rBV4	2415	1804	0.10%	0.013%
14	4.994	1208	1214	1219	rBV9	1985	2208	0.12%	0.016%
15	5.074	1222	1239	1266	rVV3	567915	1441069	75.95%	10.607%
16	5.428	1346	1349	1351	rBV2	1695	1246	0.07%	0.009%
17	5.544	1383	1385	1387	rBV3	843	422	0.02%	0.003%
18	5.640	1402	1415	1436	rBV	751315	1494056	78.75%	10.997%
19	6.036	1535	1538	1540	rBV4	2117	1678	0.09%	0.012%
20	6.097	1544	1557	1582	rVV2	334241	693129	36.53%	5.102%
21	6.412	1653	1655	1659	rVB5	2293	1489	0.08%	0.011%
22	6.434	1659	1662	1663	rBV3	1444	784	0.04%	0.006%
23	6.518	1686	1688	1693	rVB5	2204	1757	0.09%	0.013%
24	6.608	1714	1716	1718	rBV3	1036	386	0.02%	0.003%
25	6.775	1767	1768	1771	rBV3	1037	637	0.03%	0.005%
26	6.820	1780	1782	1787	rVB6	2837	1885	0.10%	0.014%
27	6.856	1791	1793	1797	rVB5	1196	533	0.03%	0.004%
28	6.881	1797	1801	1804	rBV6	1795	1416	0.07%	0.010%
29	7.010	1830	1841	1857	rBV	200263	365029	19.24%	2.687%
30	7.338	1931	1943	1958	rBV	659349	1138348	60.00%	8.379%
31	7.643	2028	2038	2061	rBV	145880	251252	13.24%	1.849%
32	7.865	2104	2107	2108	rBV2	2242	1219	0.06%	0.009%
33	8.116	2175	2185	2214	rBV2	430783	870893	45.90%	6.410%
34	8.380	2265	2267	2270	rVB4	3096	1606	0.08%	0.012%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015240.D
 Acq On : 28 Mar 2020 12:17
 Operator : SY/MD
 Sample : L1975-09 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTH4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

35	8.875	2409	2421	2449	rBV	1163113	1897282	100.00%	13.965%
36	9.148	2504	2506	2508	rBV3	1541	996	0.05%	0.007%
37	9.232	2528	2532	2535	rBV6	2164	2527	0.13%	0.019%
38	9.341	2565	2566	2568	rBV2	977	427	0.02%	0.003%
39	9.511	2616	2619	2621	rBV4	2645	1604	0.08%	0.012%
40	9.550	2629	2631	2633	rBV2	1502	870	0.05%	0.006%
41	9.714	2680	2682	2684	rBV2	1056	558	0.03%	0.004%
42	9.753	2688	2694	2697	rBV7	2303	2342	0.12%	0.017%
43	9.801	2707	2709	2713	rVB4	2044	1290	0.07%	0.009%
44	9.826	2713	2717	2721	rBV7	2773	3032	0.16%	0.022%
45	10.023	2774	2778	2779	rBV4	2113	1728	0.09%	0.013%
46	10.077	2792	2795	2797	rBV4	1246	632	0.03%	0.005%
47	10.183	2825	2828	2829	rBV3	1591	909	0.05%	0.007%
48	10.193	2829	2831	2832	rVV2	2117	1002	0.05%	0.007%
49	10.238	2834	2845	2863	rVV	507159	794560	41.88%	5.848%
50	10.363	2881	2884	2888	rBV5	2284	1690	0.09%	0.012%
51	10.447	2907	2910	2912	rBV4	2016	1023	0.05%	0.008%
52	10.634	2966	2968	2970	rBV3	1635	843	0.04%	0.006%
53	10.669	2976	2979	2980	rBV2	1417	1013	0.05%	0.007%
54	10.868	3036	3041	3042	rBV6	1800	1630	0.09%	0.012%
55	10.910	3050	3054	3057	rBV5	3103	2623	0.14%	0.019%
56	10.936	3059	3062	3066	rBV5	2088	1790	0.09%	0.013%
57	10.974	3072	3074	3075	rBV2	1449	547	0.03%	0.004%
58	11.100	3111	3113	3117	rVB4	1035	502	0.03%	0.004%
59	11.122	3117	3120	3122	rBV4	1262	759	0.04%	0.006%
60	11.273	3155	3167	3183	rBV	1129213	1745242	91.99%	12.846%
61	11.650	3272	3284	3300	rBV	722311	1147031	60.46%	8.443%
62	11.823	3335	3338	3342	rVB6	3061	2295	0.12%	0.017%
63	11.929	3368	3371	3374	rBV5	1488	1032	0.05%	0.008%
64	12.026	3399	3401	3402	rBV2	1129	471	0.02%	0.003%
65	12.080	3416	3418	3420	rBV3	1256	582	0.03%	0.004%
66	12.158	3439	3442	3443	rBV2	1467	745	0.04%	0.005%
67	12.225	3460	3463	3464	rBV3	2006	821	0.04%	0.006%
68	12.251	3468	3471	3474	rBV4	2349	1952	0.10%	0.014%
69	12.556	3562	3566	3570	rVB6	1991	1316	0.07%	0.010%
70	12.633	3587	3590	3595	rBV7	2217	1903	0.10%	0.014%
71	12.672	3597	3602	3608	rBV9	3406	4989	0.26%	0.037%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
Data File : VV015240.D
Acq On : 28 Mar 2020 12:17
Operator : SY/MD
Sample : L1975-09 40X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTH4

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Title : VOC Analysis

72	12.730	3614	3620	3623	rBV8	2181	1971	0.10%	0.015%
73	13.010	3705	3707	3713	rBV7	2026	1221	0.06%	0.009%
74	13.106	3732	3737	3741	rBV7	2893	3227	0.17%	0.024%
75	13.145	3747	3749	3750	rBV2	833	374	0.02%	0.003%
76	13.402	3827	3829	3830	rBV2	1566	662	0.03%	0.005%
77	13.621	3888	3897	3900	rBV9	3390	4484	0.24%	0.033%
78	13.775	3938	3945	3955	rVB9	5172	7445	0.39%	0.055%
79	13.907	3984	3986	3989	rBV4	1892	1044	0.06%	0.008%
80	14.029	4022	4024	4028	rVB4	1857	891	0.05%	0.007%
81	14.257	4092	4095	4098	rBV5	2009	1636	0.09%	0.012%
82	14.553	4184	4187	4190	rBV3	2943	1937	0.10%	0.014%


Sum of corrected areas: 13585958

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032720\
Data File : VV015240.D
Acq On : 28 Mar 2020 12:17
Operator : SY/MD
Sample : L1975-09 40X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTH4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

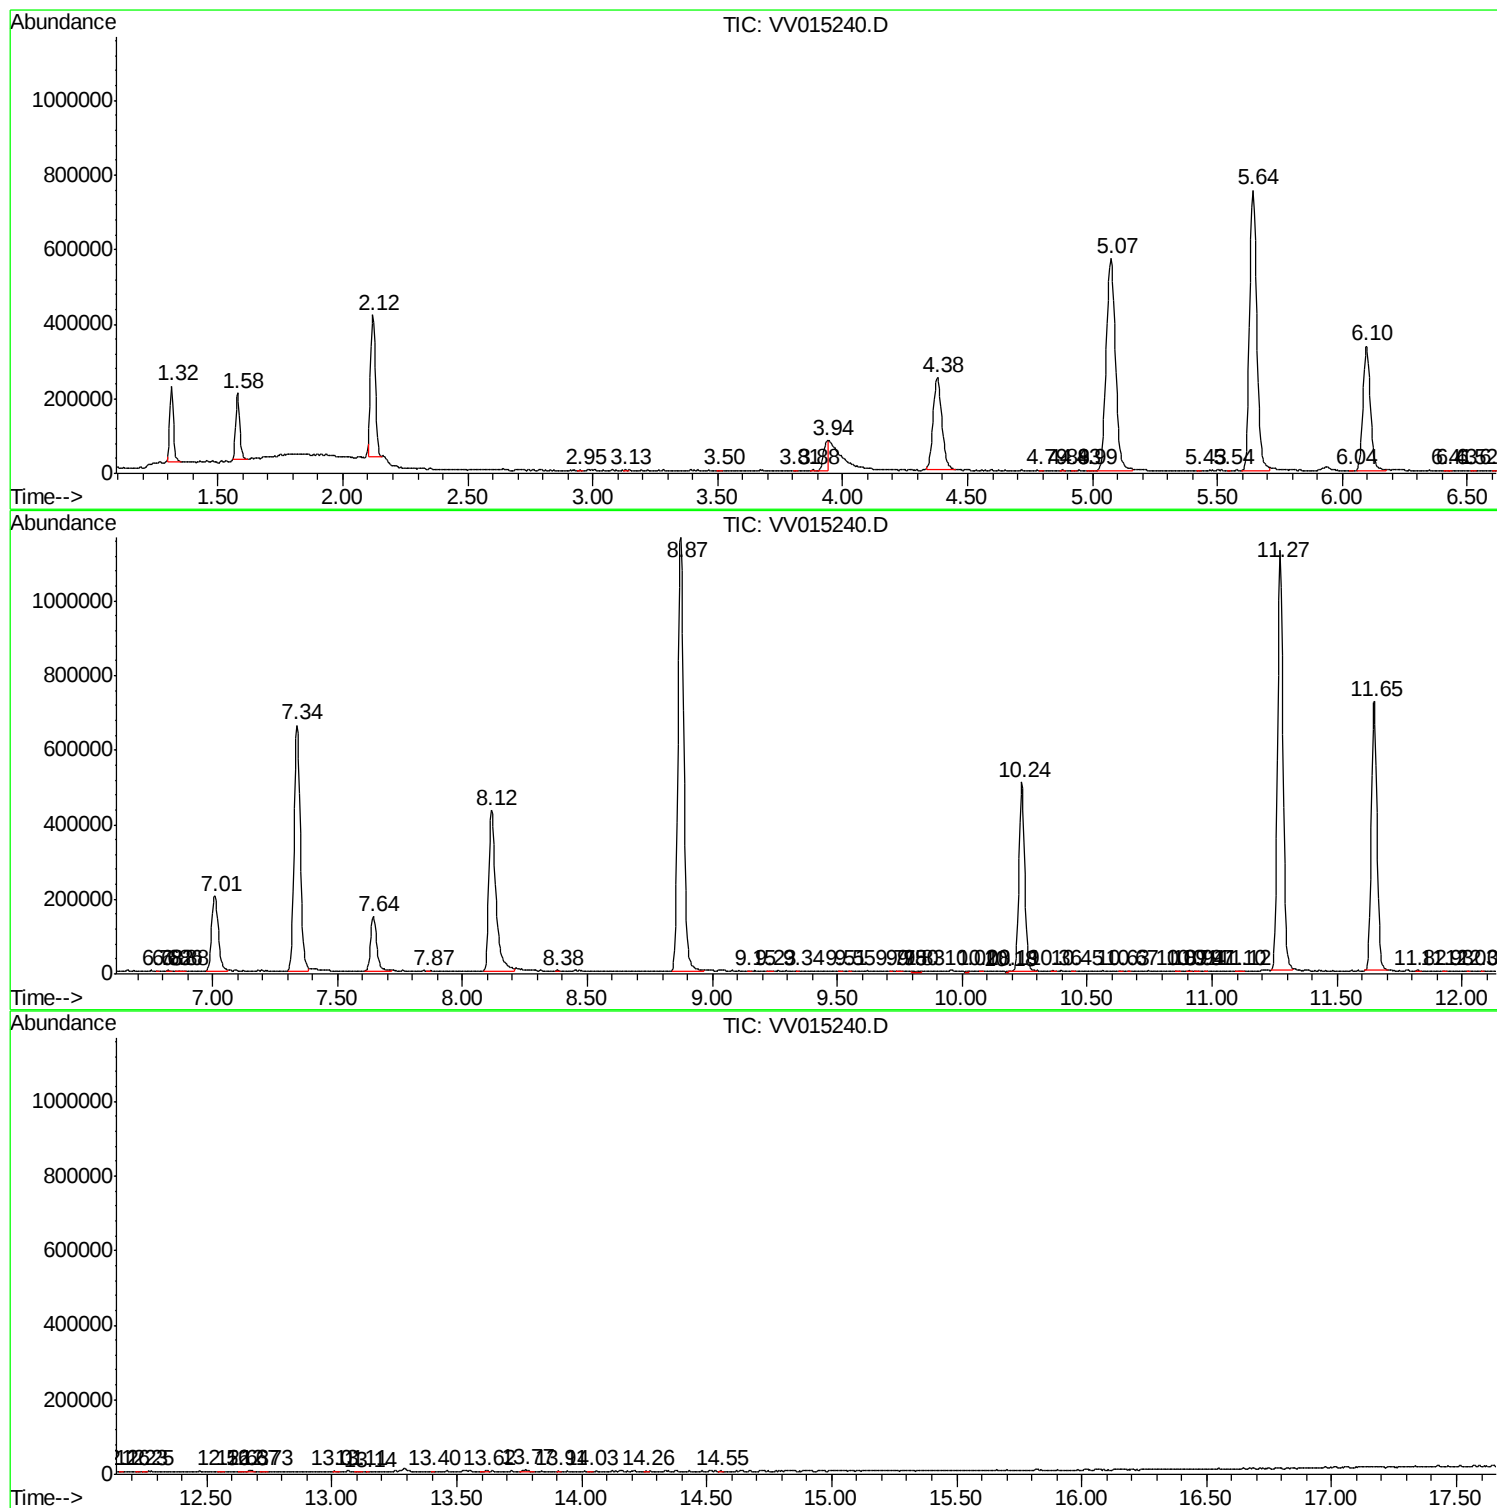

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV032720\
Data File : VV015240.D
Acq On : 28 Mar 2020 12:17
Operator : SY/MD
Sample : L1975-09 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTH4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032720\
Data File : VV015240.D
Acq On : 28 Mar 2020 12:17
Operator : SY/MD
Sample : L1975-09 40X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
ETTH4

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc