

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015241.D
 Acq On : 28 Mar 2020 12:45
 Operator : SY/MD
 Sample : L1975-01 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTG6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	80	rVB	227396	236466	10.60%	1.434%
2	1.576	146	151	162	rVB	205970	241393	10.82%	1.464%
3	2.119	313	320	347	rVB	470489	718741	32.23%	4.359%
4	3.097	621	624	625	rBV2	1996	1234	0.06%	0.007%
5	3.190	650	653	655	rBV3	1038	742	0.03%	0.004%
6	3.222	659	663	664	rBV4	1158	945	0.04%	0.006%
7	3.380	709	712	714	rBV3	1887	951	0.04%	0.006%
8	3.473	740	741	743	rBV2	1235	627	0.03%	0.004%
9	3.634	786	791	793	rVB5	1762	1271	0.06%	0.008%
10	3.936	874	885	923	rBV	90407	431267	19.34%	2.615%
11	4.376	1009	1022	1050	rVB	294262	727307	32.61%	4.410%
12	4.550	1073	1076	1078	rBV4	3195	2007	0.09%	0.012%
13	4.727	1129	1131	1133	rBV3	1578	889	0.04%	0.005%
14	5.006	1215	1218	1219	rBV2	2017	907	0.04%	0.006%
15	5.071	1222	1238	1266	rVV2	666841	1684962	75.55%	10.218%
16	5.402	1339	1341	1342	rBV2	1865	733	0.03%	0.004%
17	5.640	1402	1415	1440	rBV	901555	1788065	80.17%	10.843%
18	6.003	1526	1528	1532	rBV3	2122	1957	0.09%	0.012%
19	6.035	1535	1538	1540	rBV3	1785	1055	0.05%	0.006%
20	6.093	1543	1556	1579	rVV	394459	810708	36.35%	4.916%
21	6.289	1615	1617	1620	rVB4	2536	1280	0.06%	0.008%
22	6.312	1620	1624	1625	rBV4	1937	1139	0.05%	0.007%
23	6.479	1674	1676	1679	rVB4	1445	672	0.03%	0.004%
24	6.630	1718	1723	1725	rBV5	2641	2608	0.12%	0.016%
25	6.775	1766	1768	1771	rBV3	1673	1148	0.05%	0.007%
26	6.826	1782	1784	1788	rVB5	1429	891	0.04%	0.005%
27	6.852	1788	1792	1796	rBV6	2253	1753	0.08%	0.011%
28	6.916	1808	1812	1813	rBV3	1591	1141	0.05%	0.007%
29	7.006	1826	1840	1857	rBV	243965	442339	19.83%	2.682%
30	7.251	1913	1916	1919	rBV5	1798	1478	0.07%	0.009%
31	7.338	1931	1943	1963	rBV	786784	1357065	60.85%	8.229%
32	7.566	2012	2014	2017	rBV3	1528	762	0.03%	0.005%
33	7.588	2019	2021	2023	rVV3	1745	766	0.03%	0.005%
34	7.643	2028	2038	2054	rBV	170111	292016	13.09%	1.771%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015241.D
 Acq On : 28 Mar 2020 12:45
 Operator : SY/MD
 Sample : L1975-01 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTG6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

35	7.923	2123	2125	2129	rBV4	1902	1319	0.06%	0.008%
36	8.116	2175	2185	2226	rBV2	464193	978212	43.86%	5.932%
37	8.592	2329	2333	2334	rBV4	1868	1260	0.06%	0.008%
38	8.804	2396	2399	2400	rBV2	1620	855	0.04%	0.005%
39	8.871	2409	2420	2448	rBV	1390543	2230209	100.00%	13.524%
40	9.064	2478	2480	2483	rBV4	1366	929	0.04%	0.006%
41	9.254	2537	2539	2541	rBV3	1533	726	0.03%	0.004%
42	9.334	2561	2564	2566	rBV3	1432	1041	0.05%	0.006%
43	9.376	2571	2577	2580	rBV8	2233	2688	0.12%	0.016%
44	9.415	2587	2589	2593	rBV4	1412	1111	0.05%	0.007%
45	9.444	2596	2598	2600	rBV3	1646	865	0.04%	0.005%
46	9.511	2614	2619	2622	rVV7	2072	2238	0.10%	0.014%
47	9.826	2715	2717	2719	rBV3	1193	716	0.03%	0.004%
48	9.981	2761	2765	2766	rBV3	1372	1093	0.05%	0.007%
49	10.064	2789	2791	2794	rBV4	1560	1071	0.05%	0.006%
50	10.096	2798	2801	2804	rVV4	1430	1004	0.05%	0.006%
51	10.132	2810	2812	2814	rBV3	1789	943	0.04%	0.006%
52	10.238	2830	2845	2859	rBV	584135	921074	41.30%	5.585%
53	10.489	2920	2923	2924	rBV3	1942	1141	0.05%	0.007%
54	10.556	2941	2944	2947	rBV5	1897	1402	0.06%	0.009%
55	10.659	2972	2976	2977	rBV4	1440	970	0.04%	0.006%
56	10.685	2979	2984	2986	rBV5	1643	1339	0.06%	0.008%
57	10.720	2992	2995	2997	rBV3	1907	1300	0.06%	0.008%
58	10.784	3011	3015	3017	rBV4	2187	1382	0.06%	0.008%
59	10.817	3022	3025	3027	rBV4	1949	1301	0.06%	0.008%
60	10.997	3079	3081	3084	rBV3	1813	1032	0.05%	0.006%
61	11.064	3100	3102	3104	rVB2	1325	633	0.03%	0.004%
62	11.080	3104	3107	3110	rBV5	2166	1706	0.08%	0.010%
63	11.119	3117	3119	3122	rBV4	1336	700	0.03%	0.004%
64	11.273	3155	3167	3184	rBV	1366114	2131651	95.58%	12.927%
65	11.498	3233	3237	3241	rBV6	1645	1836	0.08%	0.011%
66	11.649	3271	3284	3301	rBV	858729	1383030	62.01%	8.387%
67	11.916	3365	3367	3371	rVB4	1150	669	0.03%	0.004%
68	11.939	3371	3374	3376	rVB4	1159	721	0.03%	0.004%
69	11.955	3376	3379	3380	rBV3	1558	678	0.03%	0.004%
70	12.009	3392	3396	3397	rBV4	1515	985	0.04%	0.006%
71	12.022	3397	3400	3405	rVB6	2023	1723	0.08%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015241.D
 Acq On : 28 Mar 2020 12:45
 Operator : SY/MD
 Sample : L1975-01 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTG6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

72	12.045	3405	3407	3409	rBV3	1666	811	0.04%	0.005%
73	12.099	3419	3424	3425	rBV5	1571	1278	0.06%	0.008%
74	12.209	3456	3458	3459	rBV2	1550	852	0.04%	0.005%
75	12.228	3462	3464	3467	rVV3	1577	863	0.04%	0.005%
76	12.315	3489	3491	3495	rBV4	1507	1019	0.05%	0.006%
77	12.379	3507	3511	3512	rBV3	2118	1255	0.06%	0.008%
78	12.614	3581	3584	3585	rBV3	1420	718	0.03%	0.004%
79	12.784	3631	3637	3638	rBV6	1793	1641	0.07%	0.010%
80	12.823	3646	3649	3653	rBV4	2374	2111	0.09%	0.013%
81	12.897	3669	3672	3673	rBV3	1895	1048	0.05%	0.006%
82	13.003	3702	3705	3708	rVB5	2145	1220	0.05%	0.007%
83	13.019	3708	3710	3712	rBV3	1234	740	0.03%	0.004%
84	13.067	3722	3725	3727	rBV4	1385	824	0.04%	0.005%
85	13.080	3727	3729	3733	rVB4	2043	1615	0.07%	0.010%
86	13.106	3733	3737	3738	rBV3	1350	1113	0.05%	0.007%
87	13.177	3756	3759	3764	rVB6	1693	1494	0.07%	0.009%
88	13.244	3777	3780	3784	rBV4	2031	1629	0.07%	0.010%
89	13.286	3786	3793	3803	rVV9	7418	13944	0.63%	0.085%
90	13.421	3830	3835	3837	rBV6	2524	2151	0.10%	0.013%
91	13.627	3897	3899	3902	rBV4	1636	820	0.04%	0.005%
92	13.881	3976	3978	3981	rBV4	1719	945	0.04%	0.006%
93	13.968	4002	4005	4007	rBV4	1699	1343	0.06%	0.008%
94	14.019	4019	4021	4023	rVB2	2152	949	0.04%	0.006%
95	14.035	4023	4026	4030	rBV6	1778	1759	0.08%	0.011%
96	14.058	4030	4033	4036	rBV4	1938	1617	0.07%	0.010%
97	14.414	4139	4144	4145	rBV5	2725	1794	0.08%	0.011%
98	14.447	4151	4154	4159	rBV6	3129	2921	0.13%	0.018%
99	14.598	4198	4201	4203	rBV3	2978	1851	0.08%	0.011%
100	14.636	4210	4213	4214	rBV3	2186	1354	0.06%	0.008%


Sum of corrected areas: 16490517

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032720\
Data File : VV015241.D
Acq On : 28 Mar 2020 12:45
Operator : SY/MD
Sample : L1975-01 40X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTG6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

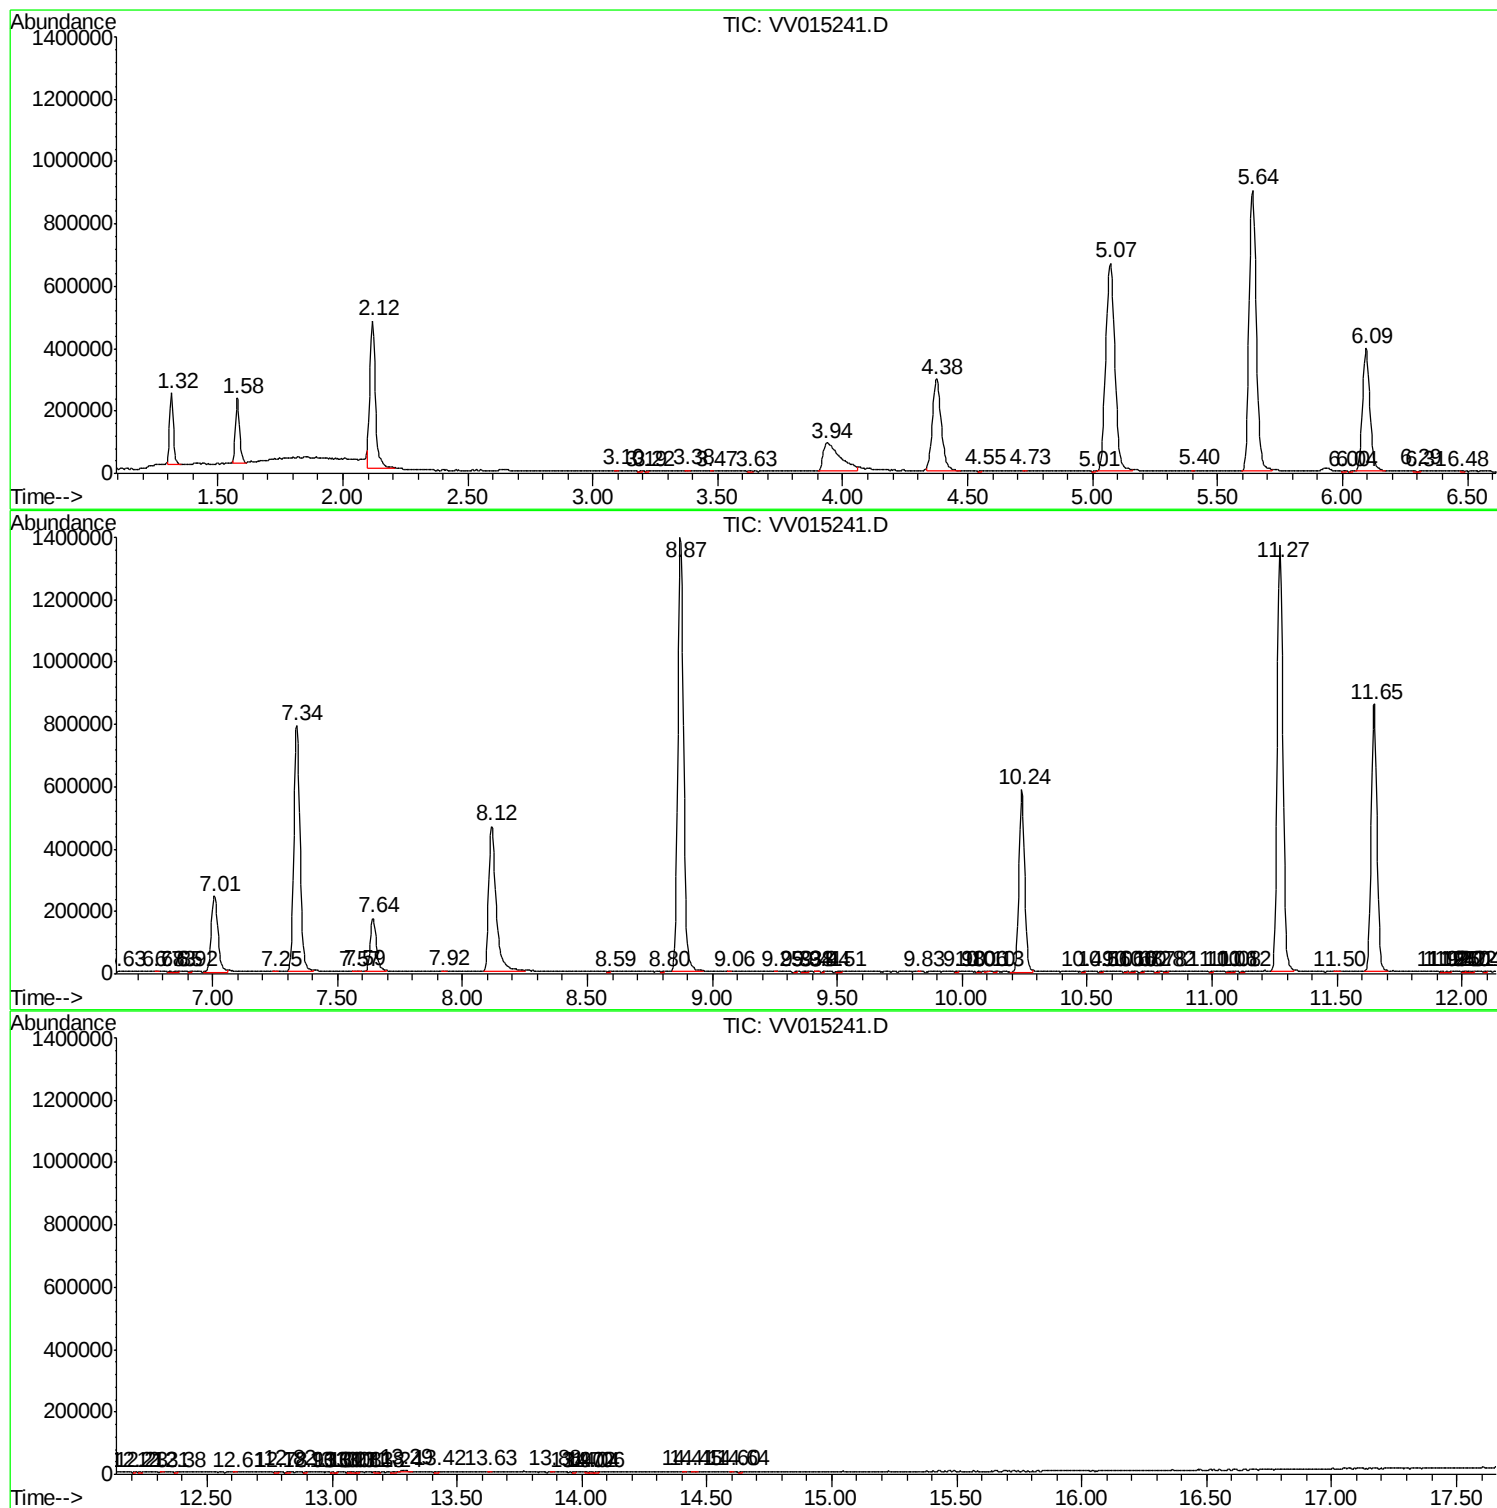

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV032720\
Data File : VV015241.D
Acq On : 28 Mar 2020 12:45
Operator : SY/MD
Sample : L1975-01 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETT66

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032720\
Data File : VV015241.D
Acq On : 28 Mar 2020 12:45
Operator : SY/MD
Sample : L1975-01 40X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
ETT66

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
