

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015242.D
 Acq On : 28 Mar 2020 13:31
 Operator : SY/MD
 Sample : L1975-02 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTG7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	65	70	78	rVB	165877	165827	14.46%	1.630%
2	1.579	146	152	161	rVB	159057	177426	15.47%	1.744%
3	2.119	314	320	331	rVB	318708	437960	38.19%	4.304%
4	2.862	548	551	554	rBV4	1863	1594	0.14%	0.016%
5	3.444	730	732	738	rVB7	2185	1203	0.10%	0.012%
6	3.579	772	774	776	rVB3	1596	507	0.04%	0.005%
7	3.592	776	778	782	rVB5	1700	793	0.07%	0.008%
8	3.634	784	791	792	rBV5	2710	2831	0.25%	0.028%
9	3.711	812	815	818	rBV4	2621	2132	0.19%	0.021%
10	3.791	838	840	842	rBV3	1255	579	0.05%	0.006%
11	3.810	843	846	849	rVB4	2121	1334	0.12%	0.013%
12	3.942	875	887	908	rBV	60137	244806	21.35%	2.406%
13	4.373	1009	1021	1046	rVB	200261	494467	43.12%	4.859%
14	4.833	1160	1164	1166	rBV5	2041	1598	0.14%	0.016%
15	4.900	1183	1185	1188	rBV4	2614	1512	0.13%	0.015%
16	5.068	1223	1237	1261	rVB2	457942	1146694	100.00%	11.268%
17	5.428	1347	1349	1353	rBV4	1876	1232	0.11%	0.012%
18	5.637	1400	1414	1438	rBV	448614	915690	79.85%	8.998%
19	6.093	1543	1556	1579	rBV2	273981	563213	49.12%	5.535%
20	6.531	1687	1692	1694	rBV6	2052	2213	0.19%	0.022%
21	6.579	1706	1707	1710	rBV3	1255	793	0.07%	0.008%
22	6.627	1719	1722	1723	rBV3	1717	794	0.07%	0.008%
23	6.826	1781	1784	1785	rBV3	1346	765	0.07%	0.008%
24	6.965	1824	1827	1829	rBV3	2928	1884	0.16%	0.019%
25	7.006	1829	1840	1860	rVV	169055	308069	26.87%	3.027%
26	7.222	1905	1907	1912	rBV5	1550	1365	0.12%	0.013%
27	7.334	1931	1942	1963	rBV	534711	937385	81.75%	9.212%
28	7.601	2021	2025	2027	rBV5	1630	1405	0.12%	0.014%
29	7.643	2028	2038	2056	rVV	115331	206465	18.01%	2.029%
30	7.916	2121	2123	2127	rBV5	1870	1614	0.14%	0.016%
31	8.116	2176	2185	2212	rBV2	308126	642352	56.02%	6.312%
32	8.350	2256	2258	2260	rBV3	1837	845	0.07%	0.008%
33	8.437	2279	2285	2288	rBV7	1856	2374	0.21%	0.023%
34	8.453	2288	2290	2293	rBV3	1417	1039	0.09%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015242.D
 Acq On : 28 Mar 2020 13:31
 Operator : SY/MD
 Sample : L1975-02 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTG7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

35	8.492	2298	2302	2305	rBV6	2131	2172	0.19%	0.021%
36	8.585	2328	2331	2334	rBV4	1989	1751	0.15%	0.017%
37	8.637	2342	2347	2350	rBV7	1664	1539	0.13%	0.015%
38	8.720	2369	2373	2374	rBV4	1161	649	0.06%	0.006%
39	8.871	2409	2420	2443	rBV	689551	1143006	99.68%	11.232%
40	9.109	2492	2494	2495	rBV2	2927	1323	0.12%	0.013%
41	9.161	2508	2510	2513	rBV4	1947	1339	0.12%	0.013%
42	9.334	2559	2564	2566	rBV6	2059	1794	0.16%	0.018%
43	9.347	2566	2568	2572	rBV5	1976	1405	0.12%	0.014%
44	9.685	2669	2673	2675	rBV4	1204	952	0.08%	0.009%
45	9.720	2680	2684	2685	rBV3	832	565	0.05%	0.006%
46	9.829	2716	2718	2721	rVB4	1567	799	0.07%	0.008%
47	9.871	2728	2731	2733	rBV4	1543	956	0.08%	0.009%
48	9.884	2733	2735	2736	rVV2	1624	628	0.05%	0.006%
49	9.948	2750	2755	2761	rBV9	3515	4758	0.41%	0.047%
50	9.993	2767	2769	2772	rBV3	1265	653	0.06%	0.006%
51	10.022	2776	2778	2781	rVV3	1310	535	0.05%	0.005%
52	10.055	2784	2788	2791	rBV5	1611	1476	0.13%	0.015%
53	10.096	2799	2801	2803	rBV3	1059	471	0.04%	0.005%
54	10.109	2803	2805	2806	rBV2	1540	683	0.06%	0.007%
55	10.193	2827	2831	2832	rBV4	2093	1343	0.12%	0.013%
56	10.238	2834	2845	2857	rVV	401341	625817	54.58%	6.150%
57	10.437	2905	2907	2910	rBV3	2013	1522	0.13%	0.015%
58	10.502	2922	2927	2930	rBV7	3074	2693	0.23%	0.026%
59	10.534	2936	2937	2939	rBV2	1001	390	0.03%	0.004%
60	10.566	2944	2947	2951	rVB5	3020	2192	0.19%	0.022%
61	10.714	2987	2993	2996	rBV7	2366	2373	0.21%	0.023%
62	10.791	3015	3017	3020	rBV4	1558	1302	0.11%	0.013%
63	10.977	3072	3075	3077	rBV4	1156	948	0.08%	0.009%
64	11.032	3089	3092	3095	rBV5	1492	1074	0.09%	0.011%
65	11.083	3105	3108	3109	rBV4	1591	972	0.08%	0.010%
66	11.270	3155	3166	3191	rVB	681825	1078956	94.09%	10.603%
67	11.646	3271	3283	3300	rBV	603021	963225	84.00%	9.465%
68	11.964	3380	3382	3384	rBV3	1750	874	0.08%	0.009%
69	12.096	3421	3423	3426	rBV4	916	666	0.06%	0.007%
70	12.135	3433	3435	3437	rBV3	1124	571	0.05%	0.006%
71	12.154	3437	3441	3444	rVV5	1738	1854	0.16%	0.018%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015242.D
 Acq On : 28 Mar 2020 13:31
 Operator : SY/MD
 Sample : L1975-02 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTG7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

72	12.183	3447	3450	3453	rVV3	1276	874	0.08%	0.009%
73	12.238	3465	3467	3469	rVB3	1738	809	0.07%	0.008%
74	12.251	3469	3471	3473	rBV3	1351	791	0.07%	0.008%
75	12.366	3502	3507	3509	rBV6	2645	2100	0.18%	0.021%
76	12.456	3531	3535	3537	rBV4	2559	2168	0.19%	0.021%
77	12.543	3560	3562	3564	rBV3	1239	633	0.06%	0.006%
78	12.604	3579	3581	3585	rVB4	1964	813	0.07%	0.008%
79	12.624	3585	3587	3589	rBV3	1604	482	0.04%	0.005%
80	12.640	3589	3592	3593	rBV3	1623	931	0.08%	0.009%
81	12.704	3609	3612	3615	rBV5	1951	1035	0.09%	0.010%
82	12.778	3633	3635	3636	rBV2	1386	495	0.04%	0.005%
83	12.820	3646	3648	3650	rBV3	1601	904	0.08%	0.009%
84	12.865	3658	3662	3663	rVB3	1114	491	0.04%	0.005%
85	12.887	3663	3669	3671	rBV5	2615	3084	0.27%	0.030%
86	13.042	3713	3717	3719	rBV5	1719	1531	0.13%	0.015%
87	13.148	3748	3750	3751	rBV2	1071	422	0.04%	0.004%
88	13.196	3763	3765	3768	rBV5	1712	1066	0.09%	0.010%
89	13.247	3777	3781	3785	rBV8	2051	1576	0.14%	0.015%
90	13.289	3786	3794	3802	rBV8	7361	13420	1.17%	0.132%
91	13.537	3863	3871	3875	rBV9	5137	7160	0.62%	0.070%
92	13.717	3924	3927	3929	rBV4	1419	690	0.06%	0.007%
93	13.746	3933	3936	3937	rBV3	1967	1210	0.11%	0.012%
94	14.054	4030	4032	4038	rBV7	1786	1514	0.13%	0.015%
95	14.173	4065	4069	4070	rBV4	2383	1458	0.13%	0.014%
96	14.231	4085	4087	4093	rBV7	1811	1808	0.16%	0.018%
97	14.296	4104	4107	4110	rBV5	2081	1343	0.12%	0.013%
98	14.398	4137	4139	4141	rBV3	1798	968	0.08%	0.010%
99	14.437	4149	4151	4153	rBV3	1849	1025	0.09%	0.010%
100	14.575	4193	4194	4196	rBV2	1506	409	0.04%	0.004%


Sum of corrected areas: 10176196

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032720\
Data File : VV015242.D
Acq On : 28 Mar 2020 13:31
Operator : SY/MD
Sample : L1975-02 40X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTG7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

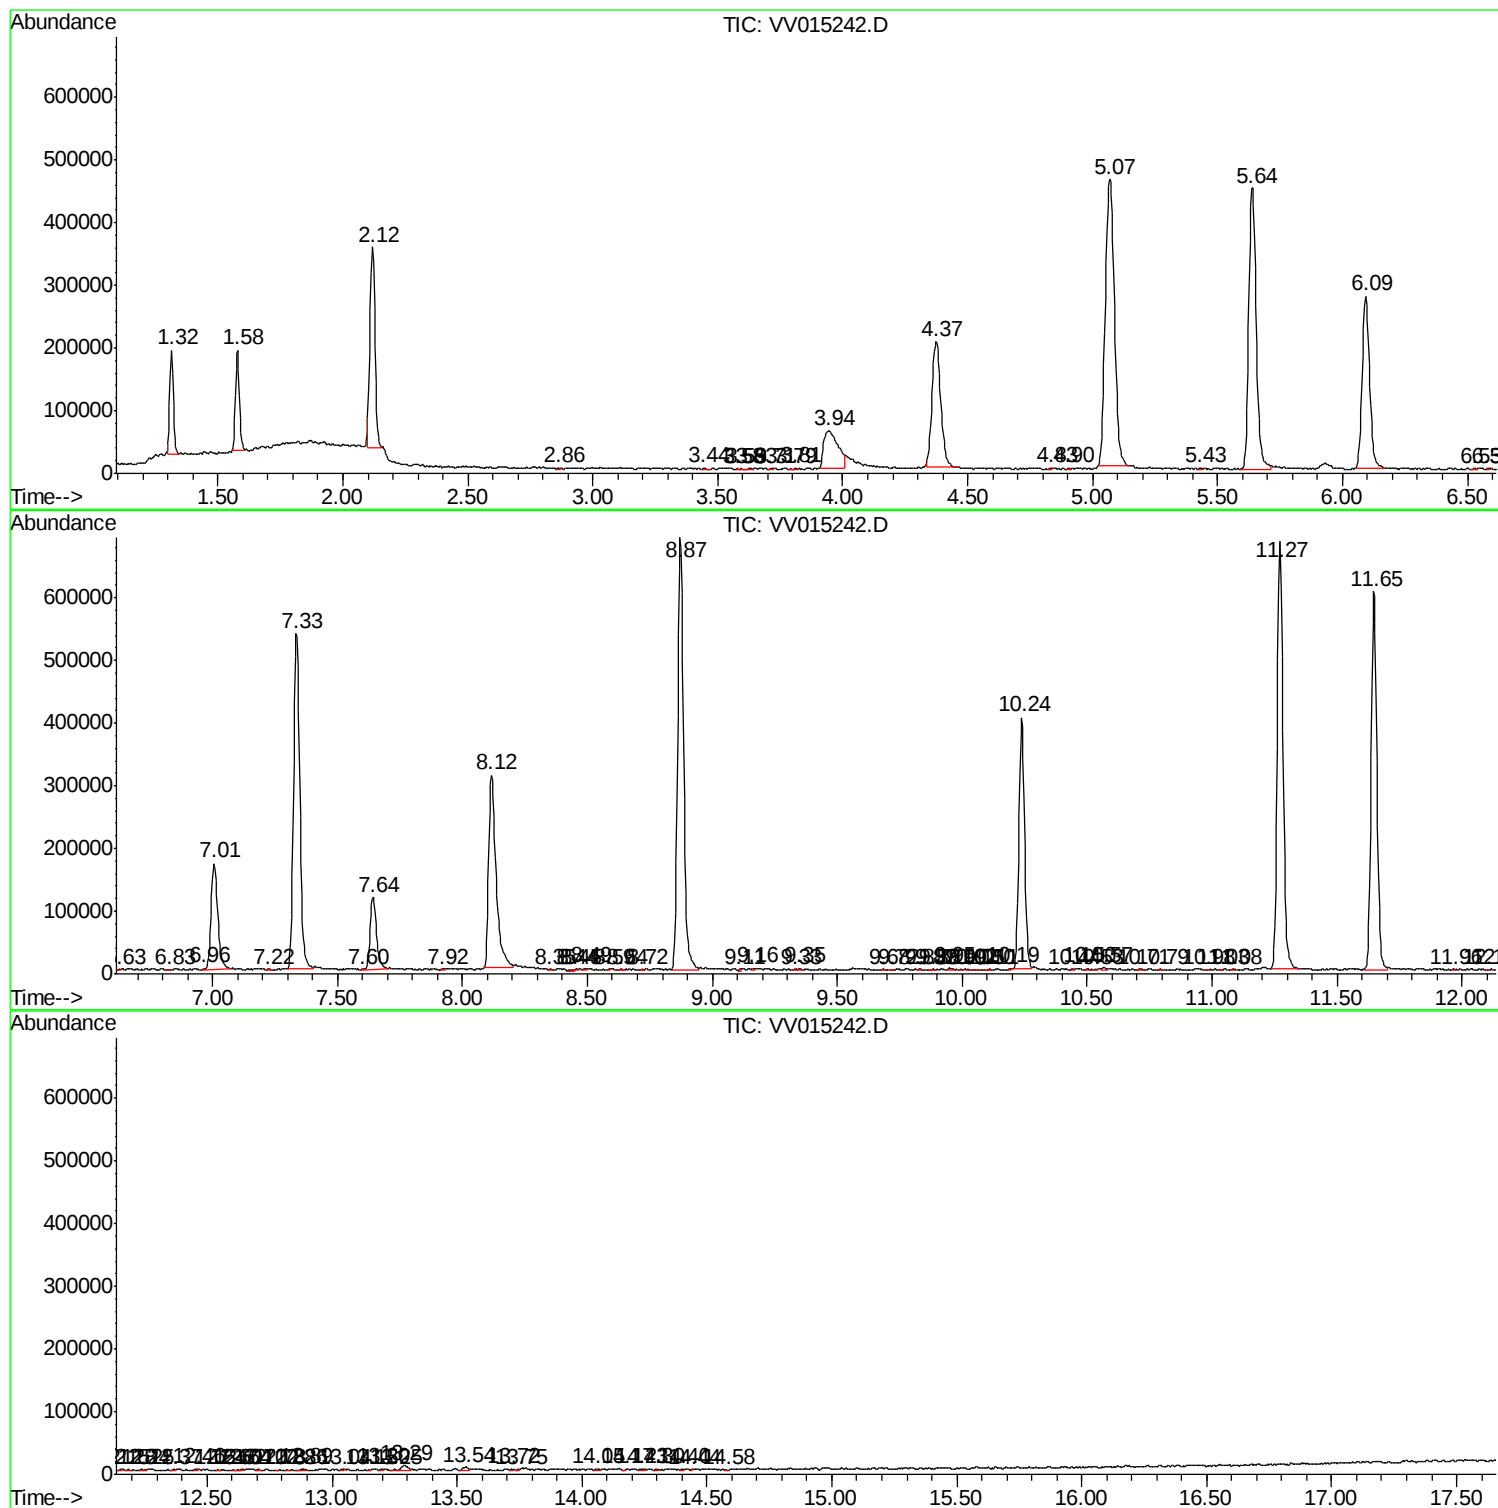

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV032720\
Data File : VV015242.D
Acq On : 28 Mar 2020 13:31
Operator : SY/MD
Sample : L1975-02 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETT67

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV032720\
Data File : VV015242.D
Acq On : 28 Mar 2020 13:31
Operator : SY/MD
Sample : L1975-02 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETT67

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc