

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015243.D
 Acq On : 28 Mar 2020 13:55
 Operator : SY/MD
 Sample : L1975-04 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTG9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	65	70	82	rVB	194874	190312	12.34%	1.539%
2	1.579	147	152	165	rVB	171887	201016	13.03%	1.625%
3	2.119	314	320	335	rVB	360607	500516	32.44%	4.047%
4	3.241	664	669	672	rBV7	2600	2340	0.15%	0.019%
5	3.627	786	789	791	rBV3	1865	1035	0.07%	0.008%
6	3.765	829	832	834	rBV4	1389	1110	0.07%	0.009%
7	3.942	874	887	922	rBV3	76324	369699	23.96%	2.989%
8	4.379	1010	1023	1047	rVB2	230921	570440	36.97%	4.612%
9	4.785	1146	1149	1151	rBV3	1676	960	0.06%	0.008%
10	4.839	1162	1166	1168	rBV3	2764	1893	0.12%	0.015%
11	4.859	1168	1172	1174	rVV4	2569	1547	0.10%	0.013%
12	4.961	1203	1204	1207	rBV3	944	421	0.03%	0.003%
13	4.981	1207	1210	1213	rVB4	1860	1121	0.07%	0.009%
14	5.016	1219	1221	1222	rBV2	1848	790	0.05%	0.006%
15	5.071	1223	1238	1272	rVB2	530660	1348464	87.40%	10.902%
16	5.640	1403	1415	1443	rBV	614279	1230684	79.77%	9.950%
17	5.884	1487	1491	1492	rBV4	1730	1255	0.08%	0.010%
18	6.096	1545	1557	1581	rVB	320052	643475	41.71%	5.202%
19	6.248	1602	1604	1607	rBV3	2424	1299	0.08%	0.011%
20	6.360	1635	1639	1644	rBV8	2162	2565	0.17%	0.021%
21	6.444	1660	1665	1666	rBV5	1523	1141	0.07%	0.009%
22	6.826	1780	1784	1786	rBV4	2399	2062	0.13%	0.017%
23	6.916	1809	1812	1815	rBV4	1907	1392	0.09%	0.011%
24	7.010	1831	1841	1859	rVB	185899	332914	21.58%	2.692%
25	7.193	1895	1898	1899	rBV3	1849	1312	0.09%	0.011%
26	7.264	1918	1920	1921	rBV2	1765	734	0.05%	0.006%
27	7.338	1931	1943	1965	rBV	622972	1072128	69.49%	8.668%
28	7.643	2029	2038	2059	rVB	134491	231758	15.02%	1.874%
29	7.804	2086	2088	2089	rBV2	1727	629	0.04%	0.005%
30	7.968	2137	2139	2141	rBV3	1570	693	0.04%	0.006%
31	8.064	2167	2169	2172	rBV3	2109	1371	0.09%	0.011%
32	8.119	2176	2186	2212	rVV2	378230	790587	51.24%	6.392%
33	8.640	2345	2348	2351	rBV5	1464	928	0.06%	0.008%
34	8.701	2365	2367	2369	rBV3	929	518	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015243.D
 Acq On : 28 Mar 2020 13:55
 Operator : SY/MD
 Sample : L1975-04 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTG9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

35	8.874	2409	2421	2446	rBV	936761	1542831	100.00%	12.473%
36	9.087	2483	2487	2489	rBV4	2533	2018	0.13%	0.016%
37	9.524	2620	2623	2626	rBV5	1717	1129	0.07%	0.009%
38	9.755	2693	2695	2700	rVB5	2060	1389	0.09%	0.011%
39	9.778	2700	2702	2707	rVB6	1718	831	0.05%	0.007%
40	9.807	2707	2711	2718	rBV8	1731	2191	0.14%	0.018%
41	9.842	2721	2722	2724	rBV2	997	523	0.03%	0.004%
42	9.939	2750	2752	2754	rBV3	1310	702	0.05%	0.006%
43	10.099	2801	2802	2805	rBV3	741	533	0.03%	0.004%
44	10.122	2808	2809	2811	rVB2	1481	495	0.03%	0.004%
45	10.141	2811	2815	2818	rBV6	1351	1158	0.08%	0.009%
46	10.186	2826	2829	2830	rBV3	2210	1094	0.07%	0.009%
47	10.241	2834	2846	2861	rVV	466928	743316	48.18%	6.010%
48	10.440	2906	2908	2911	rBV4	1889	992	0.06%	0.008%
49	10.492	2921	2924	2926	rVB4	1655	731	0.05%	0.006%
50	10.591	2952	2955	2956	rBV3	1740	975	0.06%	0.008%
51	10.646	2969	2972	2974	rVB4	1960	1106	0.07%	0.009%
52	10.662	2975	2977	2980	rBV4	1248	555	0.04%	0.004%
53	10.678	2980	2982	2983	rBV2	1112	373	0.02%	0.003%
54	11.038	3091	3094	3097	rVB4	1372	907	0.06%	0.007%
55	11.202	3139	3145	3147	rBV6	4499	4220	0.27%	0.034%
56	11.273	3155	3167	3183	rBV	929542	1428956	92.62%	11.553%
57	11.553	3250	3254	3255	rBV3	1840	1398	0.09%	0.011%
58	11.649	3272	3284	3303	rBV	681373	1090383	70.67%	8.816%
59	12.016	3395	3398	3401	rBV3	1817	1449	0.09%	0.012%
60	12.141	3434	3437	3439	rBV4	1506	924	0.06%	0.007%
61	12.437	3527	3529	3530	rBV2	1499	644	0.04%	0.005%
62	12.492	3544	3546	3547	rBV2	1677	635	0.04%	0.005%
63	12.652	3593	3596	3599	rBV5	2073	1746	0.11%	0.014%
64	12.701	3609	3611	3613	rVV3	1539	532	0.03%	0.004%
65	12.710	3613	3614	3616	rVB2	1465	464	0.03%	0.004%
66	12.804	3642	3643	3644	rBV	1678	629	0.04%	0.005%
67	12.900	3671	3673	3676	rBV4	1981	909	0.06%	0.007%
68	13.029	3712	3713	3716	rBV3	1147	805	0.05%	0.007%
69	13.144	3746	3749	3752	rBV4	1919	1382	0.09%	0.011%
70	13.344	3807	3811	3812	rBV3	1356	1015	0.07%	0.008%
71	13.379	3820	3822	3828	rVB6	3076	2401	0.16%	0.019%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
Data File : VV015243.D
Acq On : 28 Mar 2020 13:55
Operator : SY/MD
Sample : L1975-04 40X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTG9

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Title : VOC Analysis

72	13.411	3828	3832	3836	rBV6	1826	1760	0.11%	0.014%
73	13.431	3836	3838	3840	rBV2	2177	1099	0.07%	0.009%
74	13.681	3913	3916	3920	rBV6	2502	2271	0.15%	0.018%
75	13.868	3972	3974	3975	rBV2	1336	589	0.04%	0.005%
76	14.035	4023	4026	4028	rBV3	2216	1187	0.08%	0.010%
77	14.222	4081	4084	4088	rBV5	2075	2231	0.14%	0.018%
78	14.369	4127	4130	4135	rVB7	2711	2266	0.15%	0.018%
79	14.617	4203	4207	4210	rBV6	2976	3035	0.20%	0.025%
80	15.212	4388	4392	4396	rBV6	3071	3020	0.20%	0.024%


Sum of corrected areas: 12368908

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032720\
Data File : VV015243.D
Acq On : 28 Mar 2020 13:55
Operator : SY/MD
Sample : L1975-04 40X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTG9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

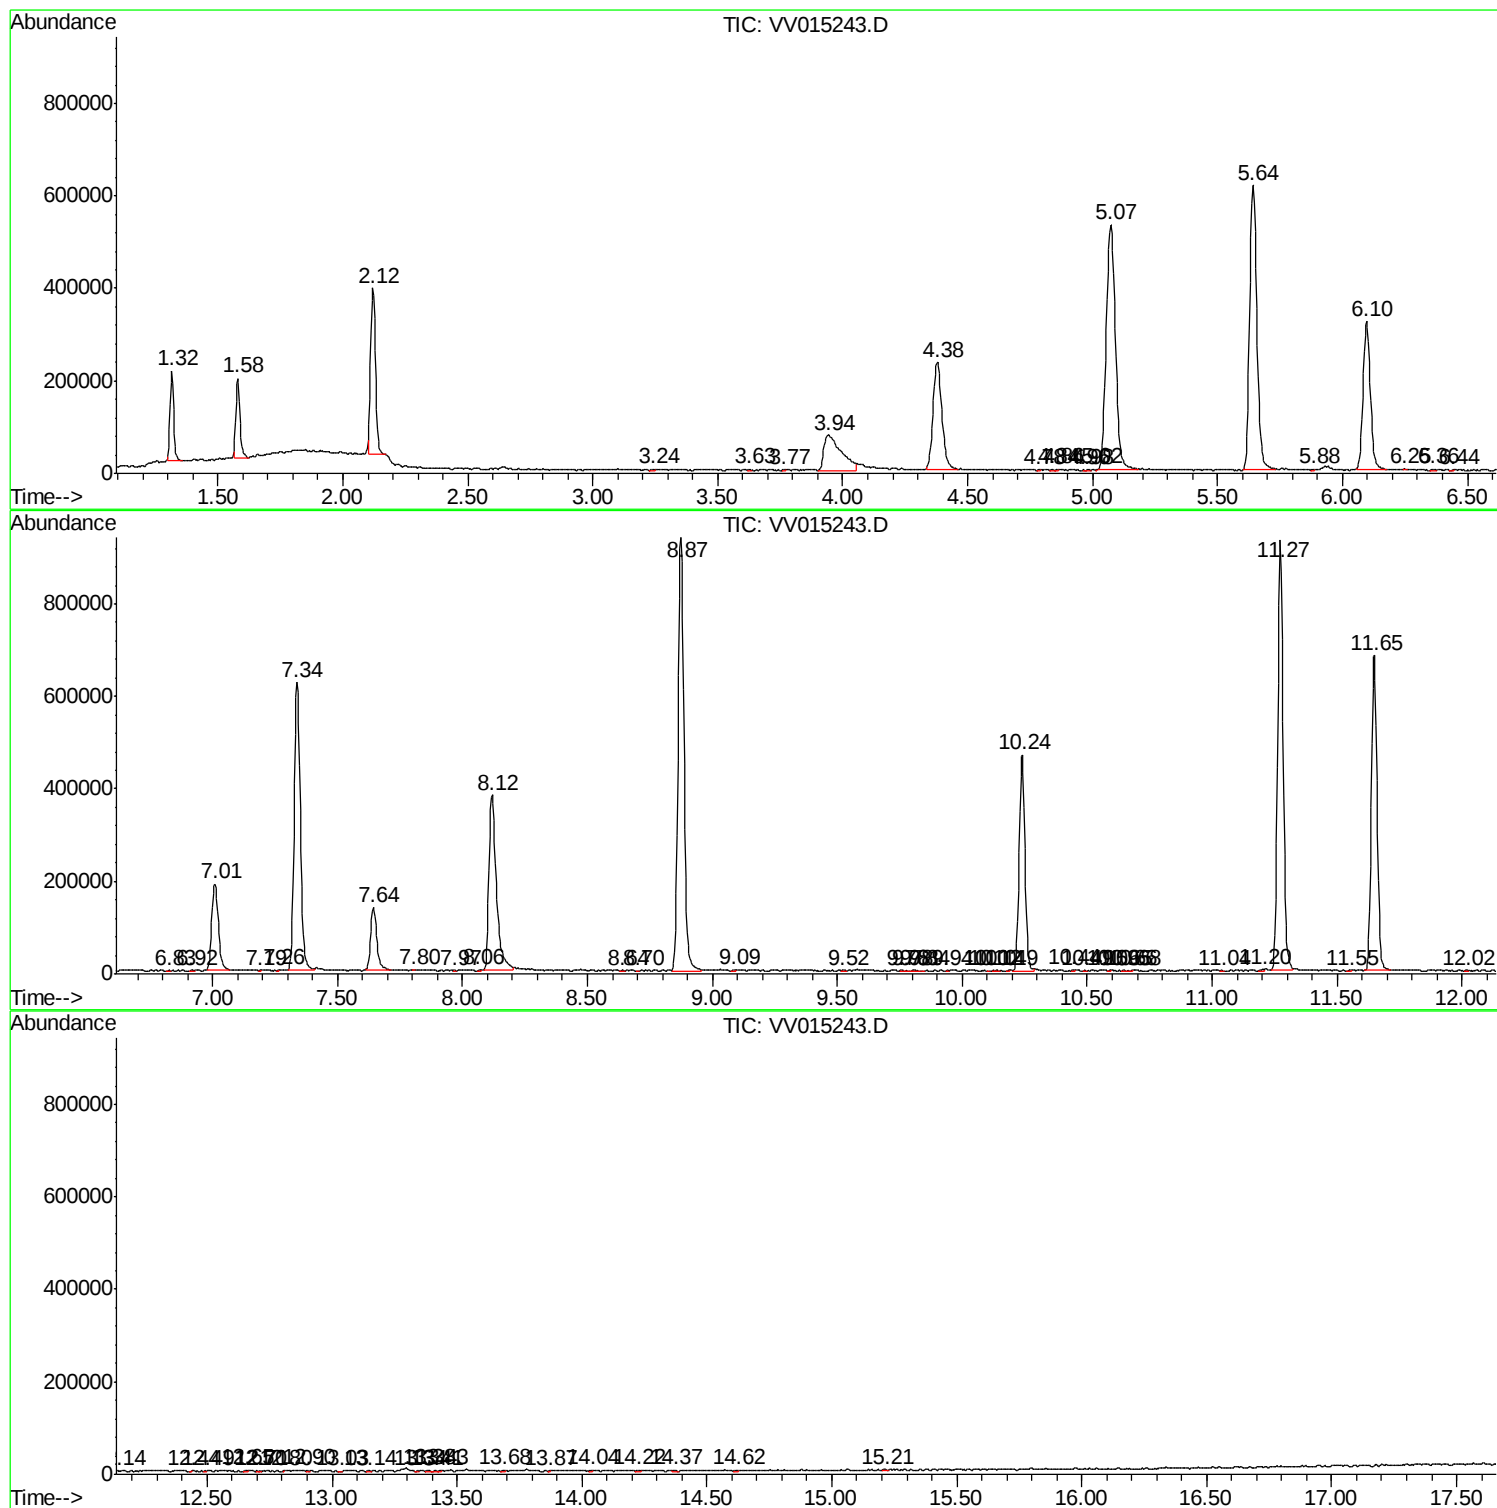

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV032720\
Data File : VV015243.D
Acq On : 28 Mar 2020 13:55
Operator : SY/MD
Sample : L1975-04 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETT9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032720\
Data File : VV015243.D
Acq On : 28 Mar 2020 13:55
Operator : SY/MD
Sample : L1975-04 40X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
ETT9

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc