

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015244.D
 Acq On : 28 Mar 2020 14:19
 Operator : SY/MD
 Sample : L1975-07 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTH2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	65	70	81	rVB	157885	157587	9.38%	1.482%
2	1.579	147	152	165	rVB	133881	153326	9.13%	1.441%
3	3.155	638	642	645	rBV4	2308	1913	0.11%	0.018%
4	3.222	660	663	664	rBV2	1651	1001	0.06%	0.009%
5	3.283	679	682	686	rBV5	2392	2027	0.12%	0.019%
6	3.299	686	687	692	rVV5	1867	1283	0.08%	0.012%
7	3.357	702	705	708	rBV4	1510	912	0.05%	0.009%
8	3.457	733	736	742	rVB6	2609	2315	0.14%	0.022%
9	3.531	754	759	763	rBV9	2106	2249	0.13%	0.021%
10	3.557	763	767	772	rBV7	1605	2062	0.12%	0.019%
11	3.634	789	791	794	rBV3	1876	1027	0.06%	0.010%
12	3.717	813	817	820	rBV6	3268	1981	0.12%	0.019%
13	3.881	862	868	869	rBV4	1789	1712	0.10%	0.016%
14	3.946	875	888	916	rBV3	62024	274882	16.37%	2.584%
15	4.380	1010	1023	1044	rVB3	176276	437090	26.02%	4.109%
16	4.659	1107	1110	1112	rBV4	1743	1116	0.07%	0.010%
17	4.798	1149	1153	1156	rBV5	2421	1752	0.10%	0.016%
18	4.833	1160	1164	1165	rBV3	1328	954	0.06%	0.009%
19	4.913	1185	1189	1191	rBV3	1982	1130	0.07%	0.011%
20	4.929	1191	1194	1197	rBV4	1671	1132	0.07%	0.011%
21	5.074	1220	1239	1262	rBV3	419532	1060861	63.16%	9.973%
22	5.447	1352	1355	1356	rBV3	2229	1215	0.07%	0.011%
23	5.643	1402	1416	1437	rBV	671147	1342028	79.90%	12.617%
24	6.010	1528	1530	1533	rVB3	2240	915	0.05%	0.009%
25	6.048	1537	1542	1543	rBV4	2091	1453	0.09%	0.014%
26	6.097	1544	1557	1578	rBV	244573	506926	30.18%	4.766%
27	6.296	1617	1619	1623	rBV5	1889	1563	0.09%	0.015%
28	6.527	1687	1691	1693	rBV5	1295	1055	0.06%	0.010%
29	6.685	1736	1740	1742	rBV4	3653	2713	0.16%	0.026%
30	6.736	1754	1756	1759	rVV4	1370	836	0.05%	0.008%
31	6.862	1793	1795	1800	rBV5	1531	1339	0.08%	0.013%
32	7.010	1830	1841	1861	rBV2	146423	268352	15.98%	2.523%
33	7.177	1891	1893	1897	rBV4	1907	1324	0.08%	0.012%
34	7.219	1903	1906	1908	rBV4	1499	873	0.05%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015244.D
 Acq On : 28 Mar 2020 14:19
 Operator : SY/MD
 Sample : L1975-07 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTH2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

35	7.338	1931	1943	1962	rVV	477285	837813	49.88%	7.877%
36	7.505	1992	1995	1998	rVB5	1763	1124	0.07%	0.011%
37	7.601	2022	2025	2029	rBV5	1485	1536	0.09%	0.014%
38	7.643	2029	2038	2059	rVV2	103412	182120	10.84%	1.712%
39	7.807	2086	2089	2092	rBV4	2257	1375	0.08%	0.013%
40	7.952	2130	2134	2135	rBV3	1952	1307	0.08%	0.012%
41	8.003	2148	2150	2157	rVB7	2612	2477	0.15%	0.023%
42	8.119	2174	2186	2211	rBV2	300588	627156	37.34%	5.896%
43	8.752	2381	2383	2387	rVB5	2782	1440	0.09%	0.014%
44	8.785	2387	2393	2397	rVB6	2424	2535	0.15%	0.024%
45	8.820	2401	2404	2407	rBV5	2065	1768	0.11%	0.017%
46	8.875	2407	2421	2443	rBV	1025896	1679623	100.00%	15.791%
47	9.093	2483	2489	2493	rBV8	2625	2963	0.18%	0.028%
48	9.122	2494	2498	2502	rVV7	2649	2258	0.13%	0.021%
49	9.322	2558	2560	2564	rBV5	1746	1372	0.08%	0.013%
50	9.357	2567	2571	2575	rBV6	1937	1528	0.09%	0.014%
51	9.415	2586	2589	2599	rVB10	2000	2328	0.14%	0.022%
52	9.460	2599	2603	2605	rBV4	2190	1790	0.11%	0.017%
53	9.550	2629	2631	2633	rBV3	1331	915	0.05%	0.009%
54	9.820	2711	2715	2718	rVB5	2589	2082	0.12%	0.020%
55	9.852	2721	2725	2726	rBV4	1821	1221	0.07%	0.011%
56	9.862	2726	2728	2733	rVB6	1724	1057	0.06%	0.010%
57	9.904	2738	2741	2745	rVB5	2408	1846	0.11%	0.017%
58	9.942	2745	2753	2755	rBV8	2285	3520	0.21%	0.033%
59	10.029	2778	2780	2783	rVB3	2337	905	0.05%	0.009%
60	10.051	2783	2787	2790	rBV5	1794	2033	0.12%	0.019%
61	10.145	2810	2816	2821	rBV9	1967	2175	0.13%	0.020%
62	10.170	2821	2824	2829	rBV6	2101	1942	0.12%	0.018%
63	10.238	2833	2845	2858	rBV	366639	577793	34.40%	5.432%
64	10.402	2894	2896	2898	rBV3	1500	909	0.05%	0.009%
65	10.469	2915	2917	2923	rVB5	2925	2022	0.12%	0.019%
66	10.498	2923	2926	2927	rBV3	1826	1097	0.07%	0.010%
67	10.756	3002	3006	3007	rBV4	1756	1075	0.06%	0.010%
68	10.794	3015	3018	3020	rBV4	1427	810	0.05%	0.008%
69	10.858	3036	3038	3043	rVB5	1359	932	0.06%	0.009%
70	11.068	3100	3103	3105	rBV4	1519	886	0.05%	0.008%
71	11.080	3105	3107	3113	rVB7	2304	2113	0.13%	0.020%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015244.D
 Acq On : 28 Mar 2020 14:19
 Operator : SY/MD
 Sample : L1975-07 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTH2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

72	11.106	3113	3115	3119	rBV5	3186	2283	0.14%	0.021%
73	11.273	3155	3167	3186	rBV	996302	1552461	92.43%	14.595%
74	11.534	3244	3248	3253	rBV8	1336	1657	0.10%	0.016%
75	11.563	3253	3257	3260	rBV6	1914	1829	0.11%	0.017%
76	11.608	3267	3271	3272	rBV4	2026	1222	0.07%	0.011%
77	11.649	3272	3284	3300	rVV	525191	842776	50.18%	7.923%
78	11.862	3347	3350	3353	rBV5	1815	1143	0.07%	0.011%
79	11.884	3353	3357	3363	rVB8	2816	3008	0.18%	0.028%
80	11.910	3363	3365	3370	rBV5	1867	1195	0.07%	0.011%
81	11.936	3370	3373	3375	rBV4	1935	1531	0.09%	0.014%
82	11.984	3385	3388	3390	rBV3	2086	1324	0.08%	0.012%
83	12.064	3409	3413	3414	rBV4	1850	1157	0.07%	0.011%
84	12.254	3470	3472	3474	rBV3	1643	1024	0.06%	0.010%
85	12.370	3505	3508	3510	rBV5	1588	1087	0.06%	0.010%
86	12.479	3539	3542	3546	rVB5	2462	1789	0.11%	0.017%
87	12.502	3546	3549	3551	rBV4	1623	888	0.05%	0.008%
88	12.563	3565	3568	3570	rBV4	1668	859	0.05%	0.008%
89	12.772	3629	3633	3634	rBV3	1843	1275	0.08%	0.012%
90	12.926	3678	3681	3684	rBV5	2149	1195	0.07%	0.011%
91	13.061	3719	3723	3731	rBV5	2709	4154	0.25%	0.039%
92	13.103	3732	3736	3738	rVV4	1944	1336	0.08%	0.013%
93	13.186	3759	3762	3764	rBV4	1690	872	0.05%	0.008%
94	13.694	3917	3920	3923	rBV4	2753	2434	0.14%	0.023%
95	13.746	3932	3936	3939	rBV6	1481	1301	0.08%	0.012%
96	13.775	3939	3945	3946	rBV5	3697	3390	0.20%	0.032%
97	13.820	3955	3959	3961	rBV5	2198	1693	0.10%	0.016%
98	14.038	4024	4027	4030	rBV3	1945	1630	0.10%	0.015%
99	14.090	4041	4043	4045	rBV3	1736	994	0.06%	0.009%
100	14.135	4053	4057	4062	rBV7	2242	2573	0.15%	0.024%


Sum of corrected areas: 10636830

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032720\
Data File : VV015244.D
Acq On : 28 Mar 2020 14:19
Operator : SY/MD
Sample : L1975-07 40X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTH2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

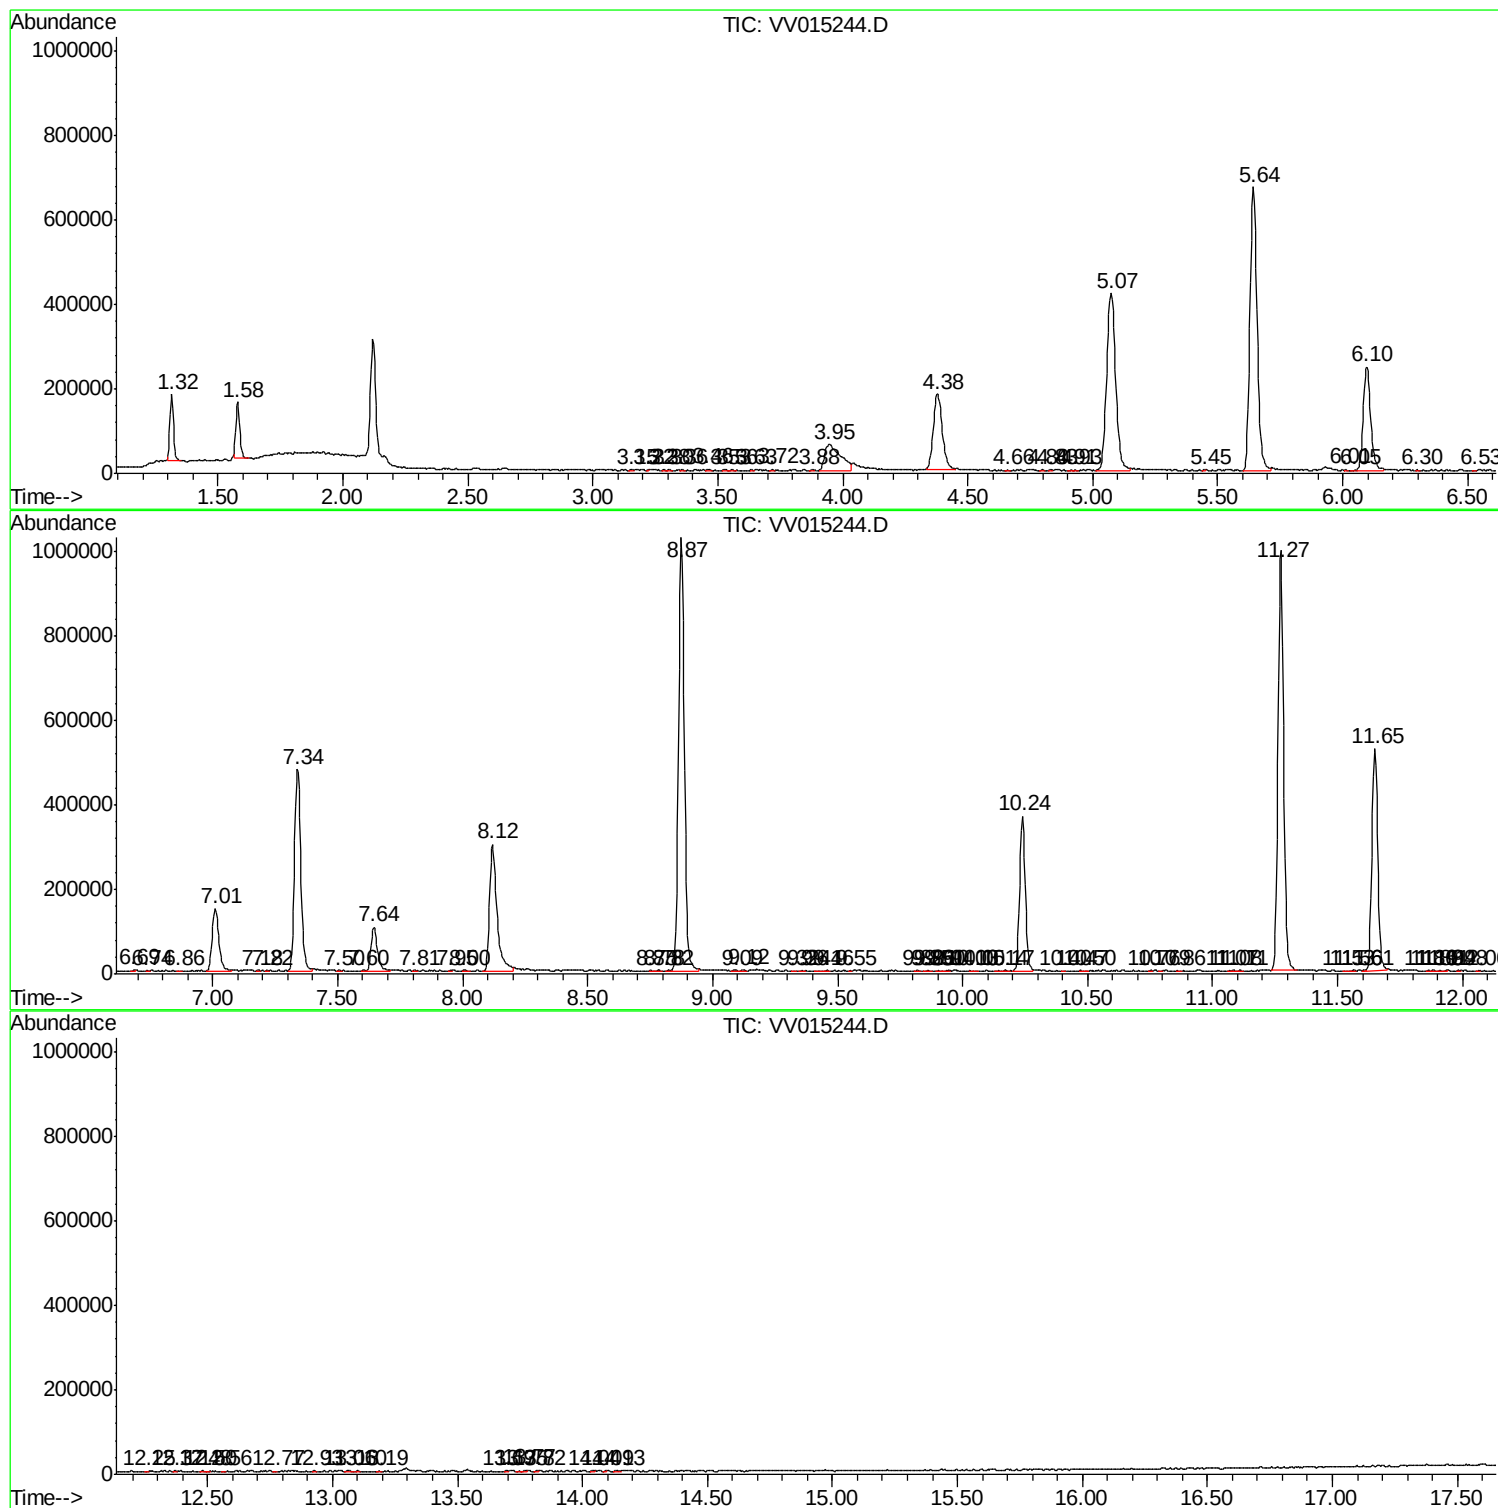

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV032720\
Data File : VV015244.D
Acq On : 28 Mar 2020 14:19
Operator : SY/MD
Sample : L1975-07 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTH2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032720\
Data File : VV015244.D
Acq On : 28 Mar 2020 14:19
Operator : SY/MD
Sample : L1975-07 40X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
ETTH2

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
