

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015245.D
 Acq On : 28 Mar 2020 14:44
 Operator : SY/MD
 Sample : L1975-13 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTH6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	83	rVB	215239	227923	12.09%	1.549%
2	1.579	146	152	165	rVB	193805	226053	11.99%	1.536%
3	2.119	314	320	347	rVB	427381	660761	35.06%	4.490%
4	3.045	606	608	613	rBV6	1630	1099	0.06%	0.007%
5	3.100	623	625	628	rVB3	1677	760	0.04%	0.005%
6	3.116	628	630	633	rBV4	1791	845	0.04%	0.006%
7	3.229	662	665	668	rBV5	2002	1436	0.08%	0.010%
8	3.415	720	723	728	rVB7	3063	2676	0.14%	0.018%
9	3.447	728	733	736	rBV5	2171	1959	0.10%	0.013%
10	3.470	736	740	742	rBV4	1569	1320	0.07%	0.009%
11	3.521	753	756	757	rBV3	1647	970	0.05%	0.007%
12	3.730	819	821	824	rBV4	2391	1241	0.07%	0.008%
13	3.856	857	860	866	rBV8	1518	1732	0.09%	0.012%
14	3.939	874	886	928	rBV2	92543	417150	22.13%	2.834%
15	4.380	1008	1023	1047	rVB	266726	660255	35.03%	4.486%
16	4.711	1123	1126	1127	rBV3	1857	981	0.05%	0.007%
17	4.746	1134	1137	1140	rBV5	1845	1196	0.06%	0.008%
18	4.843	1165	1167	1171	rVB4	1938	932	0.05%	0.006%
19	4.865	1171	1174	1175	rBV3	1456	903	0.05%	0.006%
20	4.917	1188	1190	1194	rBV4	1251	885	0.05%	0.006%
21	5.074	1222	1239	1265	rBV2	612844	1543106	81.87%	10.485%
22	5.344	1320	1323	1330	rBV7	2143	2227	0.12%	0.015%
23	5.640	1401	1415	1442	rBV	748006	1518407	80.56%	10.317%
24	5.865	1483	1485	1489	rBV4	2098	1323	0.07%	0.009%
25	5.888	1489	1492	1495	rBV4	1464	1255	0.07%	0.009%
26	6.019	1528	1533	1537	rBV7	1836	1657	0.09%	0.011%
27	6.097	1543	1557	1580	rBV	365735	751121	39.85%	5.104%
28	6.479	1673	1676	1681	rVB7	1132	954	0.05%	0.006%
29	6.521	1682	1689	1690	rBV6	1634	1657	0.09%	0.011%
30	6.640	1722	1726	1728	rBV5	2511	1527	0.08%	0.010%
31	6.711	1746	1748	1751	rBV3	1855	1251	0.07%	0.009%
32	7.010	1830	1841	1862	rBV	221050	391938	20.79%	2.663%
33	7.180	1892	1894	1897	rBV3	1481	859	0.05%	0.006%
34	7.338	1930	1943	1963	rBV	718384	1244686	66.04%	8.457%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015245.D
 Acq On : 28 Mar 2020 14:44
 Operator : SY/MD
 Sample : L1975-13 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTH6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

35	7.543	2004	2007	2009	rBV4	1706	1299	0.07%	0.009%
36	7.643	2028	2038	2053	rBV	154389	265332	14.08%	1.803%
37	7.778	2076	2080	2081	rBV3	1965	1340	0.07%	0.009%
38	7.987	2142	2145	2149	rBV5	3046	2870	0.15%	0.020%
39	8.058	2163	2167	2172	rBV8	1767	1425	0.08%	0.010%
40	8.116	2174	2185	2220	rBV2	449907	948150	50.30%	6.443%
41	8.469	2293	2295	2299	rVB4	1843	1109	0.06%	0.008%
42	8.650	2348	2351	2353	rVB3	1390	800	0.04%	0.005%
43	8.875	2408	2421	2440	rBV	1158543	1884816	100.00%	12.807%
44	9.238	2532	2534	2538	rBV5	1423	1113	0.06%	0.008%
45	9.341	2561	2566	2567	rBV6	1573	1061	0.06%	0.007%
46	9.373	2573	2576	2581	rBV7	1934	1807	0.10%	0.012%
47	9.412	2585	2588	2591	rBV5	2261	1585	0.08%	0.011%
48	9.495	2612	2614	2616	rBV3	1449	812	0.04%	0.006%
49	9.633	2654	2657	2660	rBV4	1269	832	0.04%	0.006%
50	9.649	2660	2662	2667	rVB6	1218	1057	0.06%	0.007%
51	9.820	2711	2715	2718	rBV5	1600	1348	0.07%	0.009%
52	9.916	2743	2745	2750	rVB6	1452	1082	0.06%	0.007%
53	9.952	2750	2756	2757	rBV6	3273	2985	0.16%	0.020%
54	10.010	2771	2774	2775	rBV3	1987	998	0.05%	0.007%
55	10.071	2790	2793	2796	rBV4	1355	868	0.05%	0.006%
56	10.132	2810	2812	2816	rVB5	1541	1014	0.05%	0.007%
57	10.154	2816	2819	2821	rBV3	2234	1447	0.08%	0.010%
58	10.238	2834	2845	2862	rVV	539108	857839	45.51%	5.829%
59	10.402	2892	2896	2900	rBV7	2197	1874	0.10%	0.013%
60	10.489	2918	2923	2925	rBV5	1352	1372	0.07%	0.009%
61	10.604	2954	2959	2962	rBV7	1137	1425	0.08%	0.010%
62	10.633	2966	2968	2973	rVB4	1384	888	0.05%	0.006%
63	10.759	3004	3007	3012	rVB6	1834	1412	0.07%	0.010%
64	10.846	3028	3034	3036	rBV6	1789	1479	0.08%	0.010%
65	10.900	3049	3051	3053	rBV3	1994	978	0.05%	0.007%
66	11.273	3155	3167	3190	rBV	1122463	1749859	92.84%	11.890%
67	11.482	3230	3232	3235	rBV4	1517	994	0.05%	0.007%
68	11.498	3235	3237	3239	rVV4	2184	993	0.05%	0.007%
69	11.518	3241	3243	3247	rVB4	2427	1366	0.07%	0.009%
70	11.566	3254	3258	3259	rBV4	1383	938	0.05%	0.006%
71	11.649	3271	3284	3301	rBV	781229	1244310	66.02%	8.455%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015245.D
 Acq On : 28 Mar 2020 14:44
 Operator : SY/MD
 Sample : L1975-13 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTH6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

72	11.977	3382	3386	3390	rVB7	2061	1806	0.10%	0.012%
73	11.993	3390	3391	3395	rBV4	1350	1176	0.06%	0.008%
74	12.109	3423	3427	3430	rBV6	1488	1649	0.09%	0.011%
75	12.151	3435	3440	3444	rBV8	2155	2315	0.12%	0.016%
76	12.228	3462	3464	3466	rVB3	1756	752	0.04%	0.005%
77	12.241	3466	3468	3470	rBV3	1584	970	0.05%	0.007%
78	12.289	3477	3483	3485	rBV6	2190	2271	0.12%	0.015%
79	12.318	3490	3492	3494	rBV3	1872	808	0.04%	0.005%
80	12.399	3512	3517	3521	rBV8	2630	2626	0.14%	0.018%
81	12.569	3568	3570	3572	rVB3	1934	759	0.04%	0.005%
82	12.582	3572	3574	3577	rBV4	2272	1503	0.08%	0.010%
83	12.682	3600	3605	3607	rBV5	2304	2043	0.11%	0.014%
84	12.810	3638	3645	3646	rBV7	1930	2104	0.11%	0.014%
85	12.820	3646	3648	3650	rBV3	1377	857	0.05%	0.006%
86	12.939	3683	3685	3689	rBV5	1761	1362	0.07%	0.009%
87	13.029	3711	3713	3721	rBV8	1393	1583	0.08%	0.011%
88	13.190	3759	3763	3767	rBV6	2023	1792	0.10%	0.012%
89	13.260	3782	3785	3786	rBV3	1480	885	0.05%	0.006%
90	13.286	3790	3793	3803	rVB10	7375	9827	0.52%	0.067%
91	13.421	3831	3835	3838	rBV4	1828	1834	0.10%	0.012%
92	13.456	3842	3846	3848	rBV4	1673	1226	0.07%	0.008%
93	13.498	3856	3859	3861	rBV4	1934	1058	0.06%	0.007%
94	13.582	3881	3885	3886	rBV4	2673	1604	0.09%	0.011%
95	13.855	3965	3970	3972	rBV6	2695	2238	0.12%	0.015%
96	13.913	3985	3988	3989	rBV3	2035	1211	0.06%	0.008%
97	13.942	3994	3997	4000	rBV5	1633	1217	0.06%	0.008%
98	14.038	4024	4027	4030	rBV4	1652	1100	0.06%	0.007%
99	14.524	4171	4178	4180	rBV6	3442	3613	0.19%	0.025%
100	14.726	4239	4241	4244	rBV4	1864	966	0.05%	0.007%


Sum of corrected areas: 14717077

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032720\
Data File : VV015245.D
Acq On : 28 Mar 2020 14:44
Operator : SY/MD
Sample : L1975-13 40X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTH6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

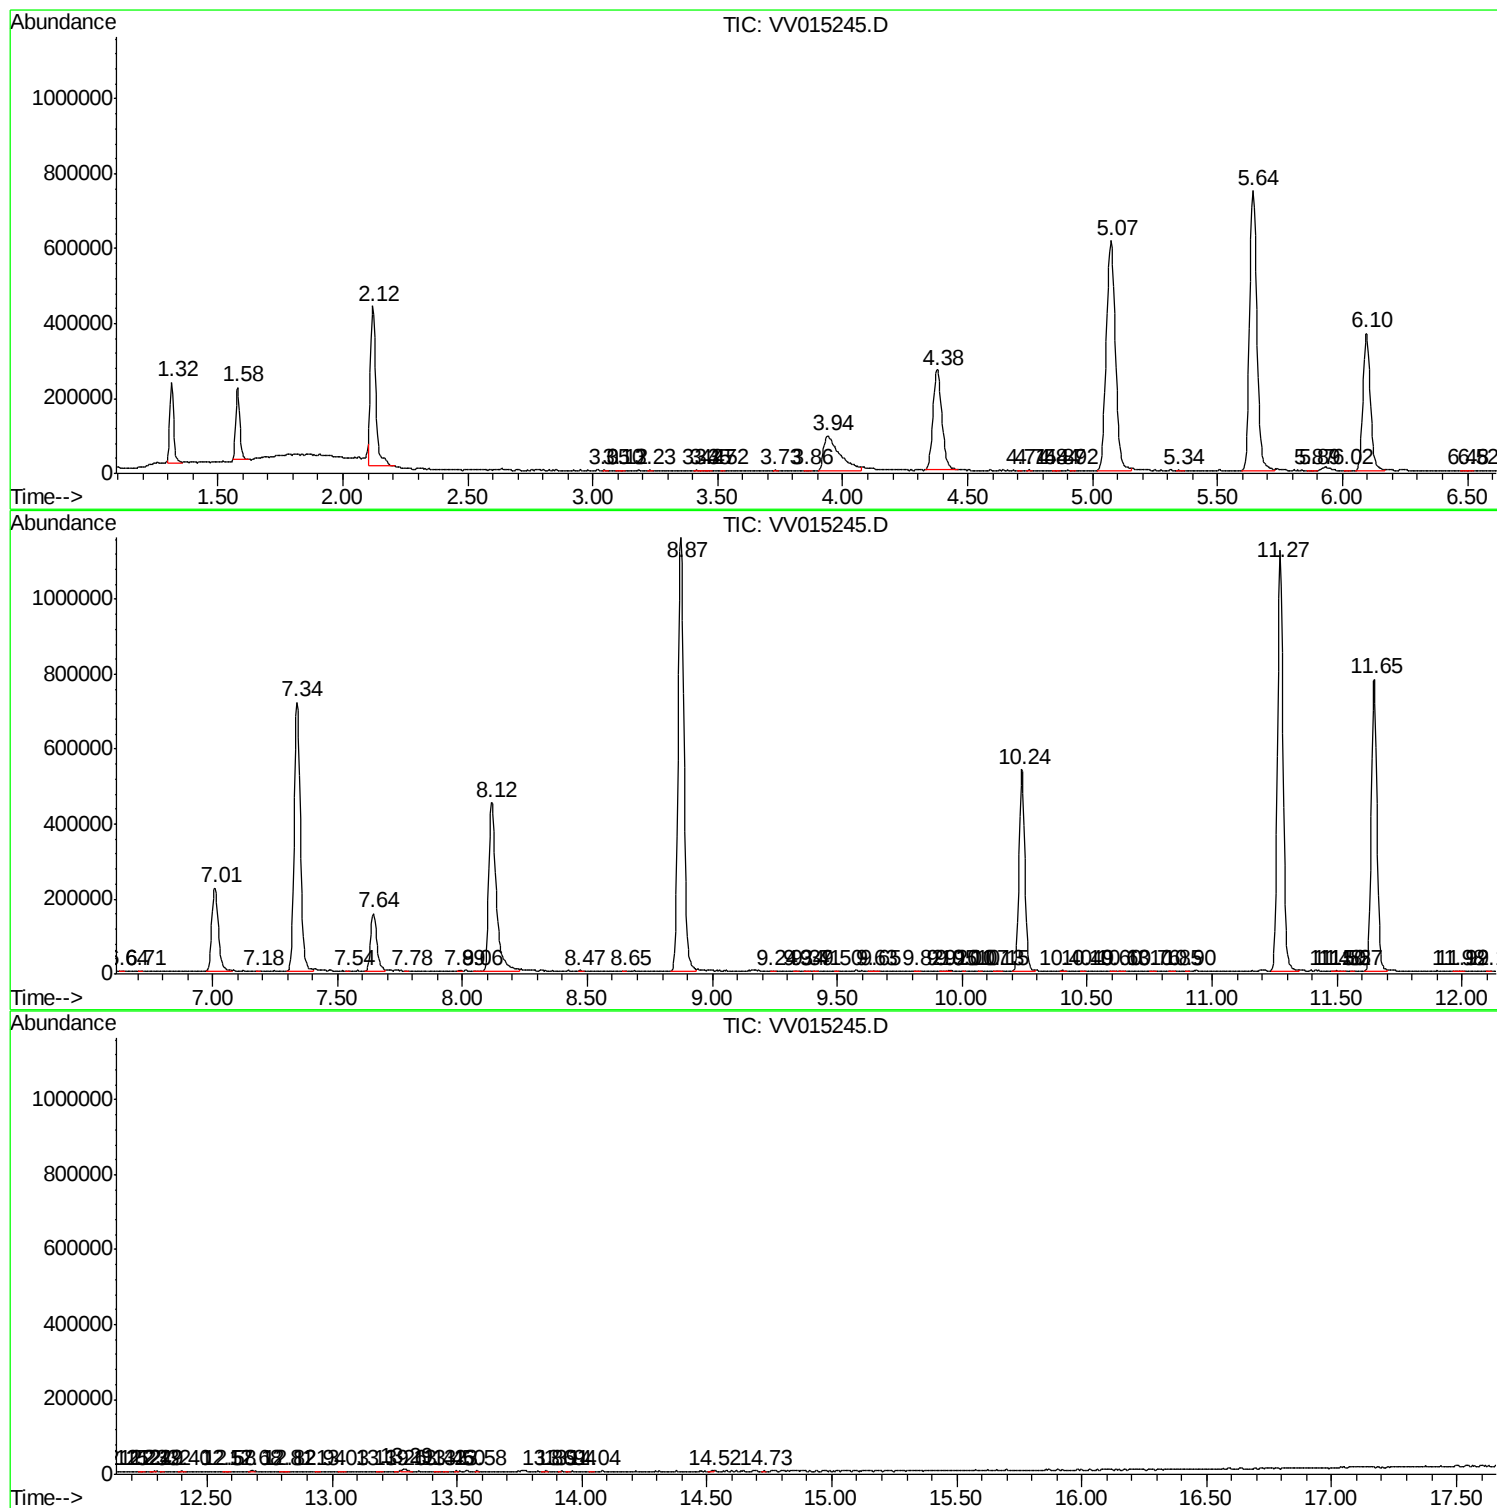

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV032720\
Data File : VV015245.D
Acq On : 28 Mar 2020 14:44
Operator : SY/MD
Sample : L1975-13 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTH6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV032720\
Data File : VV015245.D
Acq On : 28 Mar 2020 14:44
Operator : SY/MD
Sample : L1975-13 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTH6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc