

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015247.D
 Acq On : 28 Mar 2020 15:32
 Operator : SY/MD
 Sample : L1975-19 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTK0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	64	69	79	rVB	211103	210520	11.41%	1.458%
2	1.576	146	151	164	rVB	195319	233527	12.66%	1.617%
3	2.116	313	319	330	rVB	408934	571363	30.97%	3.957%
4	3.119	629	631	633	rBV3	2578	1565	0.08%	0.011%
5	3.418	721	724	725	rBV3	1432	896	0.05%	0.006%
6	3.672	801	803	808	rBV4	2283	1911	0.10%	0.013%
7	3.807	841	845	850	rBV7	2320	3131	0.17%	0.022%
8	3.946	875	888	925	rBV2	87666	400555	21.71%	2.774%
9	4.376	1009	1022	1046	rVB2	269535	657314	35.62%	4.553%
10	5.071	1223	1238	1259	rBV2	616070	1525678	82.68%	10.567%
11	5.405	1340	1342	1347	rVB4	2542	1627	0.09%	0.011%
12	5.431	1347	1350	1353	rBV5	2239	1451	0.08%	0.010%
13	5.505	1368	1373	1375	rBV4	2670	2605	0.14%	0.018%
14	5.640	1403	1415	1442	rBV	739376	1466863	79.50%	10.160%
15	5.881	1488	1490	1493	rBV4	1300	892	0.05%	0.006%
16	6.097	1544	1557	1576	rBV	367507	744013	40.32%	5.153%
17	6.457	1666	1669	1674	rBV7	1143	1138	0.06%	0.008%
18	6.592	1706	1711	1712	rBV5	1828	1666	0.09%	0.012%
19	6.624	1717	1721	1723	rBV4	2243	1816	0.10%	0.013%
20	6.672	1733	1736	1738	rBV4	2313	1645	0.09%	0.011%
21	6.765	1762	1765	1767	rBV4	1736	1412	0.08%	0.010%
22	6.852	1789	1792	1796	rBV5	1957	1779	0.10%	0.012%
23	6.961	1824	1826	1829	rBV4	1481	1080	0.06%	0.007%
24	7.010	1829	1841	1864	rVV	220668	400935	21.73%	2.777%
25	7.244	1911	1914	1915	rBV3	1576	1003	0.05%	0.007%
26	7.338	1931	1943	1963	rBV	718852	1236316	67.00%	8.563%
27	7.595	2021	2023	2026	rBV4	1639	1216	0.07%	0.008%
28	7.643	2027	2038	2057	rVV	154995	271625	14.72%	1.881%
29	7.781	2078	2081	2082	rBV3	2188	1017	0.06%	0.007%
30	7.839	2093	2099	2102	rVB6	2472	2507	0.14%	0.017%
31	7.945	2127	2132	2135	rBV6	2714	2630	0.14%	0.018%
32	8.029	2155	2158	2160	rBV3	1361	899	0.05%	0.006%
33	8.080	2172	2174	2175	rBV3	1647	850	0.05%	0.006%
34	8.119	2175	2186	2214	rVV3	448419	933334	50.58%	6.464%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015247.D
 Acq On : 28 Mar 2020 15:32
 Operator : SY/MD
 Sample : L1975-19 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTK0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

35	8.395	2267	2272	2276	rBV7	2398	2519	0.14%	0.017%
36	8.759	2381	2385	2387	rBV5	1525	1351	0.07%	0.009%
37	8.807	2397	2400	2402	rBV4	1201	840	0.05%	0.006%
38	8.875	2409	2421	2452	rBV	1135724	1845178	100.00%	12.780%
39	9.113	2492	2495	2498	rVB4	2302	1052	0.06%	0.007%
40	9.254	2537	2539	2542	rBV3	1253	907	0.05%	0.006%
41	9.309	2551	2556	2564	rBV10	2090	3136	0.17%	0.022%
42	9.354	2567	2570	2571	rBV3	1679	900	0.05%	0.006%
43	9.383	2576	2579	2581	rBV4	1885	805	0.04%	0.006%
44	9.402	2583	2585	2588	rVB3	2221	1163	0.06%	0.008%
45	9.543	2627	2629	2631	rBV3	1886	940	0.05%	0.007%
46	9.598	2643	2646	2647	rBV3	1978	977	0.05%	0.007%
47	9.624	2651	2654	2657	rBV5	1603	920	0.05%	0.006%
48	9.656	2661	2664	2666	rBV2	1643	1021	0.06%	0.007%
49	9.685	2669	2673	2674	rBV5	1324	881	0.05%	0.006%
50	9.711	2678	2681	2682	rBV3	1572	807	0.04%	0.006%
51	9.784	2701	2704	2709	rBV7	2170	2299	0.12%	0.016%
52	9.955	2753	2757	2759	rBV4	2209	1707	0.09%	0.012%
53	10.013	2771	2775	2778	rBV7	1944	1256	0.07%	0.009%
54	10.045	2783	2785	2789	rVB5	2832	2073	0.11%	0.014%
55	10.064	2789	2791	2793	rBV4	1619	852	0.05%	0.006%
56	10.112	2804	2806	2813	rVB8	2293	1863	0.10%	0.013%
57	10.145	2813	2816	2824	rBV10	1373	1482	0.08%	0.010%
58	10.238	2833	2845	2860	rBV	537475	860511	46.64%	5.960%
59	10.492	2922	2924	2927	rVB5	1372	782	0.04%	0.005%
60	10.534	2934	2937	2938	rBV3	1634	936	0.05%	0.006%
61	10.585	2951	2953	2958	rVB5	2355	1260	0.07%	0.009%
62	10.678	2979	2982	2984	rVB3	2384	1297	0.07%	0.009%
63	10.694	2984	2987	2990	rBV4	2235	1725	0.09%	0.012%
64	10.746	3000	3003	3004	rBV3	2077	1215	0.07%	0.008%
65	10.846	3031	3034	3036	rBV3	2702	1755	0.10%	0.012%
66	10.868	3039	3041	3043	rBV3	2055	1001	0.05%	0.007%
67	10.923	3055	3058	3059	rBV3	1658	869	0.05%	0.006%
68	10.987	3075	3078	3081	rBV5	2109	1525	0.08%	0.011%
69	11.129	3118	3122	3124	rBV4	1822	1395	0.08%	0.010%
70	11.273	3154	3167	3184	rBV	1104631	1720009	93.22%	11.913%
71	11.463	3223	3226	3227	rBV3	1359	916	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015247.D
 Acq On : 28 Mar 2020 15:32
 Operator : SY/MD
 Sample : L1975-19 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTK0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

72	11.569	3257	3259	3262	rVB3	1633	819	0.04%	0.006%
73	11.592	3262	3266	3271	rBV7	1508	1658	0.09%	0.011%
74	11.649	3272	3284	3301	rVV	785181	1235336	66.95%	8.556%
75	11.794	3326	3329	3335	rVB7	2555	2265	0.12%	0.016%
76	11.894	3356	3360	3362	rBV4	1218	840	0.05%	0.006%
77	12.029	3399	3402	3403	rBV3	1479	870	0.05%	0.006%
78	12.083	3416	3419	3424	rVB6	2420	2022	0.11%	0.014%
79	12.106	3424	3426	3429	rBV4	1755	1099	0.06%	0.008%
80	12.125	3429	3432	3436	rBV5	1408	1194	0.06%	0.008%
81	12.235	3464	3466	3471	rVB7	2194	1331	0.07%	0.009%
82	12.575	3570	3572	3577	rVB5	1967	1374	0.07%	0.010%
83	12.627	3585	3588	3590	rBV4	2261	1304	0.07%	0.009%
84	12.749	3623	3626	3629	rVB4	2566	1472	0.08%	0.010%
85	12.836	3650	3653	3655	rVB4	2109	1268	0.07%	0.009%
86	13.038	3713	3716	3719	rBV5	1085	791	0.04%	0.005%
87	13.083	3728	3730	3733	rBV3	1914	990	0.05%	0.007%
88	13.099	3733	3735	3738	rBV3	1871	834	0.05%	0.006%
89	13.170	3756	3757	3762	rVB3	2592	1417	0.08%	0.010%
90	13.193	3762	3764	3767	rBV4	1622	1213	0.07%	0.008%
91	13.286	3788	3793	3795	rBV5	5330	5419	0.29%	0.038%
92	13.434	3832	3839	3841	rBV8	2224	2897	0.16%	0.020%
93	13.479	3851	3853	3855	rBV3	1986	1024	0.06%	0.007%
94	13.649	3904	3906	3908	rVV3	1559	774	0.04%	0.005%
95	13.688	3915	3918	3921	rBV5	2753	2818	0.15%	0.020%
96	13.897	3976	3983	3987	rBV8	2874	2958	0.16%	0.020%
97	14.151	4060	4062	4068	rVB7	2140	1307	0.07%	0.009%
98	14.247	4089	4092	4094	rBV4	3157	2363	0.13%	0.016%
99	14.347	4120	4123	4127	rBV5	2717	1628	0.09%	0.011%
100	14.784	4256	4259	4263	rBV5	2214	1981	0.11%	0.014%


Sum of corrected areas: 14438170

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032720\
Data File : VV015247.D
Acq On : 28 Mar 2020 15:32
Operator : SY/MD
Sample : L1975-19 40X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTK0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

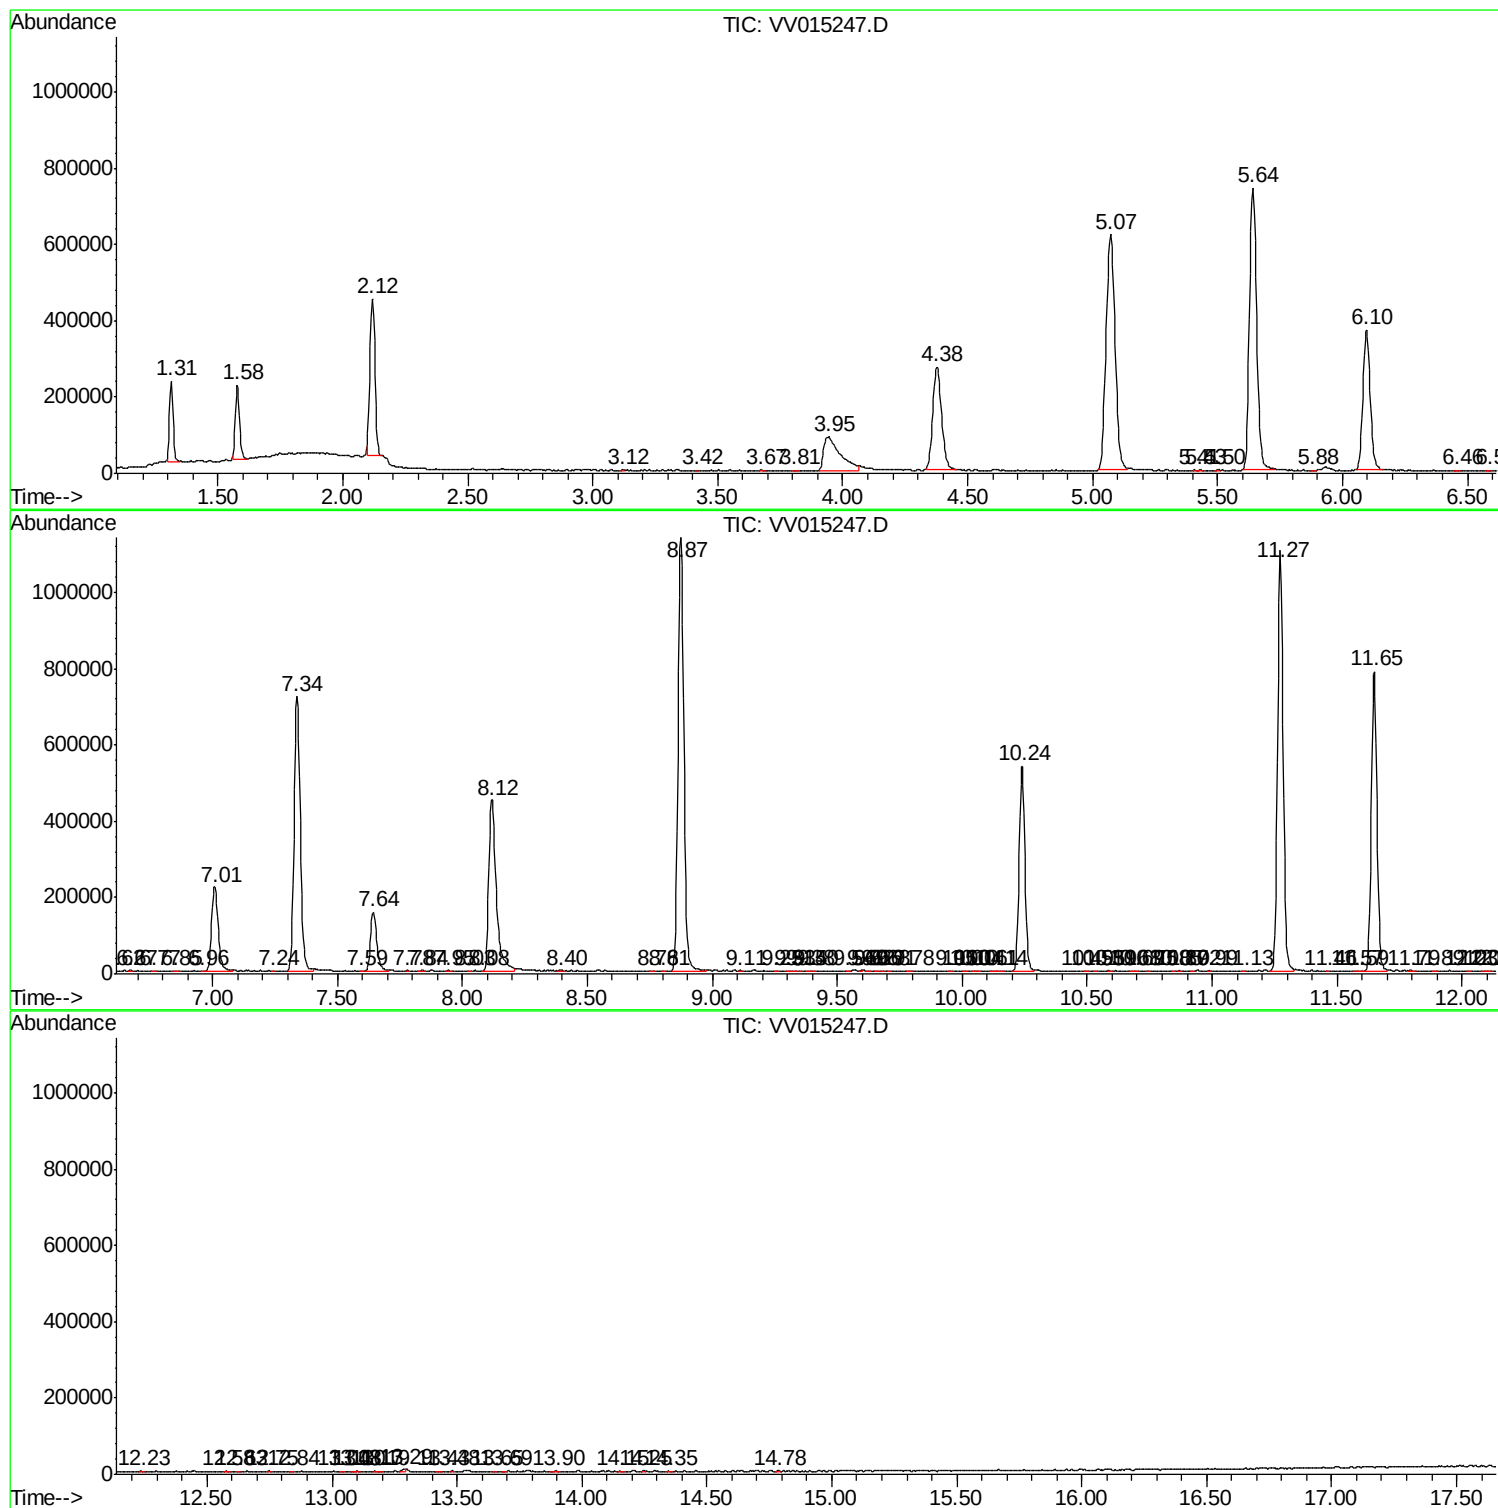

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV032720\
Data File : VV015247.D
Acq On : 28 Mar 2020 15:32
Operator : SY/MD
Sample : L1975-19 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTK0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032720\
Data File : VV015247.D
Acq On : 28 Mar 2020 15:32
Operator : SY/MD
Sample : L1975-19 40X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
ETTK0

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc