

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015248.D
 Acq On : 28 Mar 2020 15:56
 Operator : SY/MD
 Sample : L1975-21 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTK2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	65	70	84	rVB	211593	215114	11.46%	1.468%
2	1.579	146	152	165	rVB	191195	225402	12.00%	1.539%
3	2.119	314	320	345	rVB	432954	667592	35.55%	4.557%
4	3.421	721	725	728	rBV6	2001	1612	0.09%	0.011%
5	3.457	734	736	737	rBV2	1511	620	0.03%	0.004%
6	3.553	764	766	768	rBV2	1321	692	0.04%	0.005%
7	3.624	786	788	790	rBV3	1973	667	0.04%	0.005%
8	3.872	862	865	866	rBV3	1624	1027	0.05%	0.007%
9	3.946	875	888	926	rBV2	89208	423450	22.55%	2.890%
10	4.380	1010	1023	1054	rVB	266836	669464	35.65%	4.570%
11	4.704	1122	1124	1126	rBV3	2262	1227	0.07%	0.008%
12	4.781	1146	1148	1150	rBV2	1706	883	0.05%	0.006%
13	4.798	1150	1153	1154	rBV3	1803	952	0.05%	0.006%
14	4.823	1159	1161	1165	rBV5	1190	881	0.05%	0.006%
15	4.984	1208	1211	1214	rVB6	2884	1940	0.10%	0.013%
16	5.003	1214	1217	1221	rBV5	1491	1378	0.07%	0.009%
17	5.074	1222	1239	1269	rVV2	616253	1547584	82.42%	10.564%
18	5.351	1323	1325	1326	rBV2	1552	653	0.03%	0.004%
19	5.389	1335	1337	1340	rVB4	3165	1588	0.08%	0.011%
20	5.408	1340	1343	1344	rBV3	1273	873	0.05%	0.006%
21	5.643	1403	1416	1449	rVB	747742	1494273	79.58%	10.200%
22	6.097	1540	1557	1575	rBV	365875	749699	39.93%	5.117%
23	6.306	1620	1622	1625	rVB4	1791	951	0.05%	0.006%
24	6.334	1625	1631	1632	rBV6	2392	2209	0.12%	0.015%
25	6.415	1654	1656	1658	rBV3	1723	1078	0.06%	0.007%
26	6.479	1673	1676	1680	rVB4	2102	1553	0.08%	0.011%
27	6.617	1717	1719	1721	rBV2	1150	550	0.03%	0.004%
28	6.704	1744	1746	1748	rBV3	1507	692	0.04%	0.005%
29	6.765	1762	1765	1767	rBV3	1663	1024	0.05%	0.007%
30	6.794	1767	1774	1776	rBV7	1852	2178	0.12%	0.015%
31	6.862	1793	1795	1797	rBV3	1098	437	0.02%	0.003%
32	6.910	1807	1810	1814	rVB6	2545	2115	0.11%	0.014%
33	6.939	1814	1819	1824	rBV8	2634	2902	0.15%	0.020%
34	7.010	1829	1841	1858	rBV	221287	398149	21.20%	2.718%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015248.D
 Acq On : 28 Mar 2020 15:56
 Operator : SY/MD
 Sample : L1975-21 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTK2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

35	7.338	1931	1943	1963	rBV	704917	1236735	65.87%	8.442%
36	7.643	2027	2038	2056	rBV	151482	268602	14.31%	1.833%
37	8.119	2175	2186	2221	rBV2	441857	937640	49.94%	6.400%
38	8.412	2273	2277	2279	rBV5	2363	1967	0.10%	0.013%
39	8.466	2291	2294	2295	rBV3	1687	1039	0.06%	0.007%
40	8.518	2308	2310	2318	rVB7	2172	2414	0.13%	0.016%
41	8.601	2334	2336	2338	rBV3	959	290	0.02%	0.002%
42	8.711	2367	2370	2371	rBV3	1637	1050	0.06%	0.007%
43	8.875	2409	2421	2445	rBV	1169002	1877638	100.00%	12.816%
44	9.244	2533	2536	2538	rBV3	1265	738	0.04%	0.005%
45	9.389	2579	2581	2584	rVB4	1255	775	0.04%	0.005%
46	9.415	2587	2589	2594	rVB4	1604	1047	0.06%	0.007%
47	9.492	2611	2613	2615	rBV3	1374	787	0.04%	0.005%
48	9.797	2705	2708	2710	rBV4	1433	966	0.05%	0.007%
49	9.826	2714	2717	2719	rBV3	2058	1405	0.07%	0.010%
50	9.878	2730	2733	2736	rBV5	1050	728	0.04%	0.005%
51	10.013	2773	2775	2777	rBV3	1510	744	0.04%	0.005%
52	10.061	2788	2790	2791	rBV2	952	296	0.02%	0.002%
53	10.071	2791	2793	2797	rVB4	1674	1251	0.07%	0.009%
54	10.238	2834	2845	2860	rBV	547549	859112	45.75%	5.864%
55	10.370	2884	2886	2888	rBV3	1639	565	0.03%	0.004%
56	10.402	2892	2896	2900	rBV6	1951	1500	0.08%	0.010%
57	10.527	2932	2935	2937	rBV3	2233	1369	0.07%	0.009%
58	10.556	2942	2944	2946	rBV3	1509	882	0.05%	0.006%
59	10.592	2953	2955	2957	rBV3	1525	673	0.04%	0.005%
60	10.640	2966	2970	2975	rBV7	2040	2037	0.11%	0.014%
61	10.678	2980	2982	2985	rBV4	998	704	0.04%	0.005%
62	10.730	2996	2998	3001	rBV4	1968	1486	0.08%	0.010%
63	10.846	3032	3034	3035	rBV2	1080	315	0.02%	0.002%
64	10.916	3051	3056	3057	rBV5	1899	1701	0.09%	0.012%
65	11.051	3094	3098	3099	rBV3	2185	1406	0.07%	0.010%
66	11.167	3132	3134	3136	rBV3	1029	598	0.03%	0.004%
67	11.273	3155	3167	3189	rBV	1119231	1744064	92.89%	11.905%
68	11.537	3243	3249	3252	rBV8	2533	3283	0.17%	0.022%
69	11.591	3261	3266	3268	rBV5	1452	1282	0.07%	0.009%
70	11.601	3268	3269	3270	rBV	1438	418	0.02%	0.003%
71	11.649	3272	3284	3300	rVV	774446	1243539	66.23%	8.488%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015248.D
 Acq On : 28 Mar 2020 15:56
 Operator : SY/MD
 Sample : L1975-21 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTK2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

72	11.974	3383	3385	3386	rBV2	1162	408	0.02%	0.003%
73	11.997	3391	3392	3394	rVV2	1130	355	0.02%	0.002%
74	12.090	3417	3421	3422	rBV3	679	425	0.02%	0.003%
75	12.170	3444	3446	3448	rBV3	1238	593	0.03%	0.004%
76	12.344	3497	3500	3503	rVB5	1927	1355	0.07%	0.009%
77	12.427	3524	3526	3528	rVB3	1071	371	0.02%	0.003%
78	12.437	3528	3529	3531	rBV2	1478	837	0.04%	0.006%
79	12.472	3538	3540	3542	rBV3	1233	505	0.03%	0.003%
80	12.521	3552	3555	3558	rBV4	1117	788	0.04%	0.005%
81	12.791	3638	3639	3642	rBV3	1426	761	0.04%	0.005%
82	12.897	3670	3672	3676	rVB5	2117	1437	0.08%	0.010%
83	12.916	3676	3678	3679	rBV2	1790	841	0.04%	0.006%
84	13.289	3787	3794	3798	rBV8	8069	11704	0.62%	0.080%
85	13.325	3803	3805	3808	rVB4	1327	606	0.03%	0.004%
86	13.537	3868	3871	3874	rBV4	2487	1601	0.09%	0.011%
87	13.656	3906	3908	3911	rBV4	994	452	0.02%	0.003%
88	13.723	3927	3929	3931	rBV3	1187	585	0.03%	0.004%
89	13.952	3997	4000	4003	rBV4	1502	1020	0.05%	0.007%
90	14.045	4026	4029	4032	rBV5	2344	1722	0.09%	0.012%
91	14.533	4179	4181	4183	rBV3	2090	976	0.05%	0.007%
92	14.566	4190	4191	4192	rBV2	1270	462	0.02%	0.003%


Sum of corrected areas: 14650259

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032720\
Data File : VV015248.D
Acq On : 28 Mar 2020 15:56
Operator : SY/MD
Sample : L1975-21 40X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTK2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

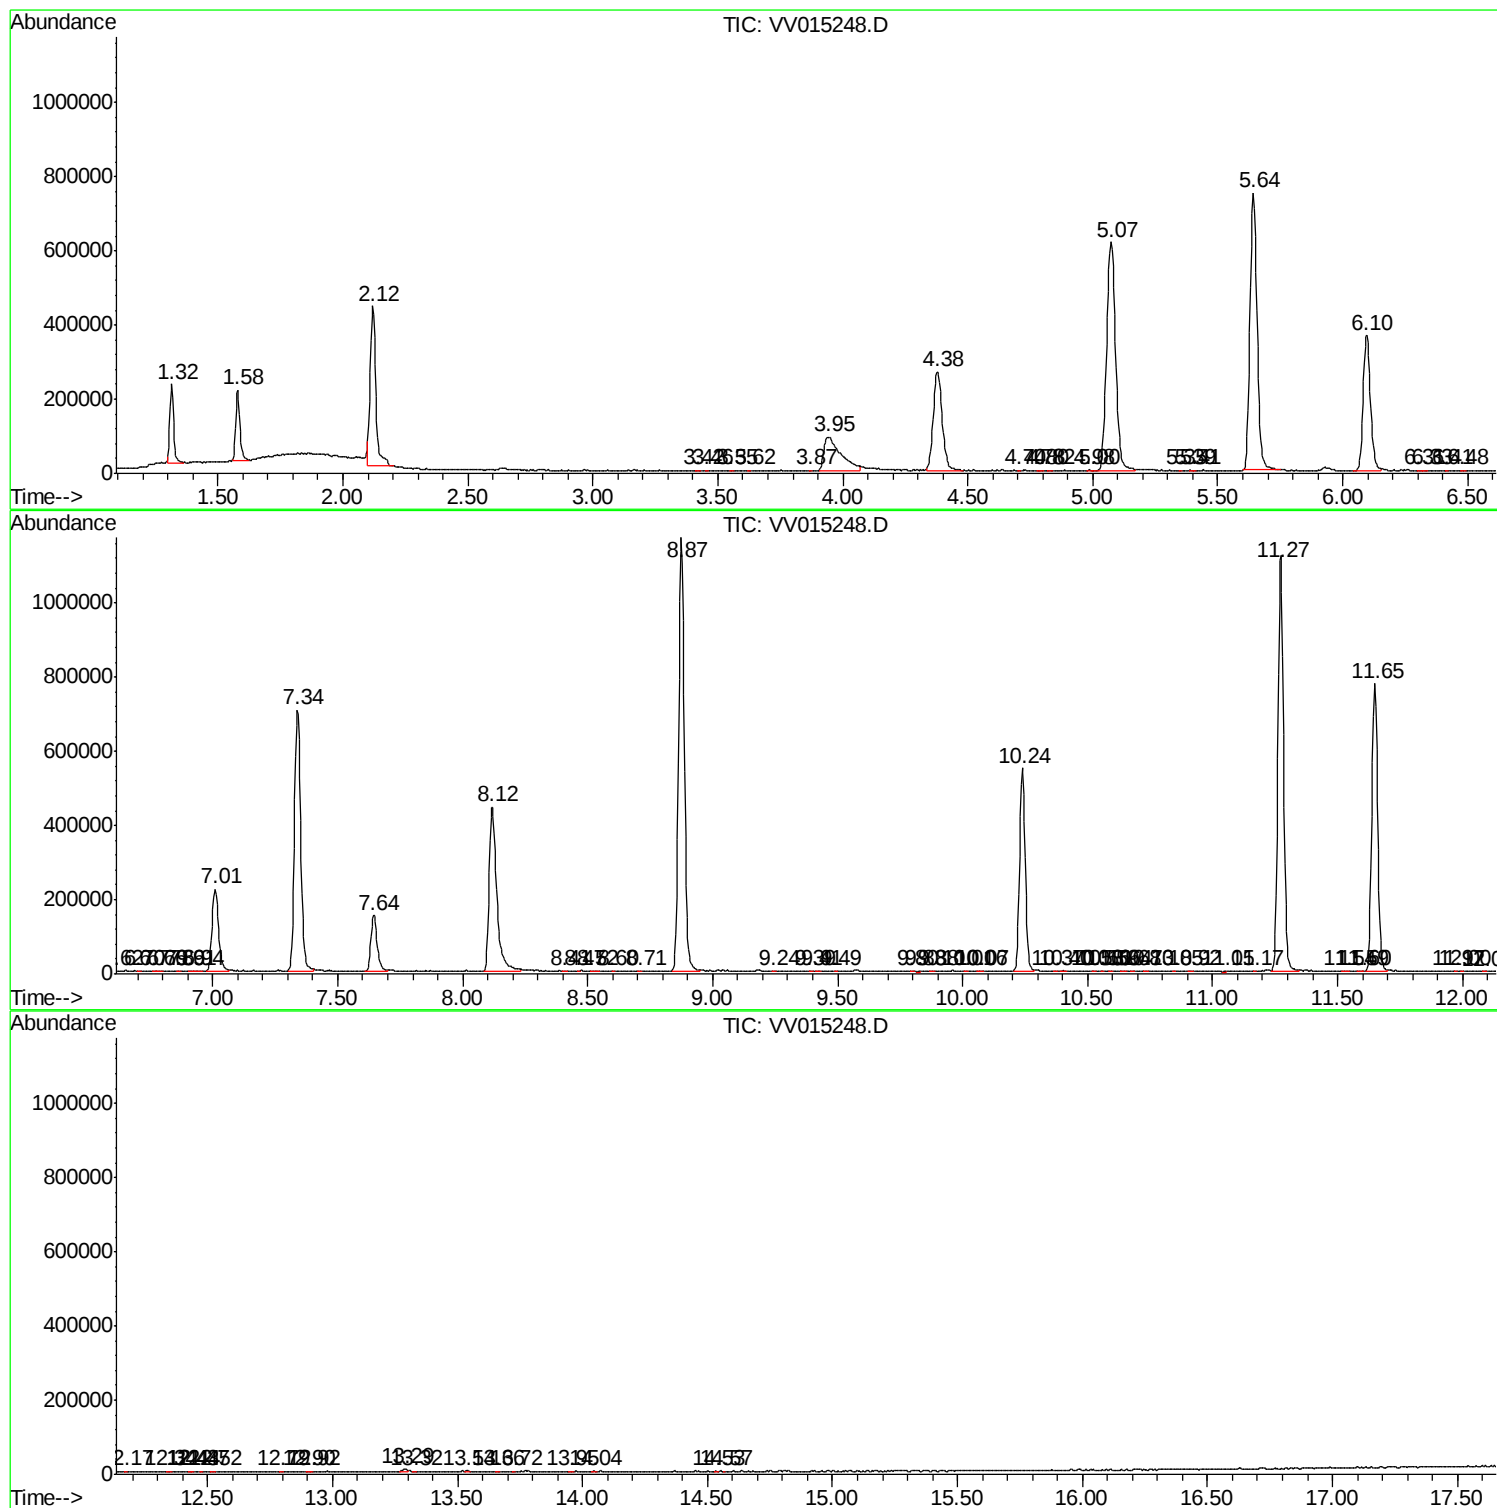

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV032720\
Data File : VV015248.D
Acq On : 28 Mar 2020 15:56
Operator : SY/MD
Sample : L1975-21 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTK2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV032720\
Data File : VV015248.D
Acq On : 28 Mar 2020 15:56
Operator : SY/MD
Sample : L1975-21 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTK2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc