

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015252.D
 Acq On : 28 Mar 2020 17:42
 Operator : SY/MD
 Sample : L1975-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTG6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	64	70	84	rVB2	379107	412555	22.64%	2.923%
2	2.119	314	320	342	rVB	387770	588905	32.31%	4.172%
3	2.460	419	426	441	rVB	80367	151967	8.34%	1.077%
4	3.290	680	684	686	rBV4	2330	1723	0.09%	0.012%
5	3.312	689	691	693	rVB3	1678	611	0.03%	0.004%
6	3.338	697	699	700	rBV3	1900	998	0.05%	0.007%
7	3.483	742	744	746	rBV3	1544	644	0.04%	0.005%
8	3.515	752	754	758	rVB4	1800	1082	0.06%	0.008%
9	3.566	767	770	772	rBV3	1585	976	0.05%	0.007%
10	3.586	772	776	779	rBV5	1585	1444	0.08%	0.010%
11	3.663	797	800	802	rBV3	1945	1140	0.06%	0.008%
12	3.682	802	806	811	rVB6	1941	1995	0.11%	0.014%
13	3.737	821	823	825	rBV3	1242	596	0.03%	0.004%
14	3.939	874	886	912	rBV3	128052	441484	24.22%	3.128%
15	4.306	998	1000	1001	rBV2	1805	933	0.05%	0.007%
16	4.377	1006	1022	1048	rBV2	246443	627326	34.42%	4.444%
17	4.891	1180	1182	1184	rVB2	767	246	0.01%	0.002%
18	4.913	1184	1189	1191	rBV6	2106	2185	0.12%	0.015%
19	5.016	1217	1221	1222	rBV3	2874	1475	0.08%	0.010%
20	5.074	1223	1239	1261	rVV2	572373	1426526	78.27%	10.106%
21	5.643	1403	1416	1442	rBV	734050	1443292	79.19%	10.225%
22	6.097	1544	1557	1582	rBV	343088	694944	38.13%	4.923%
23	6.450	1663	1667	1669	rVB4	2295	1374	0.08%	0.010%
24	6.518	1684	1688	1690	rBV5	1735	1177	0.06%	0.008%
25	6.592	1708	1711	1713	rBV4	1787	881	0.05%	0.006%
26	6.614	1716	1718	1721	rBV4	2234	1503	0.08%	0.011%
27	6.756	1759	1762	1764	rBV4	2081	1383	0.08%	0.010%
28	6.820	1779	1782	1784	rBV3	1691	1362	0.07%	0.010%
29	6.868	1795	1797	1800	rBV4	1482	1083	0.06%	0.008%
30	6.962	1821	1826	1828	rBV5	1907	1644	0.09%	0.012%
31	7.010	1831	1841	1860	rVV	184205	334839	18.37%	2.372%
32	7.257	1913	1918	1922	rBV8	2141	2571	0.14%	0.018%
33	7.338	1931	1943	1962	rBV	652552	1134502	62.25%	8.038%
34	7.643	2023	2038	2054	rBV	131741	236324	12.97%	1.674%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015252.D
 Acq On : 28 Mar 2020 17:42
 Operator : SY/MD
 Sample : L1975-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTG6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

35	7.798	2084	2086	2087	rBV2	1711	842	0.05%	0.006%
36	8.000	2147	2149	2151	rBV3	1891	1192	0.07%	0.008%
37	8.032	2157	2159	2161	rBV2	1454	879	0.05%	0.006%
38	8.116	2174	2185	2214	rBV4	482434	980074	53.77%	6.943%
39	8.373	2263	2265	2267	rBV4	1937	962	0.05%	0.007%
40	8.505	2302	2306	2309	rBV5	1819	1823	0.10%	0.013%
41	8.611	2336	2339	2343	rBV4	1622	1768	0.10%	0.013%
42	8.875	2410	2421	2445	rVB	1116120	1822595	100.00%	12.912%
43	9.154	2502	2508	2510	rBV6	2709	3375	0.19%	0.024%
44	9.376	2575	2577	2581	rBV4	1790	1248	0.07%	0.009%
45	9.392	2581	2582	2584	rBV2	1078	522	0.03%	0.004%
46	9.454	2599	2601	2604	rVB4	1492	678	0.04%	0.005%
47	9.560	2632	2634	2635	rBV2	1465	611	0.03%	0.004%
48	9.727	2683	2686	2687	rBV3	1288	756	0.04%	0.005%
49	9.781	2699	2703	2706	rBV6	1556	1216	0.07%	0.009%
50	10.003	2766	2772	2774	rBV5	1828	1589	0.09%	0.011%
51	10.158	2818	2820	2821	rBV2	1099	426	0.02%	0.003%
52	10.193	2829	2831	2832	rBV2	848	381	0.02%	0.003%
53	10.238	2832	2845	2859	rBV	525878	829422	45.51%	5.876%
54	10.396	2891	2894	2897	rBV5	2808	2187	0.12%	0.015%
55	10.437	2905	2907	2910	rVB4	1583	948	0.05%	0.007%
56	10.460	2910	2914	2916	rBV5	1528	1164	0.06%	0.008%
57	10.479	2918	2920	2922	rVB3	1461	529	0.03%	0.004%
58	10.691	2982	2986	2987	rBV3	2055	1517	0.08%	0.011%
59	10.891	3043	3048	3052	rBV7	2301	2256	0.12%	0.016%
60	10.910	3052	3054	3055	rBV2	1166	490	0.03%	0.003%
61	10.949	3064	3066	3068	rBV3	1357	889	0.05%	0.006%
62	10.990	3075	3079	3081	rBV4	2638	1977	0.11%	0.014%
63	11.032	3090	3092	3093	rBV2	1182	360	0.02%	0.003%
64	11.161	3130	3132	3133	rBV2	922	309	0.02%	0.002%
65	11.273	3154	3167	3185	rBV	1100323	1713407	94.01%	12.139%
66	11.563	3246	3257	3268	rBV3	12955	28865	1.58%	0.204%
67	11.646	3272	3283	3301	rVV	739477	1160527	63.67%	8.222%
68	12.042	3403	3406	3408	rBV3	1402	795	0.04%	0.006%
69	12.158	3440	3442	3445	rBV4	1221	789	0.04%	0.006%
70	12.257	3471	3473	3474	rBV2	681	220	0.01%	0.002%
71	12.469	3536	3539	3540	rBV3	1586	615	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015252.D
 Acq On : 28 Mar 2020 17:42
 Operator : SY/MD
 Sample : L1975-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTG6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis

72	12.514	3549	3553	3557	rVB6	1782	1701	0.09%	0.012%
73	12.540	3557	3561	3563	rBV4	2106	1579	0.09%	0.011%
74	12.608	3581	3582	3585	rBV3	1266	746	0.04%	0.005%
75	12.646	3591	3594	3596	rBV4	1428	924	0.05%	0.007%
76	12.736	3621	3622	3626	rBV4	1276	778	0.04%	0.006%
77	12.916	3675	3678	3681	rBV4	1828	969	0.05%	0.007%
78	13.051	3714	3720	3721	rBV5	1933	1636	0.09%	0.012%
79	13.145	3746	3749	3751	rBV4	1982	1078	0.06%	0.008%
80	13.894	3980	3982	3984	rBV3	1127	488	0.03%	0.003%
81	13.903	3984	3985	3986	rBV	1091	406	0.02%	0.003%
82	13.939	3990	3996	3997	rBV6	2533	1996	0.11%	0.014%
83	14.045	4025	4029	4033	rBV6	2438	2280	0.13%	0.016%
84	14.064	4033	4035	4039	rBV5	2314	1430	0.08%	0.010%
85	14.109	4047	4049	4055	rVB5	2202	1583	0.09%	0.011%
86	14.135	4055	4057	4059	rBV3	1349	477	0.03%	0.003%
87	14.222	4081	4084	4086	rBV3	2167	1310	0.07%	0.009%
88	14.518	4174	4176	4180	rBV4	1713	1160	0.06%	0.008%
89	14.717	4234	4238	4239	rBV3	2182	1549	0.08%	0.011%
90	14.765	4247	4253	4254	rBV6	3043	3056	0.17%	0.022%


Sum of corrected areas: 14115039

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032720\
Data File : VV015252.D
Acq On : 28 Mar 2020 17:42
Operator : SY/MD
Sample : L1975-01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTG6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

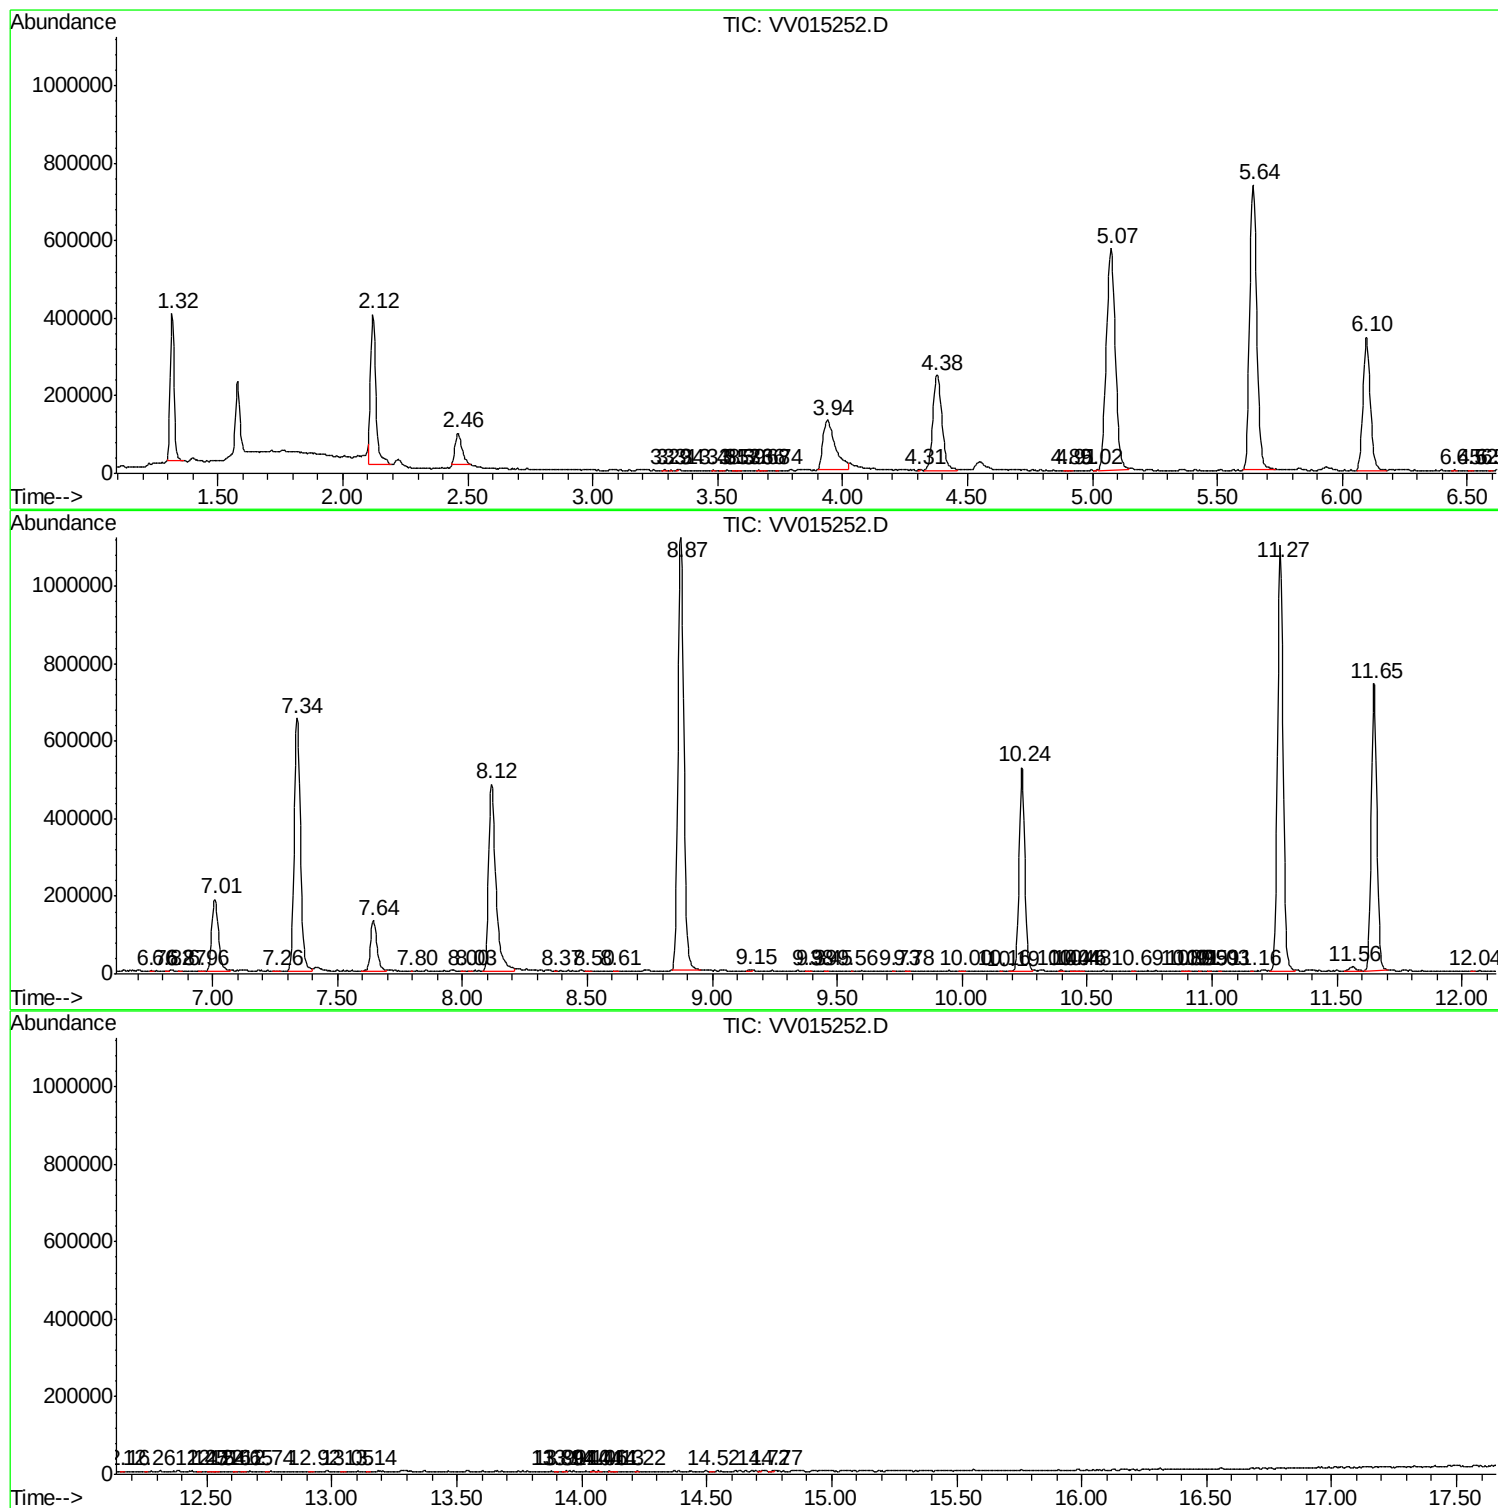

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV032720\
Data File : VV015252.D
Acq On : 28 Mar 2020 17:42
Operator : SY/MD
Sample : L1975-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETT66

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032720\
Data File : VV015252.D
Acq On : 28 Mar 2020 17:42
Operator : SY/MD
Sample : L1975-01
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
ETT66

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc