


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032720\
 Data File : VV015211.D
 Acq On : 27 Mar 2020 17:36
 Operator : SY/MD
 Sample: BFB99
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB99

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032720WMA.M
 Title : VOC Analysis
 Last Update : Mon Aug 19 16:25:56 2019

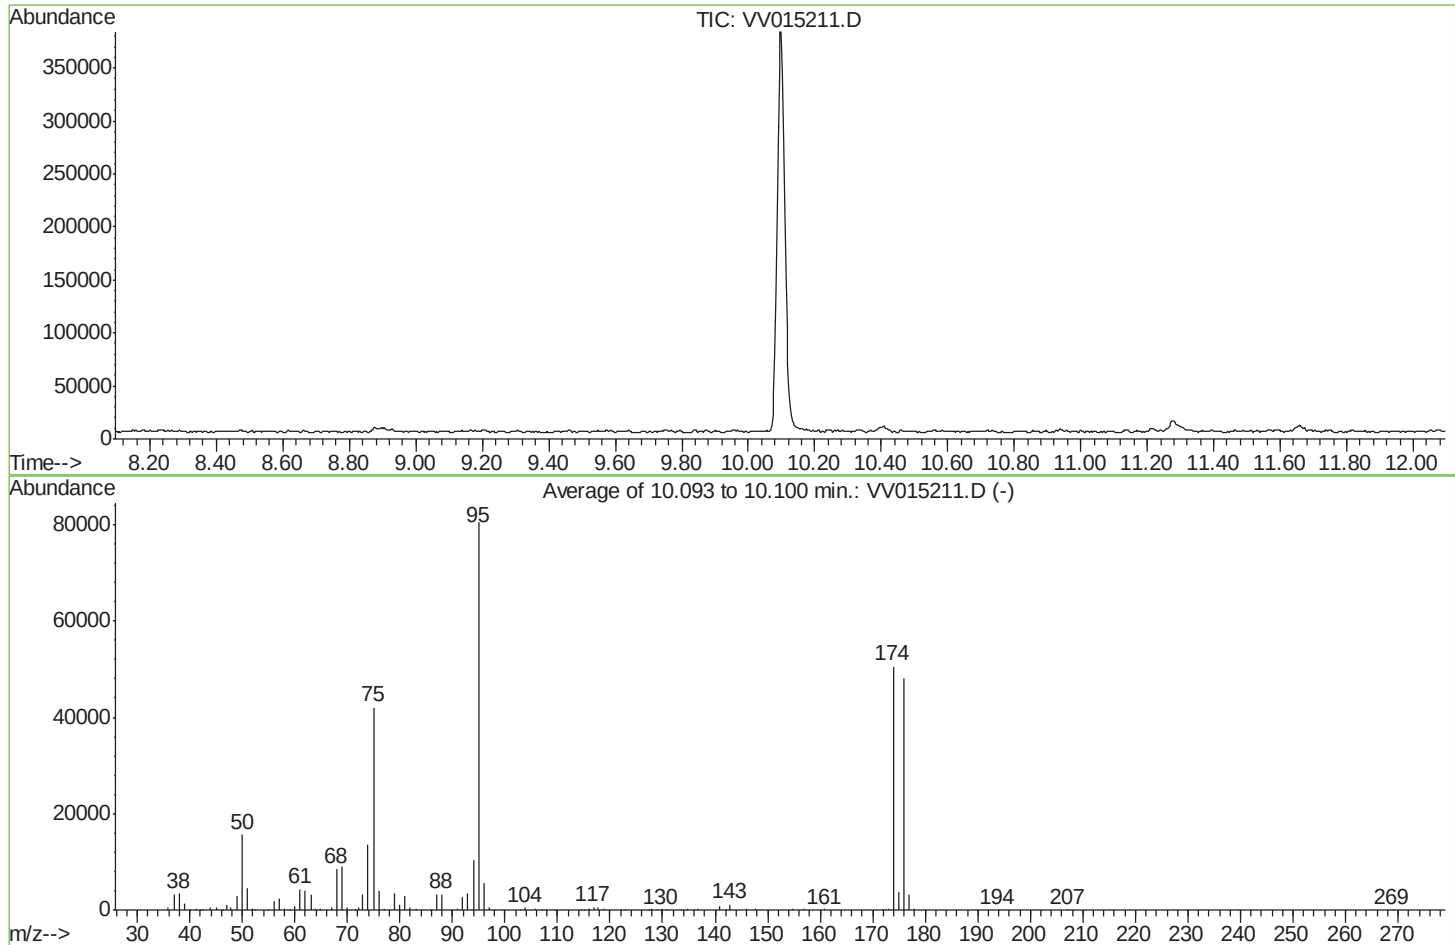

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	15593	PASS
75	95	30	80	52.2	42021	PASS
95	95	100	100	100.0	80498	PASS
96	95	5	9	7.1	5703	PASS
173	174	0.00	2	0.5	237	PASS
174	95	50	120	62.7	50504	PASS
175	174	5	9	7.6	3846	PASS
176	174	95	101	95.0	47992	PASS
177	176	5	9	6.5	3135	PASS

m/z	Abundance
36.00	695.0
37.00	3398.0
38.00	3521.0
39.00	1605.0
40.00	938.0
40.90	193.0
41.30	169.0
41.90	274.0
43.00	268.0
44.00	1338.0
45.00	670.0
46.30	132.0
47.00	1011.0
47.90	499.0
48.90	2860.0
50.00	14859.0
51.00	4496.0
52.00	313.0
53.60	148.0
54.90	462.0
55.90	1741.0
57.00	2442.0
58.00	203.0
58.90	141.0
60.00	1003.0
61.00	4469.0
62.00	3582.0
63.00	2805.0
63.90	316.0
64.90	218.0
67.00	503.0
68.00	8530.0
69.00	8482.0
69.90	713.0
71.40	113.0
72.10	397.0
72.90	3430.0
74.00	13153.0
75.00	39160.0
76.00	3772.0
77.10	347.0
78.00	255.0
78.90	3236.0
79.80	1094.0
80.90	2893.0
82.00	548.0
83.00	229.0
84.10	119.0
85.60	121.0
87.00	2920.0
87.90	3150.0
90.90	386.0
92.00	2452.0
93.00	3346.0
94.00	9670.0
95.00	76104.0
96.00	5335.0
96.90	449.0
102.80	117.0
103.90	475.0
105.90	405.0
107.00	127.0
115.00	154.0
115.90	269.0
116.90	452.0
117.80	405.0
118.80	357.0
122.70	133.0
127.90	248.0
128.80	115.0
129.80	279.0
133.50	116.0
134.80	285.0
136.00	133.0
136.70	190.0
140.80	914.0
142.90	1066.0
145.80	137.0
147.70	208.0
154.80	104.0
156.80	197.0
160.90	159.0
171.70	111.0
173.10	711.0
173.90	46352.0
175.00	3626.0
175.90	42464.0
176.90	2819.0
177.90	168.0
193.90	109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB99

m/z	Abundance
35.10	115.0
36.00	712.0
37.00	3400.0
38.00	3553.0
39.00	1582.0
40.00	976.0
41.10	249.0
41.90	279.0
43.00	257.0
44.00	1368.0
45.00	692.0
46.20	121.0
47.00	1297.0
47.80	609.0
49.00	3077.0
50.00	16165.0
51.00	4869.0
52.00	327.0
53.60	109.0
54.90	488.0
55.90	1807.0
57.00	2777.0
58.10	174.0
60.00	1024.0
61.00	4821.0
62.00	3972.0
63.00	3168.0
63.90	284.0
64.90	220.0
67.00	616.0
68.00	8766.0
69.00	9539.0
69.90	788.0
72.00	483.0
73.00	3534.0
74.00	14245.0
75.00	43320.0
76.00	4046.0
77.00	445.0
78.90	3620.0
79.90	1046.0
80.90	3157.0
82.00	616.0
83.00	180.0
85.70	151.0
87.00	3250.0
87.90	3397.0
91.00	409.0
92.00	2624.0
93.00	3456.0
94.00	10904.0
95.00	82960.0
96.00	6047.0
96.90	472.0
98.00	105.0
102.80	112.0
103.90	543.0
105.80	407.0
107.00	155.0
107.80	106.0
115.00	155.0
115.90	324.0
116.80	549.0
117.80	406.0
118.80	342.0
127.90	244.0
128.80	125.0
129.80	251.0
130.60	106.0
133.50	132.0
134.80	218.0
136.00	157.0
136.70	198.0
140.80	889.0
142.10	113.0
142.90	1128.0
145.80	180.0
147.70	159.0
154.70	144.0
156.80	194.0
160.90	216.0
171.70	141.0
172.30	188.0
173.90	52392.0
174.90	3920.0
175.90	49544.0
176.90	3214.0
177.90	194.0
207.20	118.0

Instrument :
MSVOA_V
ClientSampleId :
BFB99

m/z	Abundance
35.10	148.0
35.90	667.0
37.00	3138.0
38.00	3621.0
39.00	1429.0
40.00	895.0
41.10	319.0
41.90	247.0
42.40	158.0
43.00	261.0
44.00	1366.0
45.00	733.0
46.20	123.0
47.00	1247.0
47.80	711.0
49.00	3128.0
50.00	15755.0
51.00	4646.0
52.00	319.0
52.50	112.0
54.90	479.0
56.00	1672.0
57.00	2804.0
58.10	170.0
60.00	936.0
61.00	4310.0
62.00	4134.0
63.00	3285.0
63.90	227.0
64.90	143.0
67.10	516.0
68.00	8232.0
69.00	9383.0
69.90	722.0
72.00	588.0
73.00	3409.0
74.00	14156.0
75.00	43904.0
76.00	3814.0
76.90	516.0
78.90	3529.0
79.90	1012.0
80.90	3151.0
81.90	702.0
83.00	141.0
85.80	157.0
87.00	3231.0
87.90	3167.0
91.00	404.0
91.90	2541.0
92.90	3401.0
94.00	10711.0
95.00	82432.0
96.00	6164.0
96.90	410.0
102.90	128.0
103.90	462.0
105.90	393.0
107.10	136.0
109.60	120.0
114.60	103.0
115.10	109.0
116.00	292.0
116.80	620.0
117.80	448.0
118.80	327.0
122.10	109.0
127.50	140.0
127.90	202.0
128.90	138.0
129.90	216.0
130.50	132.0
134.80	136.0
135.90	112.0
136.70	184.0
140.90	824.0
142.10	125.0
142.90	1040.0
145.90	231.0
147.80	144.0
154.70	189.0
156.90	178.0
160.90	192.0
171.80	126.0
173.90	52768.0
174.90	3992.0
175.90	51968.0
176.90	3374.0
177.90	148.0
207.20	117.0
269.00	102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB99

m/z	Abundance
35.20	124.0
35.90	105.0
38.20	174.0
38.90	163.0
39.90	858.0
41.00	313.0
42.10	149.0
43.00	386.0
43.80	923.0
45.00	220.0
47.10	108.0
48.20	122.0
50.40	103.0
51.10	134.0
53.00	182.0
53.80	113.0
54.90	345.0
56.20	118.0
56.90	153.0
60.00	126.0
60.90	148.0
66.80	149.0
68.90	168.0
69.80	162.0
72.90	166.0
73.90	154.0
75.10	107.0
77.00	248.0
78.30	118.0
81.00	230.0
83.80	115.0
85.20	184.0
91.00	192.0
95.90	145.0
100.90	117.0
105.00	110.0
112.80	101.0
118.10	151.0
123.20	126.0
125.10	118.0

Instrument :
MSVOA_V
ClientSampleId :
BFB99