


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV032819\
Data File : VV009958.D
Acq On : 28 Mar 2019 10:31
Operator : SY/MD
Sample : BFB78
Misc : 5.00G/10mL/MSVOA V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB78

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM032619S.M
Title : VOC Analysis
Last Update : Fri Mar 29 04:20:29 2019

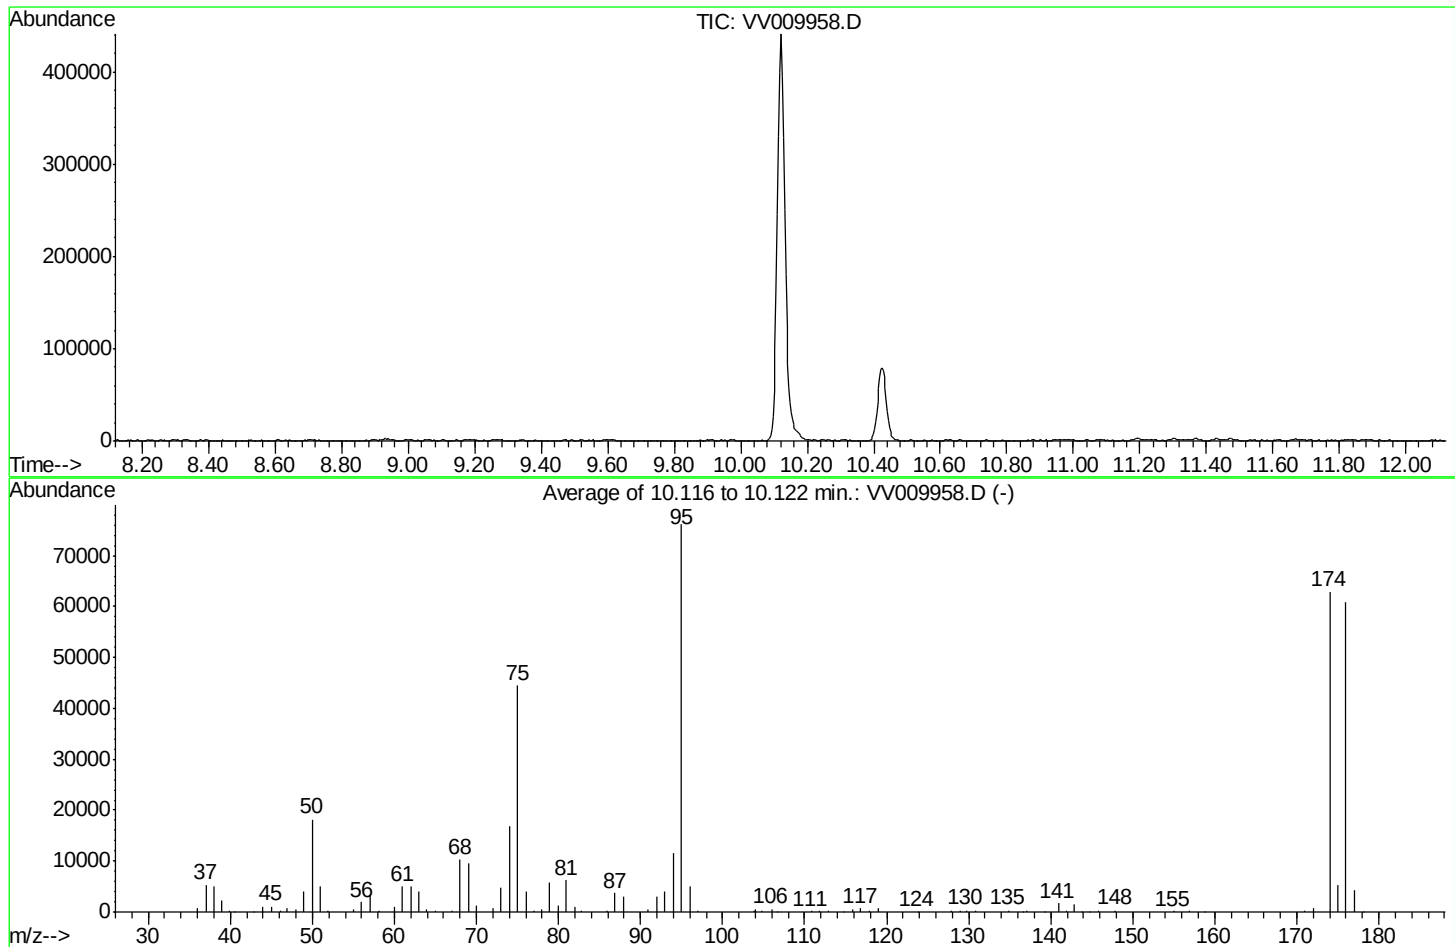

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.9	18208	PASS
75	95	30	80	58.4	44445	PASS
95	95	100	100	100.0	76146	PASS
96	95	5	9	6.7	5081	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	82.5	62858	PASS
175	174	5	9	8.4	5255	PASS
176	174	95	101	96.8	60816	PASS
177	176	5	9	7.1	4295	PASS

Scan 2795 (10.077 min): VV009958.D
BFB78

m/z	Abundance
40.10	277.0
44.00	185.0
48.00	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB78

m/z	Abundance
36.00	747.0
37.00	4998.0
38.00	4634.0
39.00	2324.0
39.90	249.0
44.10	1214.0
45.00	1094.0
46.20	195.0
46.90	729.0
47.90	662.0
49.00	4140.0
50.00	17256.0
51.00	4950.0
51.90	270.0
55.00	363.0
56.00	1956.0
57.00	3365.0
58.20	250.0
60.00	851.0
61.00	4834.0
62.00	4765.0
63.00	4102.0
63.90	491.0
65.00	321.0
67.00	383.0
68.00	9599.0
69.00	8944.0
70.00	1374.0
71.90	808.0
73.00	4389.0
74.00	15801.0
75.00	42240.0
76.00	3975.0
76.90	310.0
78.00	463.0
78.90	5421.0
80.00	1235.0
81.00	5757.0
82.00	985.0
82.90	230.0
85.90	147.0
86.90	3664.0
88.00	2918.0
90.90	576.0
92.00	2912.0
93.00	3739.0
94.00	10670.0
95.00	72432.0
96.00	4961.0
97.10	190.0
103.80	564.0
104.80	132.0
106.00	496.0
106.70	104.0
110.90	166.0
112.90	183.0
115.80	431.0
116.80	615.0
117.90	210.0
119.00	596.0
127.90	311.0
128.80	219.0
129.70	352.0
130.90	136.0
134.90	253.0
137.10	154.0
139.20	117.0
141.00	1614.0
141.90	162.0
142.90	1484.0
143.80	146.0
145.80	183.0
147.90	275.0
154.90	148.0
156.90	144.0
170.90	276.0
172.20	531.0
174.00	57336.0
175.00	4819.0
176.00	55192.0
176.90	3930.0

Instrument :
MSVOA_V
ClientSampleId :
BFB78

m/z	Abundance
36.00	716.0
37.00	5468.0
38.00	5086.0
39.00	2263.0
39.90	258.0
42.80	125.0
44.00	1233.0
45.00	1151.0
46.10	227.0
46.90	703.0
47.90	729.0
49.00	4243.0
50.00	18824.0
51.00	5170.0
51.90	286.0
55.00	424.0
56.00	2029.0
57.00	3273.0
58.10	229.0
60.00	967.0
61.00	5273.0
62.00	5161.0
63.00	4316.0
63.90	463.0
65.00	351.0
67.00	354.0
68.00	10590.0
69.00	9886.0
70.00	1254.0
71.90	861.0
73.00	4785.0
74.00	17256.0
75.00	46096.0
76.00	4245.0
77.00	379.0
78.00	572.0
78.90	5926.0
80.00	1192.0
81.00	6471.0
82.00	1126.0
82.80	229.0
85.90	229.0
86.90	3954.0
87.90	3098.0
90.90	583.0
91.90	2937.0
93.00	4098.0
94.00	11988.0
95.00	78976.0
96.00	5296.0
97.00	217.0
104.00	666.0
104.80	144.0
106.00	532.0
106.70	111.0
110.90	187.0
111.80	167.0
112.90	194.0
114.80	144.0
115.80	469.0
116.80	764.0
118.00	321.0
118.90	718.0
123.70	103.0
127.90	308.0
128.90	186.0
129.70	390.0
130.80	167.0
134.80	267.0
136.60	124.0
137.10	171.0
141.00	1789.0
141.90	265.0
142.90	1635.0
143.80	137.0
144.80	104.0
145.80	263.0
147.90	335.0
154.90	142.0
156.90	129.0
158.80	120.0
170.90	253.0
172.10	676.0
174.00	64776.0
175.00	5414.0
176.00	62792.0
176.90	4541.0

Instrument :
MSVOA_V
ClientSampleId :
BFB78

m/z	Abundance
36.00	688.0
37.00	5438.0
38.00	5066.0
39.00	1988.0
39.80	268.0
40.50	113.0
42.80	154.0
44.00	1086.0
45.00	1082.0
46.10	204.0
47.00	731.0
48.00	676.0
49.00	4053.0
50.00	18544.0
51.00	5313.0
51.90	270.0
55.00	439.0
56.00	2005.0
57.00	3234.0
58.00	157.0
60.00	919.0
61.00	4933.0
62.00	5054.0
63.00	4026.0
63.90	356.0
65.00	341.0
67.00	356.0
68.00	10720.0
69.00	9895.0
69.90	1082.0
72.00	756.0
73.00	4962.0
74.00	17336.0
75.00	45000.0
76.00	3838.0
77.00	468.0
77.90	558.0
78.90	5815.0
80.00	1203.0
80.90	6442.0
82.00	1217.0
82.80	191.0
85.90	193.0
86.90	3586.0
87.90	3215.0
90.90	530.0
91.90	2977.0
93.00	4294.0
94.00	11944.0
95.00	77032.0
96.00	4986.0
97.00	217.0
104.00	687.0
104.80	177.0
106.00	539.0
106.70	116.0
110.80	184.0
111.80	283.0
112.80	195.0
114.70	146.0
115.90	473.0
116.90	886.0
118.00	389.0
118.90	688.0
123.80	107.0
127.90	293.0
129.00	140.0
129.70	348.0
130.80	145.0
134.80	260.0
136.60	160.0
137.10	215.0
140.90	1688.0
141.90	296.0
142.90	1622.0
143.80	113.0
144.70	115.0
145.90	245.0
147.90	316.0
155.00	146.0
156.90	144.0
158.80	122.0
170.80	171.0
172.00	729.0
174.00	66464.0
175.00	5533.0
176.00	64464.0
177.00	4415.0
178.10	102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB78