


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032919\
 Data File : VV009995.D
 Acq On : 29 Mar 2019 10:24
 Operator : SY/MD
 Sample : BFB79
 Misc : 5.00G/10mL/MSVOA_V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB79

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM032619S.M
 Title : VOC Analysis
 Last Update : Tue Apr 02 08:12:49 2019

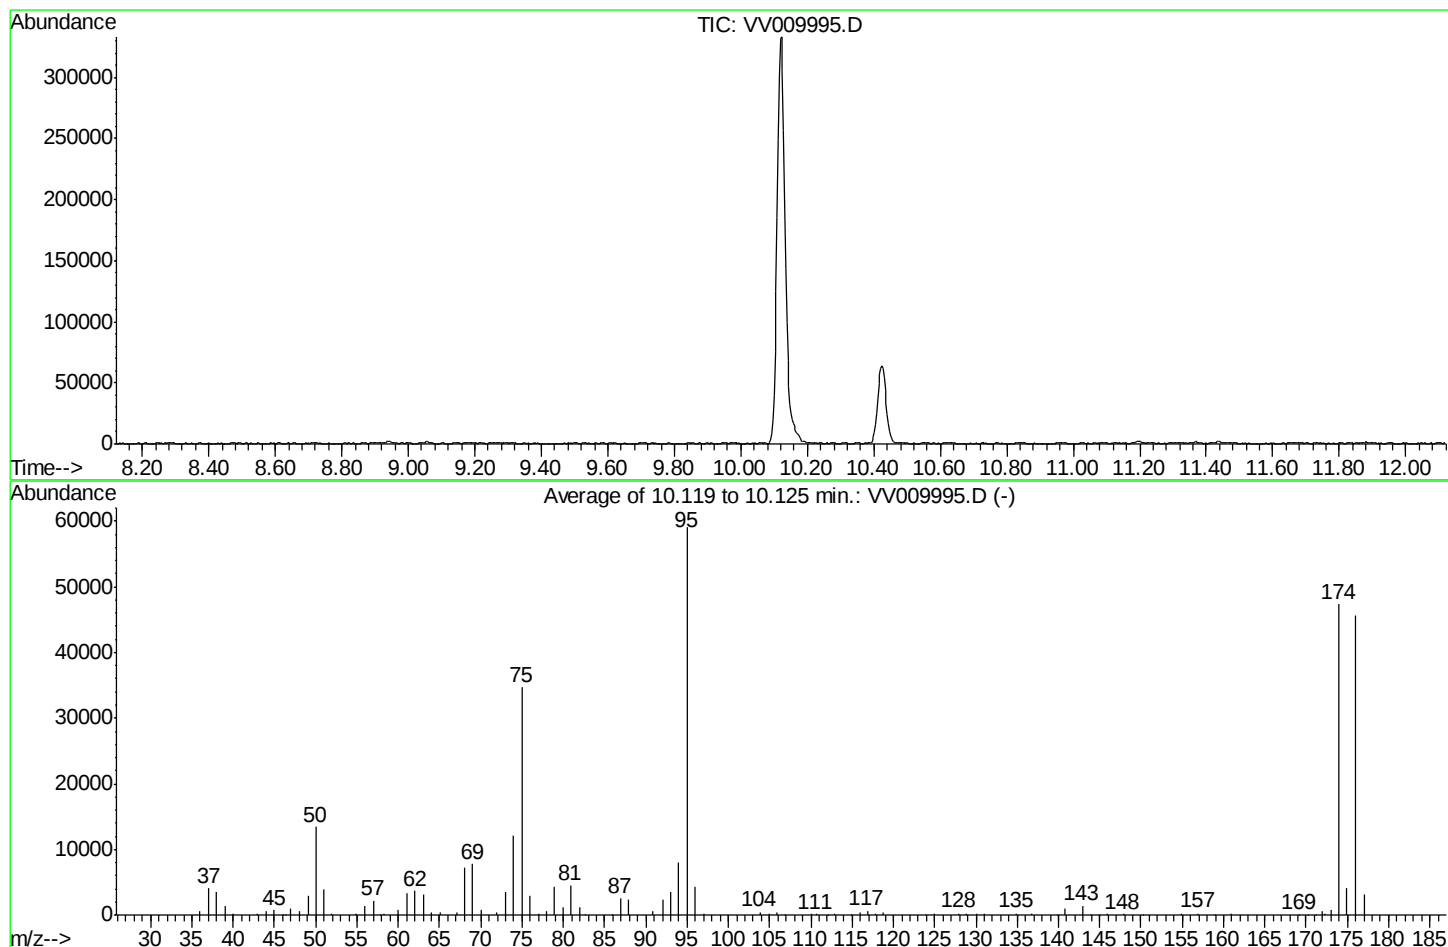

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.7	13419	PASS
75	95	30	80	58.6	34640	PASS
95	95	100	100	100.0	59082	PASS
96	95	5	9	7.2	4276	PASS
173	174	0.00	2	1.6	764	PASS
174	95	50	120	80.2	47392	PASS
175	174	5	9	8.7	4121	PASS
176	174	95	101	96.4	45693	PASS
177	176	5	9	6.7	3050	PASS

m/z	Abundance
35.90	693.0
37.00	3777.0
38.00	3359.0
39.00	1446.0
39.90	162.0
42.90	155.0
44.00	810.0
45.00	736.0
46.00	223.0
47.00	1115.0
48.00	507.0
49.10	2440.0
50.00	12195.0
51.00	3533.0
52.00	304.0
54.90	143.0
56.00	1260.0
57.00	1995.0
57.80	115.0
58.30	101.0
59.90	777.0
61.00	3199.0
62.00	3492.0
63.00	2844.0
64.00	471.0
65.00	327.0
67.00	263.0
68.00	7004.0
69.00	7315.0
70.00	723.0
71.90	352.0
73.00	3263.0
74.00	11582.0
75.00	32264.0
76.00	2796.0
77.10	198.0
78.00	526.0
78.90	3809.0
79.90	1181.0
80.90	4067.0
81.90	1083.0
82.80	110.0
86.90	2149.0
88.00	2365.0
90.80	397.0
92.00	2339.0
93.00	3405.0
94.00	7624.0
95.00	56512.0
96.00	3828.0
97.10	225.0
103.80	398.0
104.90	104.0
105.80	372.0
109.90	101.0
110.60	203.0
112.80	117.0
115.90	245.0
116.70	362.0
117.00	317.0
117.80	231.0
118.70	415.0
125.00	101.0
128.00	264.0
128.80	103.0
130.00	181.0
131.10	112.0
134.90	299.0
136.80	260.0
139.90	132.0
140.80	838.0
142.90	1395.0
145.90	121.0
150.20	102.0
154.80	133.0
157.00	159.0
158.90	113.0
160.90	113.0
169.20	104.0
170.30	138.0
171.90	398.0
172.30	457.0
174.00	46312.0
174.90	3856.0
176.00	43280.0
177.00	2836.0

Instrument :
MSVOA_V
ClientSampleId :
BFB79

m/z	Abundance
35.90	634.0
37.00	4199.0
38.00	3679.0
39.00	1502.0
40.00	176.0
42.90	210.0
43.90	851.0
45.00	779.0
45.90	194.0
47.00	1076.0
48.10	654.0
49.10	2953.0
50.00	13705.0
51.00	3994.0
51.90	305.0
54.90	263.0
56.00	1311.0
57.00	2202.0
57.80	133.0
58.20	122.0
59.90	900.0
61.00	3403.0
62.10	3712.0
63.00	3049.0
64.00	495.0
65.00	377.0
67.00	329.0
68.00	7453.0
69.00	8048.0
70.00	731.0
71.80	454.0
73.00	3512.0
74.00	12357.0
75.00	35648.0
76.00	2971.0
77.10	265.0
78.00	623.0
78.90	4262.0
79.90	1263.0
80.90	4605.0
81.90	1185.0
82.80	184.0
87.00	2478.0
88.00	2528.0
90.80	564.0
92.00	2494.0
93.00	3690.0
94.00	8350.0
95.00	60616.0
96.00	4409.0
97.10	122.0
103.80	469.0
104.90	106.0
105.80	398.0
110.00	107.0
110.60	208.0
112.10	106.0
112.80	135.0
115.90	384.0
116.70	386.0
117.00	383.0
117.80	307.0
118.80	442.0
123.90	144.0
125.00	147.0
128.00	275.0
128.80	155.0
130.00	223.0
131.10	106.0
134.90	273.0
136.80	222.0
140.90	906.0
142.90	1414.0
143.90	103.0
146.00	120.0
147.90	178.0
154.90	195.0
156.90	213.0
160.90	143.0
172.00	563.0
173.00	1260.0
174.00	48608.0
175.00	4283.0
176.00	47064.0
177.00	3173.0

Instrument :
MSVOA_V
ClientSampleId :
BFB79

m/z	Abundance
35.90	594.0
37.10	4050.0
38.00	3661.0
39.00	1435.0
40.00	150.0
42.90	202.0
43.90	771.0
45.00	819.0
45.90	120.0
46.30	101.0
47.00	920.0
48.10	622.0
49.00	3153.0
50.00	14358.0
51.00	4171.0
51.90	267.0
54.90	334.0
56.00	1312.0
57.00	2401.0
58.10	148.0
59.90	880.0
61.00	3343.0
62.10	3716.0
63.00	3356.0
64.10	463.0
65.10	369.0
67.10	370.0
68.00	7266.0
69.00	7783.0
70.00	654.0
71.80	453.0
73.00	3804.0
74.00	12410.0
75.00	36008.0
76.00	2879.0
77.10	390.0
77.90	599.0
78.90	4539.0
79.90	1283.0
80.90	4631.0
82.00	1036.0
82.70	224.0
85.80	103.0
87.00	2718.0
87.90	2300.0
90.80	719.0
92.00	2391.0
93.00	3597.0
94.00	7992.0
95.00	60120.0
96.00	4592.0
103.90	465.0
104.90	108.0
105.80	355.0
106.80	140.0
110.10	139.0
110.70	175.0
112.10	103.0
112.80	120.0
114.80	107.0
115.90	430.0
116.90	442.0
117.90	359.0
118.90	548.0
123.90	157.0
125.00	155.0
127.90	276.0
128.80	188.0
130.00	301.0
131.00	106.0
134.90	206.0
136.70	181.0
140.90	938.0
142.90	1313.0
145.00	176.0
146.00	134.0
147.90	205.0
154.90	223.0
156.90	240.0
160.90	158.0
171.10	146.0
172.00	614.0
173.00	1033.0
174.00	47256.0
175.00	4226.0
175.90	46736.0
177.00	3142.0

Instrument :
MSVOA_V
ClientSampleId :
BFB79

m/z	Abundance
44.10	228.0
46.00	107.0
82.60	158.0

Instrument :
MSVOA_V
ClientSampleId :
BFB79