

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032921\
 Data File : VV020796.D
 Acq On : 29 Mar 2021 11:42
 Operator : SY/MD
 Sample : M1816-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3G3

Quant Time: Mar 30 04:42:16 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Mar 30 04:39:28 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	647896	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	624815	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.255	152	313053	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	183566	39.91	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	79.82%
7) Chloroethane-d5	1.571	69	149632	43.03	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	86.06%
11) 1,1-Dichloroethene-d2	2.111	63	295286	34.03	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	68.06%
21) 2-Butanone-d5	3.889	46	259823	86.82	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	86.82%
24) Chloroform-d	4.352	84	414666	45.35	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.70%
26) 1,2-Dichloroethane-d4	5.034	65	285663	47.43	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.86%
32) Benzene-d6	5.053	84	782310	46.97	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.94%
36) 1,2-Dichloropropane-d6	6.072	67	237830	46.51	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	93.02%
41) Toluene-d8	7.320	98	715999	46.19	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.38%
43) trans-1,3-Dichloroprop...	7.625	79	126822	46.62	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.24%
47) 2-Hexanone-d5	8.092	63	181554	84.69	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	84.69%
57) 1,1,2,2-Tetrachloroeth...	10.220	84	310907	41.74	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	83.48%
64) 1,2-Dichlorobenzene-d4	11.632	152	307007	50.53	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.06%
Target Compounds						
13) Acetone	2.185	43	21946	10.28	ug/L	Qvalue 87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032921\
Data File : VV020796.D
Acq On : 29 Mar 2021 11:42
Operator : SY/MD
Sample : M1816-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3G3

Quant Time: Mar 30 04:42:16 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Mar 30 04:39:28 2021
Response via : Initial Calibration

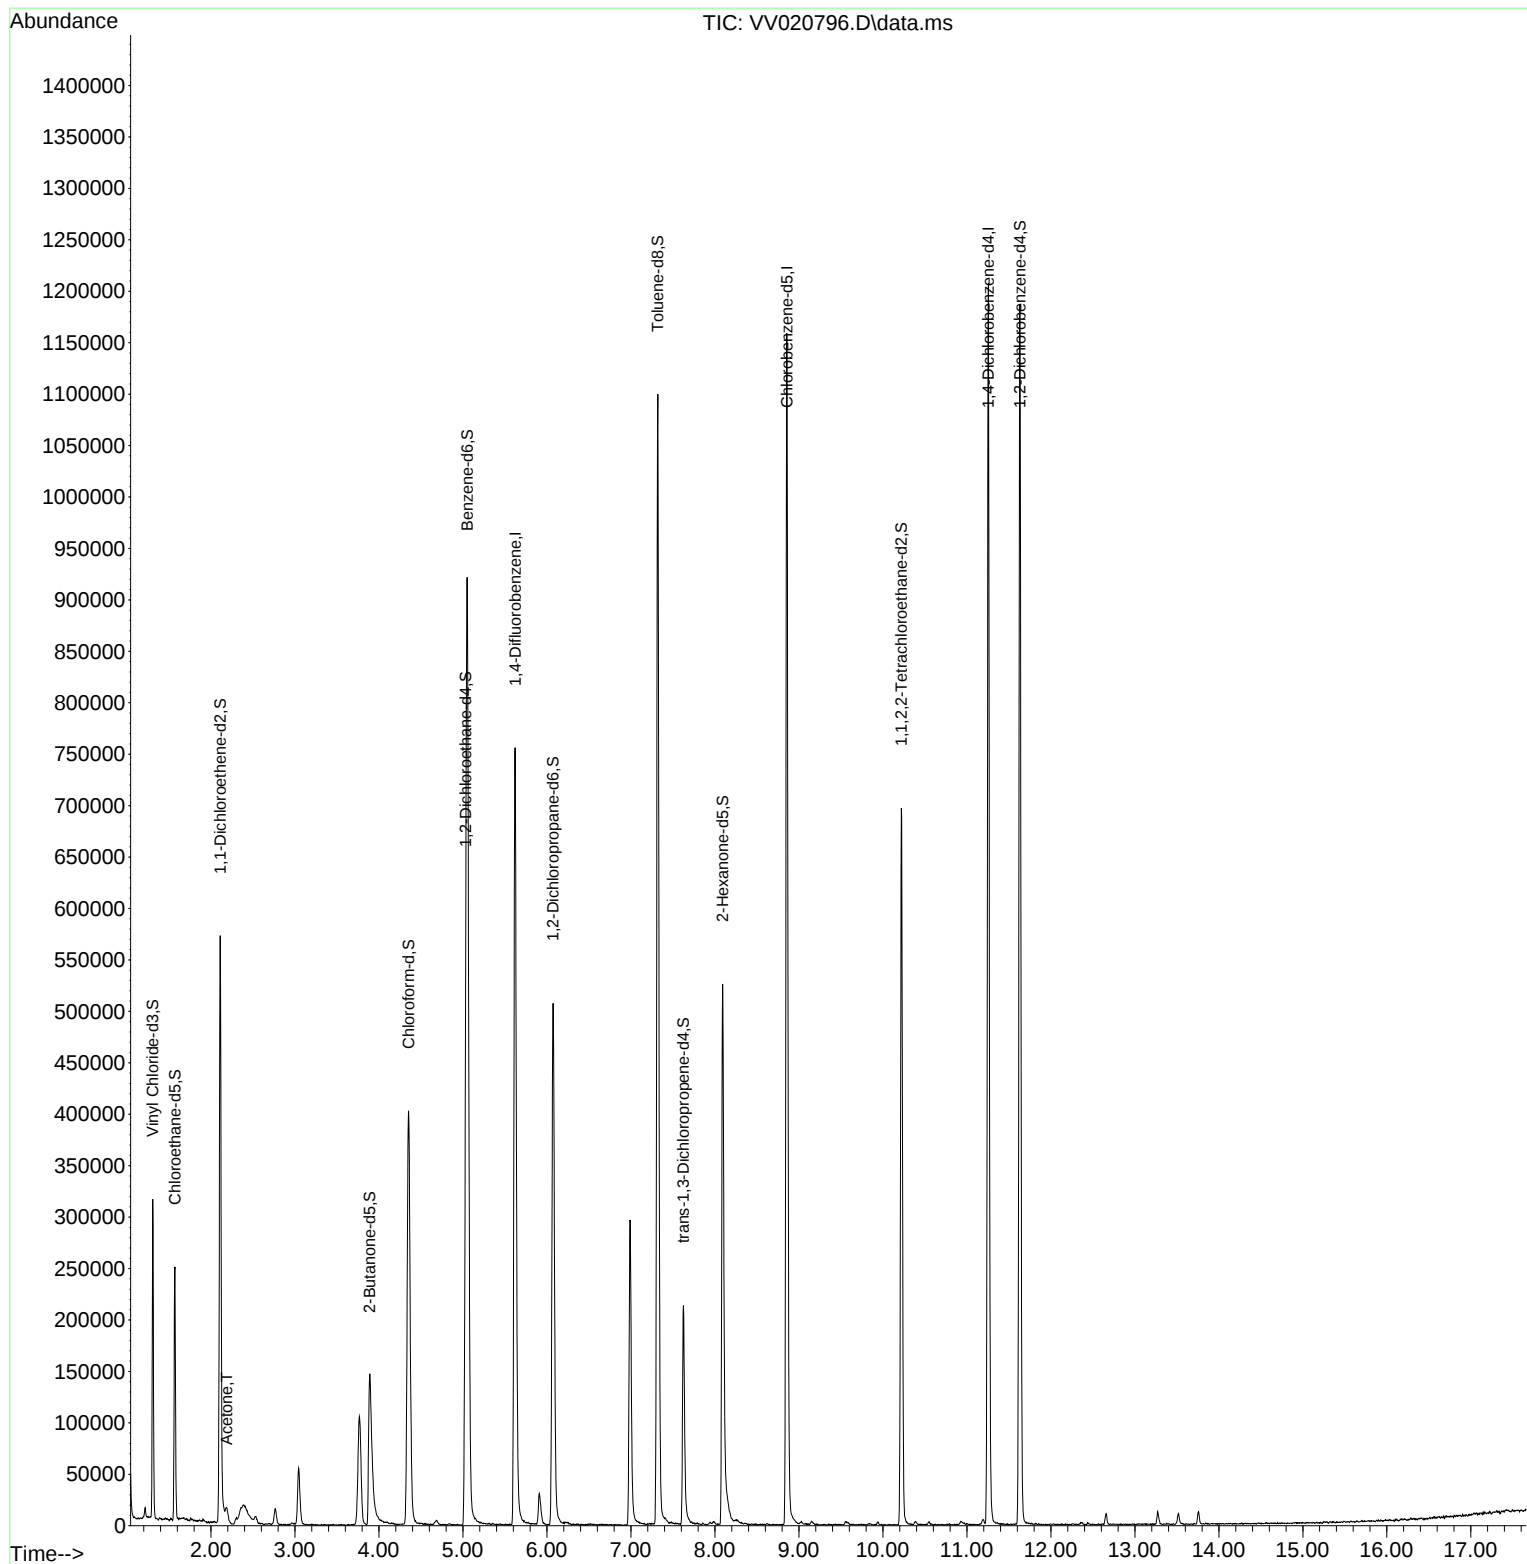

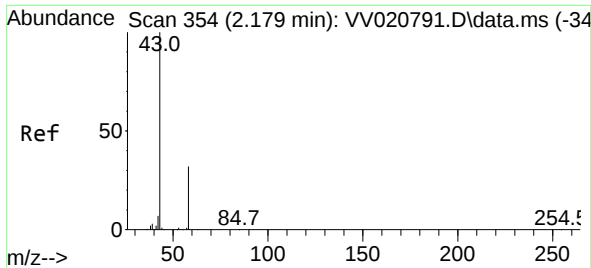

#13
Acetone
Concen: 10.28 ug/L
RT: 2.185 min Scan# 356
Delta R.T. 0.006 min
Lab File: VV020796.D
Acq: 29 Mar 2021 11:42

Instrument :
MSVOA_V
ClientSampleId :
BG3G3

Tgt Ion: 43 Resp: 21946
Ion Ratio Lower Upper
43 100
58 37.3 0.0 60.8

