

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032921\
 Data File : VV020803.D
 Acq On : 29 Mar 2021 14:27
 Operator : SY/MD
 Sample : M1816-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3G3

Quant Time: Mar 30 04:44:01 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Mar 30 04:39:28 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	661958	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	644107	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.255	152	321589	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	177593	37.79	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	75.58%
7) Chloroethane-d5	1.571	69	141808	39.91	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	79.82%
11) 1,1-Dichloroethene-d2	2.111	63	285598	32.21	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	64.42%
21) 2-Butanone-d5	3.886	46	254419	83.21	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	83.21%
24) Chloroform-d	4.352	84	415489	44.48	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.96%
26) 1,2-Dichloroethane-d4	5.037	65	288442	46.88	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.76%
32) Benzene-d6	5.053	84	769528	44.82	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.64%
36) 1,2-Dichloropropane-d6	6.072	67	236705	44.91	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	89.82%
41) Toluene-d8	7.320	98	706399	44.20	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	88.40%
43) trans-1,3-Dichloroprop...	7.625	79	122517	43.69	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.38%
47) 2-Hexanone-d5	8.092	63	176111	79.69	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	79.69%
57) 1,1,2,2-Tetrachloroeth...	10.220	84	303037	39.47	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	78.94%
64) 1,2-Dichlorobenzene-d4	11.632	152	306194	49.06	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.12%
Target Compounds						
13) Acetone	2.179	43	21278	9.76	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032921\
Data File : VV020803.D
Acq On : 29 Mar 2021 14:27
Operator : SY/MD
Sample : M1816-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3G3

Quant Time: Mar 30 04:44:01 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Mar 30 04:39:28 2021
Response via : Initial Calibration

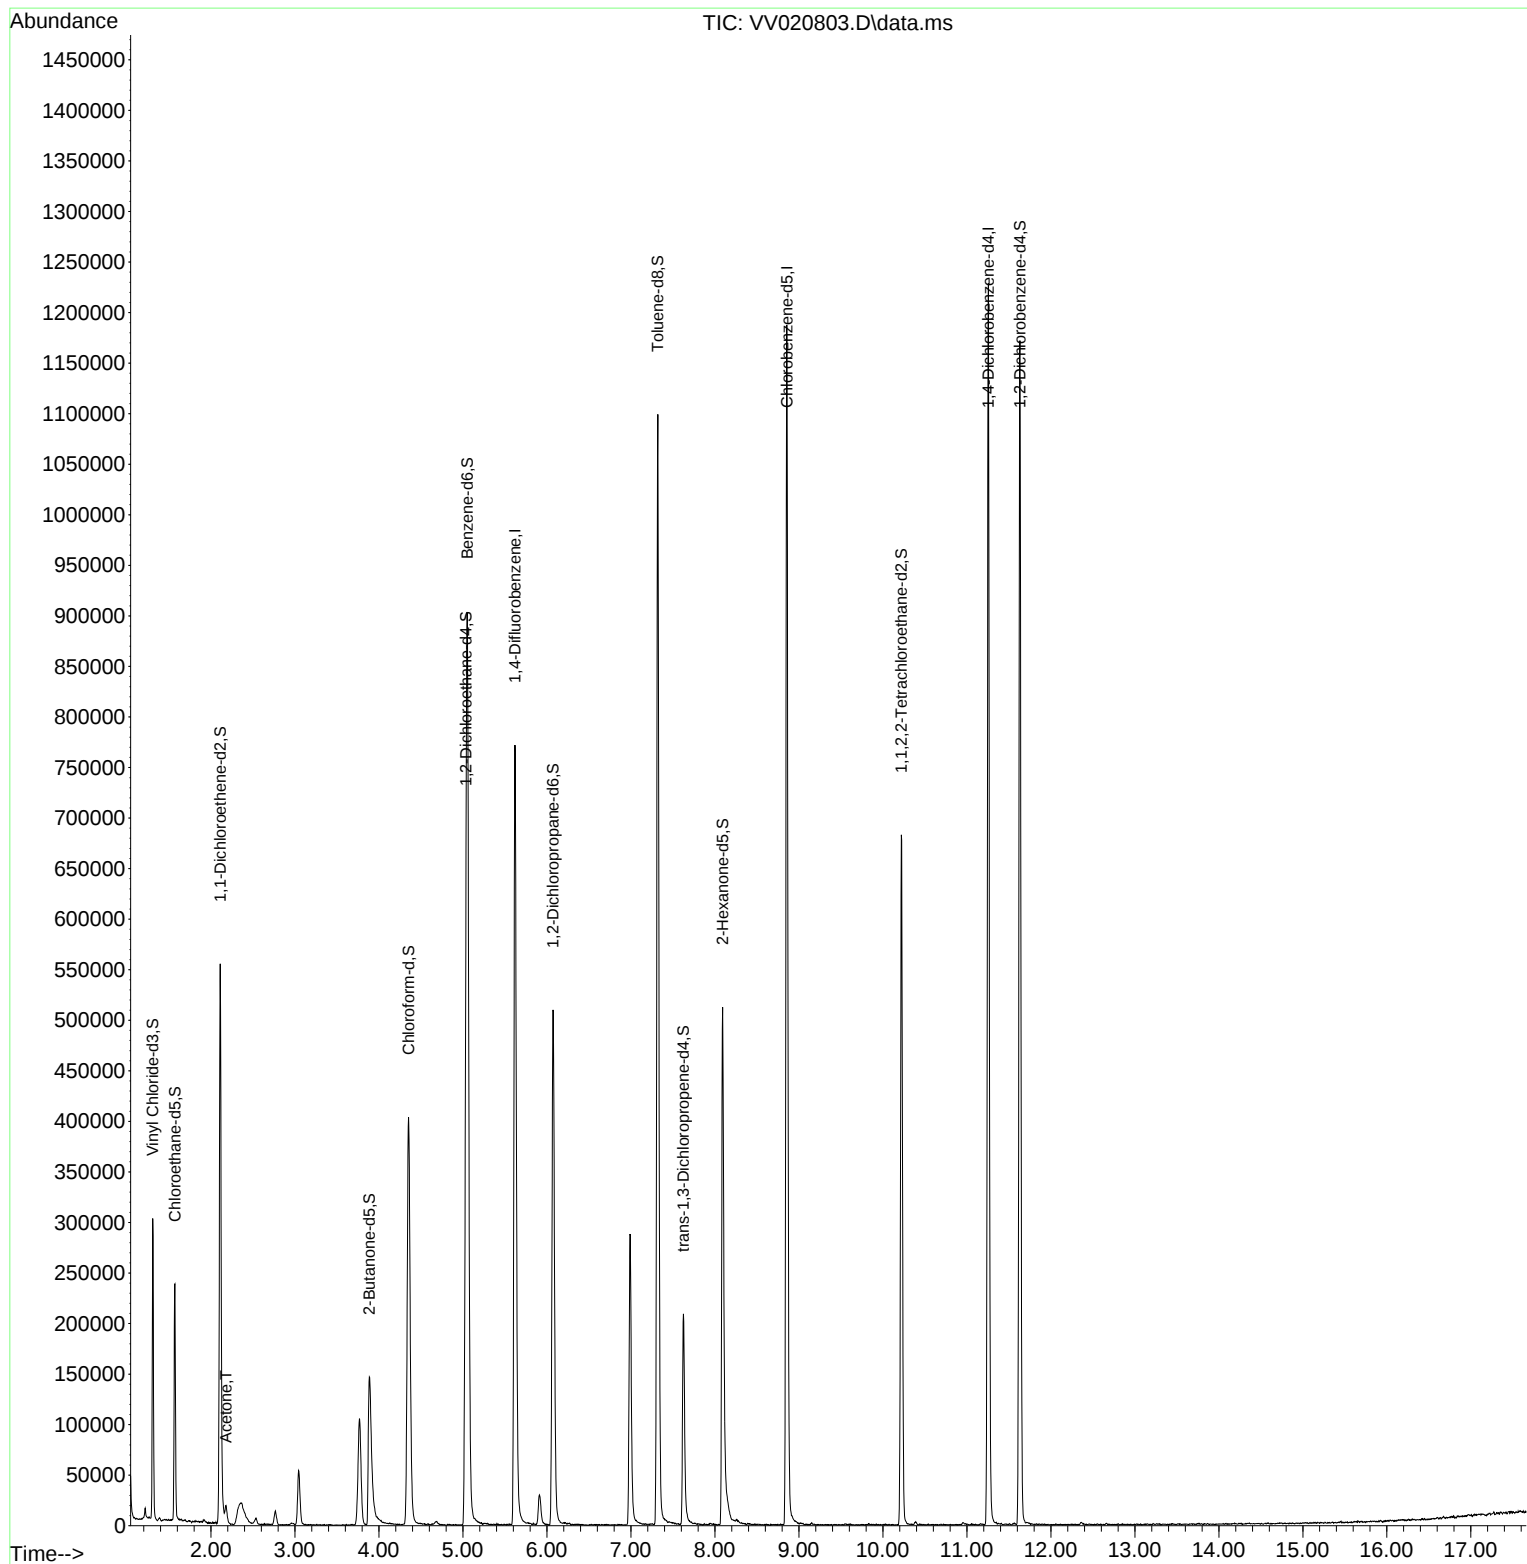

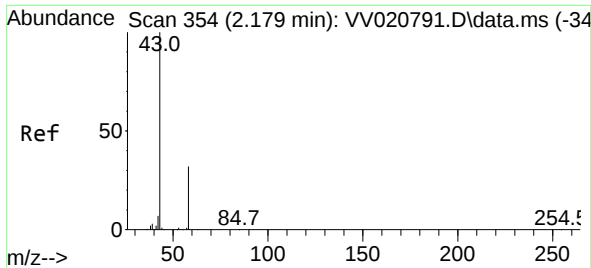

#13
 Acetone
 Concen: 9.76 ug/L
 RT: 2.179 min Scan# 354
 Delta R.T. 0.000 min
 Lab File: VV020803.D
 Acq: 29 Mar 2021 14:27

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3G3

Tgt Ion: 43 Resp: 21278
 Ion Ratio Lower Upper
 43 100
 58 30.9 0.0 60.8

