

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032921\
 Data File : VV020793.D
 Acq On : 29 Mar 2021 10:32
 Operator : SY/MD
 Sample : VV0329WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK83

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020793.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	94	rVB	292781	292978	12.26%	1.597%
2	1.571	157	165	181	rBV	244025	275529	11.53%	1.502%
3	2.111	323	333	362	rVB	559589	842813	35.26%	4.594%
4	2.294	384	390	396	rBV4	2443	3404	0.14%	0.019%
5	2.423	427	430	436	rBV3	808	473	0.02%	0.003%
6	2.510	451	457	467	rVB5	2981	4841	0.20%	0.026%
7	2.580	475	479	482	rBV3	612	533	0.02%	0.003%
8	2.629	492	494	496	rBV3	364	254	0.01%	0.001%
9	2.712	517	520	522	rBV2	628	365	0.02%	0.002%
10	2.760	532	535	536	rBV2	869	452	0.02%	0.002%
11	2.812	548	551	555	rVB2	595	401	0.02%	0.002%
12	2.847	555	562	566	rBV5	638	657	0.03%	0.004%
13	2.899	572	578	580	rBV2	546	459	0.02%	0.003%
14	2.957	593	596	598	rBV2	599	394	0.02%	0.002%
15	3.005	605	611	617	rBV4	682	781	0.03%	0.004%
16	3.034	617	620	621	rBV2	931	421	0.02%	0.002%
17	3.259	688	690	695	rVB	437	307	0.01%	0.002%
18	3.304	701	704	707	rVB2	566	353	0.01%	0.002%
19	3.323	707	710	711	rBV2	477	222	0.01%	0.001%
20	3.365	718	723	728	rVB2	591	480	0.02%	0.003%
21	3.455	749	751	756	rVB3	447	247	0.01%	0.001%
22	3.477	756	758	763	rVB2	710	424	0.02%	0.002%
23	3.513	767	769	772	rBV3	401	273	0.01%	0.001%
24	3.593	791	794	797	rBV2	355	253	0.01%	0.001%
25	3.609	797	799	801	rVV2	384	218	0.01%	0.001%
26	3.632	804	806	809	rVV3	563	330	0.01%	0.002%
27	3.728	833	836	839	rBV	477	383	0.02%	0.002%
28	3.889	875	886	923	rBV	143624	430098	17.99%	2.344%
29	4.352	1015	1030	1054	rBV	409011	1008263	42.18%	5.496%
30	4.767	1157	1159	1162	rBV2	547	241	0.01%	0.001%
31	4.821	1173	1176	1178	rBV3	614	389	0.02%	0.002%
32	4.931	1207	1210	1211	rBV	544	332	0.01%	0.002%
33	5.050	1228	1247	1275	rBV2	929177	2390349	100.00%	13.029%
34	5.442	1366	1369	1374	rBV3	456	427	0.02%	0.002%
35	5.468	1374	1377	1378	rBV	617	357	0.01%	0.002%
36	5.558	1402	1405	1407	rVB	575	267	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032921\
 Data File : VV020793.D
 Acq On : 29 Mar 2021 10:32
 Operator : SY/MD
 Sample : VV0329WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK83

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	5.622	1409	1425	1454	rBV	735024	1468330	61.43%	8.003%
38	5.911	1508	1515	1531	rVB4	16974	34639	1.45%	0.189%
39	6.024	1549	1550	1551	rBV4	774	269	0.01%	0.001%
40	6.072	1551	1565	1586	rVV	512159	1052591	44.04%	5.737%
41	6.320	1640	1642	1646	rVB4	971	634	0.03%	0.003%
42	6.358	1649	1654	1658	rVB5	1310	1104	0.05%	0.006%
43	6.378	1658	1660	1662	rVB2	607	236	0.01%	0.001%
44	6.407	1665	1669	1671	rBV3	558	365	0.02%	0.002%
45	6.429	1673	1676	1680	rBV3	653	565	0.02%	0.003%
46	6.561	1714	1717	1721	rBV2	562	468	0.02%	0.003%
47	6.583	1721	1724	1730	rVB4	843	883	0.04%	0.005%
48	6.648	1739	1744	1746	rBV5	889	721	0.03%	0.004%
49	6.699	1755	1760	1761	rBV2	729	521	0.02%	0.003%
50	6.847	1803	1806	1810	rVB3	674	580	0.02%	0.003%
51	6.866	1810	1812	1815	rBV3	482	323	0.01%	0.002%
52	6.908	1823	1825	1828	rBV2	361	238	0.01%	0.001%
53	6.989	1839	1850	1881	rBV	294388	546650	22.87%	2.980%
54	7.210	1917	1919	1924	rBV4	892	838	0.04%	0.005%
55	7.320	1941	1953	1974	rBV	1105843	1903516	79.63%	10.375%
56	7.625	2038	2048	2079	rBV	215026	376102	15.73%	2.050%
57	7.976	2154	2157	2158	rBV2	1853	1298	0.05%	0.007%
58	8.030	2170	2174	2176	rBV3	911	717	0.03%	0.004%
59	8.091	2182	2193	2229	rBV	537553	1001932	41.92%	5.461%
60	8.558	2336	2338	2341	rVB3	569	326	0.01%	0.002%
61	8.615	2352	2356	2359	rBV3	1007	754	0.03%	0.004%
62	8.664	2369	2371	2374	rBV2	480	281	0.01%	0.002%
63	8.680	2374	2376	2381	rVB3	562	321	0.01%	0.002%
64	8.712	2384	2386	2389	rBV2	541	319	0.01%	0.002%
65	8.776	2403	2406	2409	rVB3	661	422	0.02%	0.002%
66	8.792	2409	2411	2413	rBV2	434	238	0.01%	0.001%
67	8.857	2418	2431	2462	rBV	1135754	1846039	77.23%	10.062%
68	9.201	2536	2538	2540	rBV2	578	297	0.01%	0.002%
69	9.287	2562	2565	2566	rBV	371	220	0.01%	0.001%
70	9.451	2611	2616	2621	rVB3	643	546	0.02%	0.003%
71	9.619	2666	2668	2671	rBV	548	247	0.01%	0.001%
72	9.641	2671	2675	2680	rVB4	959	971	0.04%	0.005%
73	9.673	2680	2685	2687	rBV2	500	450	0.02%	0.002%
74	9.693	2689	2691	2695	rBV3	587	334	0.01%	0.002%
75	9.812	2725	2728	2730	rVB2	680	375	0.02%	0.002%
76	9.850	2735	2740	2744	rBV3	875	802	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032921\
 Data File : VV020793.D
 Acq On : 29 Mar 2021 10:32
 Operator : SY/MD
 Sample : VV0329WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK83

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

77	9.908	2755	2758	2759	rBV	1025	436	0.02%	0.002%
78	10.078	2809	2811	2813	rBV2	716	293	0.01%	0.002%
79	10.120	2821	2824	2826	rBV2	444	332	0.01%	0.002%
80	10.220	2843	2855	2877	rBV	733120	1153536	48.26%	6.287%
81	10.342	2891	2893	2900	rVB5	912	728	0.03%	0.004%
82	10.390	2906	2908	2910	rBV2	572	298	0.01%	0.002%
83	10.455	2926	2928	2931	rBV2	584	303	0.01%	0.002%
84	10.635	2982	2984	2987	rBV2	465	267	0.01%	0.001%
85	10.860	3051	3054	3057	rVB3	998	653	0.03%	0.004%
86	10.931	3070	3076	3080	rBV4	1755	2110	0.09%	0.012%
87	10.979	3089	3091	3095	rVB2	545	300	0.01%	0.002%
88	11.001	3095	3098	3099	rBV2	446	233	0.01%	0.001%
89	11.162	3144	3148	3149	rBV	701	408	0.02%	0.002%
90	11.172	3149	3151	3152	rBV	737	326	0.01%	0.002%
91	11.255	3165	3177	3207	rBV	1163071	1807859	75.63%	9.854%
92	11.541	3263	3266	3267	rBV	965	537	0.02%	0.003%
93	11.631	3281	3294	3313	rBV	1200561	1863750	77.97%	10.158%
94	11.921	3382	3384	3387	rBV2	803	478	0.02%	0.003%
95	11.982	3398	3403	3404	rBV2	630	542	0.02%	0.003%
96	12.098	3436	3439	3442	rBV4	719	380	0.02%	0.002%
97	13.278	3800	3806	3816	rVB8	2170	3128	0.13%	0.017%
98	13.490	3868	3872	3874	rBV2	1029	735	0.03%	0.004%
99	13.760	3950	3956	3959	rBV4	2487	2894	0.12%	0.016%
100	14.503	4184	4187	4189	rBV3	1458	888	0.04%	0.005%




Sum of corrected areas: 18346844

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032921\
Data File : VV020793.D
Acq On : 29 Mar 2021 10:32
Operator : SY/MD
Sample : VV0329WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK83

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

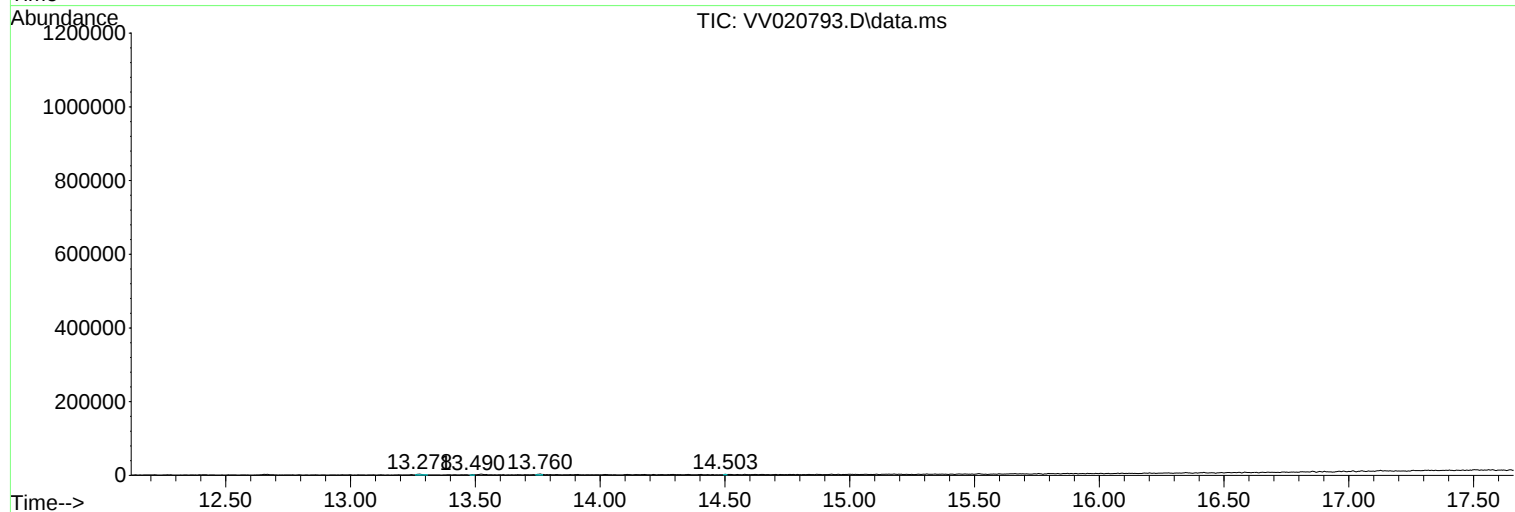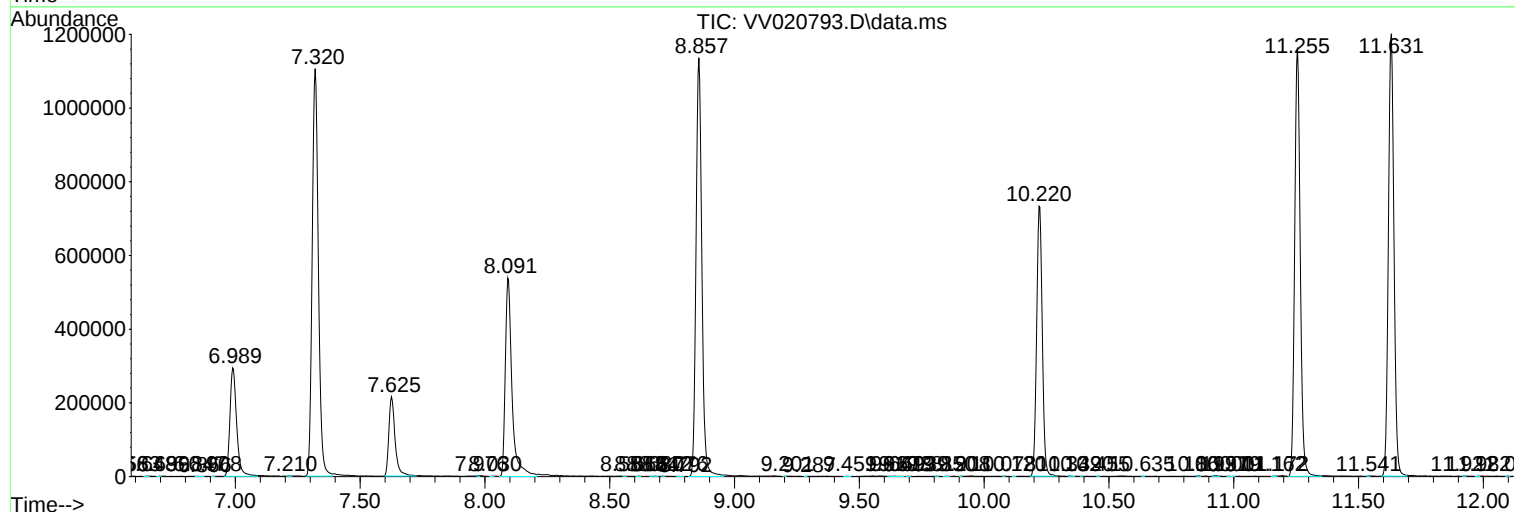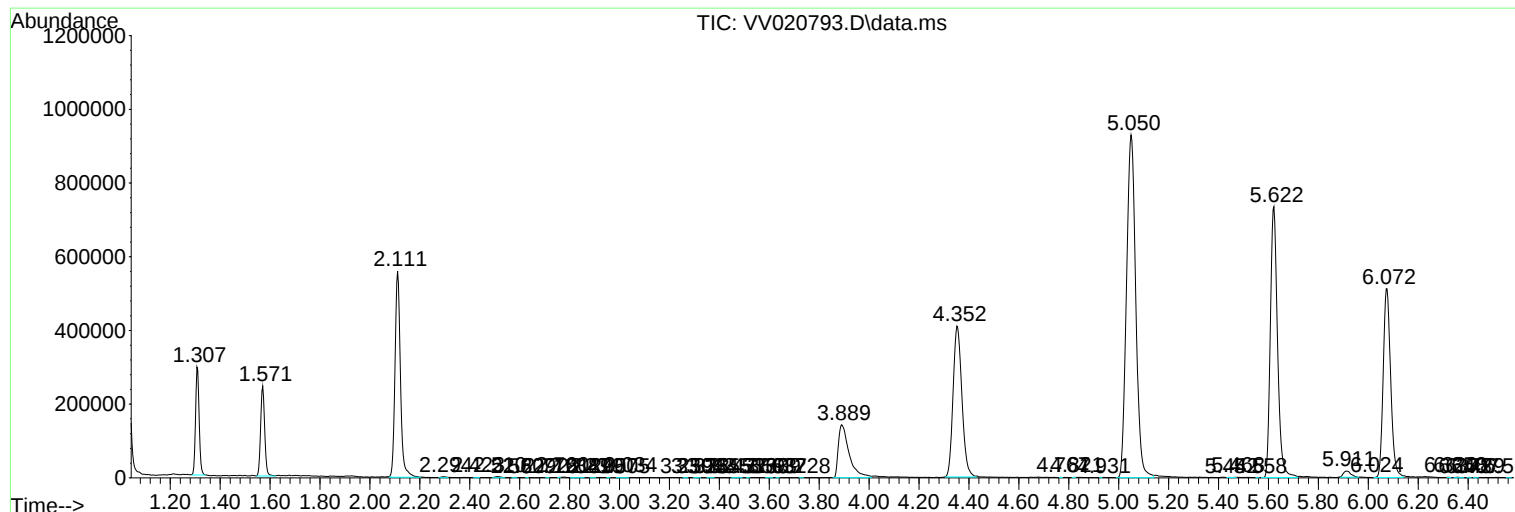

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032921\
Data File : VV020793.D
Acq On : 29 Mar 2021 10:32
Operator : SY/MD
Sample : VV0329WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK83

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032921\
Data File : VV020793.D
Acq On : 29 Mar 2021 10:32
Operator : SY/MD
Sample : VV0329WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK83

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
