

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032921\
 Data File : VV020799.D
 Acq On : 29 Mar 2021 12:53
 Operator : SY/MD
 Sample : M1824-15RE
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4W0RE

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020799.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	96	rVB	570607	567762	12.41%	1.868%
2	1.568	157	164	179	rVB	463076	522457	11.42%	1.719%
3	2.111	321	333	363	rVB	1079060	1608500	35.16%	5.292%
4	2.507	450	456	459	rBV4	2053	2221	0.05%	0.007%
5	2.568	474	475	476	rBV4	259	86	0.00%	0.000%
6	2.658	500	503	506	rVB2	509	252	0.01%	0.001%
7	2.677	506	509	512	rBV3	672	485	0.01%	0.002%
8	2.732	522	526	529	rBV2	519	469	0.01%	0.002%
9	2.761	531	535	537	rBV4	980	825	0.02%	0.003%
10	2.847	560	562	564	rBV	269	154	0.00%	0.001%
11	2.954	592	595	597	rBV	603	345	0.01%	0.001%
12	2.963	597	598	600	rBV3	717	309	0.01%	0.001%
13	3.037	618	621	623	rBV3	624	443	0.01%	0.001%
14	3.188	665	668	672	rVB	536	370	0.01%	0.001%
15	3.211	672	675	676	rBV	374	232	0.01%	0.001%
16	3.220	676	678	681	rVV2	536	249	0.01%	0.001%
17	3.233	681	682	686	rVB3	323	191	0.00%	0.001%
18	3.256	686	689	691	rBV2	429	267	0.01%	0.001%
19	3.281	695	697	701	rVV2	429	209	0.00%	0.001%
20	3.320	708	709	710	rBV2	228	48	0.00%	0.000%
21	3.359	717	721	724	rBV2	463	322	0.01%	0.001%
22	3.397	726	733	737	rBV3	528	595	0.01%	0.002%
23	3.468	753	755	757	rVB2	213	63	0.00%	0.000%
24	3.490	761	762	764	rBV2	257	113	0.00%	0.000%
25	3.545	776	779	781	rBV3	538	274	0.01%	0.001%
26	3.609	796	799	802	rBV2	465	368	0.01%	0.001%
27	3.651	810	812	813	rBV	154	65	0.00%	0.000%
28	3.658	813	814	816	rVV	197	70	0.00%	0.000%
29	3.696	824	826	831	rVB2	698	477	0.01%	0.002%
30	3.728	831	836	838	rBV3	475	434	0.01%	0.001%
31	3.757	844	845	848	rBV	335	181	0.00%	0.001%
32	3.793	854	856	860	rVB2	510	325	0.01%	0.001%
33	3.822	863	865	868	rBV	467	262	0.01%	0.001%
34	3.838	868	870	872	rVB3	608	200	0.00%	0.001%
35	3.883	872	884	918	rBV	303710	854547	18.68%	2.811%
36	4.352	1013	1030	1055	rBV2	793527	1939744	42.41%	6.382%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032921\
 Data File : VV020799.D
 Acq On : 29 Mar 2021 12:53
 Operator : SY/MD
 Sample : M1824-15RE
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4W0RE

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	4.748	1150	1153	1160	rBV6	689	846	0.02%	0.003%
38	4.896	1197	1199	1202	rVB2	468	225	0.00%	0.001%
39	4.918	1202	1206	1207	rVV2	605	378	0.01%	0.001%
40	4.928	1207	1209	1211	rVV2	752	345	0.01%	0.001%
41	4.953	1215	1217	1220	rBV2	454	216	0.00%	0.001%
42	5.050	1228	1247	1276	rBV2	1784710	4574198	100.00%	15.049%
43	5.503	1386	1388	1392	rBV4	850	640	0.01%	0.002%
44	5.561	1403	1406	1411	rBV5	951	771	0.02%	0.003%
45	5.622	1412	1425	1454	rBV	673626	1362181	29.78%	4.481%
46	5.912	1506	1515	1533	rVB5	29232	64569	1.41%	0.212%
47	5.998	1540	1542	1545	rVB3	942	508	0.01%	0.002%
48	6.021	1547	1549	1551	rBV2	880	463	0.01%	0.002%
49	6.072	1551	1565	1591	rBV	986849	2004970	43.83%	6.596%
50	6.310	1637	1639	1640	rBV2	846	299	0.01%	0.001%
51	6.339	1646	1648	1649	rBV	581	255	0.01%	0.001%
52	6.381	1659	1661	1664	rVB2	854	374	0.01%	0.001%
53	6.400	1664	1667	1668	rBV	590	299	0.01%	0.001%
54	6.449	1677	1682	1683	rBV2	860	563	0.01%	0.002%
55	6.551	1712	1714	1716	rBV2	393	250	0.01%	0.001%
56	6.622	1734	1736	1738	rBV3	585	273	0.01%	0.001%
57	6.635	1738	1740	1742	rBV	885	459	0.01%	0.002%
58	6.699	1758	1760	1762	rBV2	715	261	0.01%	0.001%
59	6.760	1777	1779	1785	rBV3	549	423	0.01%	0.001%
60	6.838	1801	1803	1804	rBV	492	197	0.00%	0.001%
61	6.989	1838	1850	1882	rBV	596348	1080580	23.62%	3.555%
62	7.320	1940	1953	1977	rBV	2219835	3750115	81.98%	12.338%
63	7.622	2037	2047	2074	rBV	438412	748520	16.36%	2.463%
64	8.092	2181	2193	2231	rBV	1143581	2024567	44.26%	6.661%
65	8.551	2334	2336	2337	rBV	736	344	0.01%	0.001%
66	8.677	2372	2375	2377	rBV2	913	488	0.01%	0.002%
67	8.789	2408	2410	2415	rBV2	567	499	0.01%	0.002%
68	8.857	2419	2431	2453	rBV	1049419	1712985	37.45%	5.636%
69	9.346	2581	2583	2586	rBV	870	448	0.01%	0.001%
70	9.580	2654	2656	2659	rBV3	498	312	0.01%	0.001%
71	9.661	2679	2681	2683	rBV	347	183	0.00%	0.001%
72	9.674	2683	2685	2687	rVB2	317	145	0.00%	0.000%
73	9.809	2724	2727	2729	rBV2	438	242	0.01%	0.001%
74	9.825	2730	2732	2733	rVV	786	180	0.00%	0.001%
75	9.841	2734	2737	2742	rVB4	851	653	0.01%	0.002%
76	9.863	2742	2744	2747	rBV	449	277	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032921\
 Data File : VV020799.D
 Acq On : 29 Mar 2021 12:53
 Operator : SY/MD
 Sample : M1824-15RE
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4W0RE

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

77	9.940	2763	2768	2770	rBV4	956	795	0.02%	0.003%
78	9.989	2780	2783	2785	rVB	651	324	0.01%	0.001%
79	10.014	2789	2791	2795	rVB	547	302	0.01%	0.001%
80	10.043	2795	2800	2802	rBV2	861	832	0.02%	0.003%
81	10.075	2808	2810	2812	rBV	535	193	0.00%	0.001%
82	10.220	2842	2855	2881	rBV	1426207	2229275	48.74%	7.334%
83	10.580	2964	2967	2968	rBV	732	360	0.01%	0.001%
84	10.805	3036	3037	3041	rBV2	469	379	0.01%	0.001%
85	10.857	3049	3053	3061	rBV5	2175	2957	0.06%	0.010%
86	11.175	3149	3152	3155	rBV4	984	774	0.02%	0.003%
87	11.255	3166	3177	3200	rBV	1085404	1678083	36.69%	5.521%
88	11.542	3263	3266	3268	rBV	1319	738	0.02%	0.002%
89	11.632	3281	3294	3314	rBV	2350328	3641110	79.60%	11.979%
90	13.519	3877	3881	3884	rBV5	1266	1376	0.03%	0.005%




Sum of corrected areas: 30395913

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032921\
Data File : VV020799.D
Acq On : 29 Mar 2021 12:53
Operator : SY/MD
Sample : M1824-15RE
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4W0RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

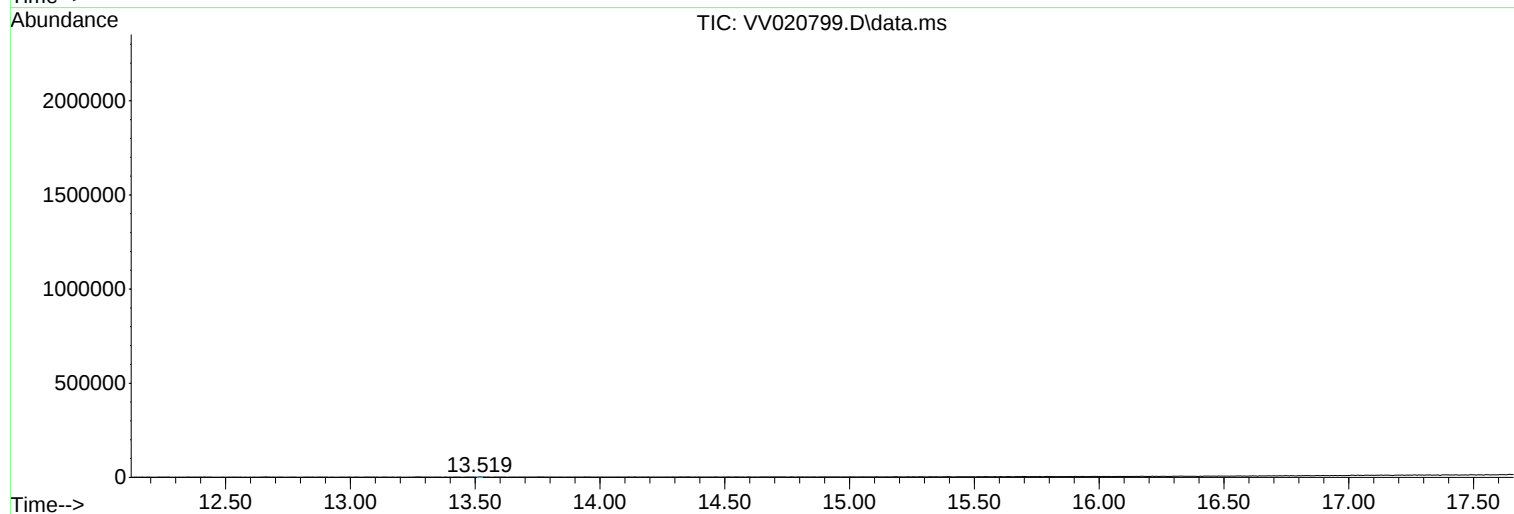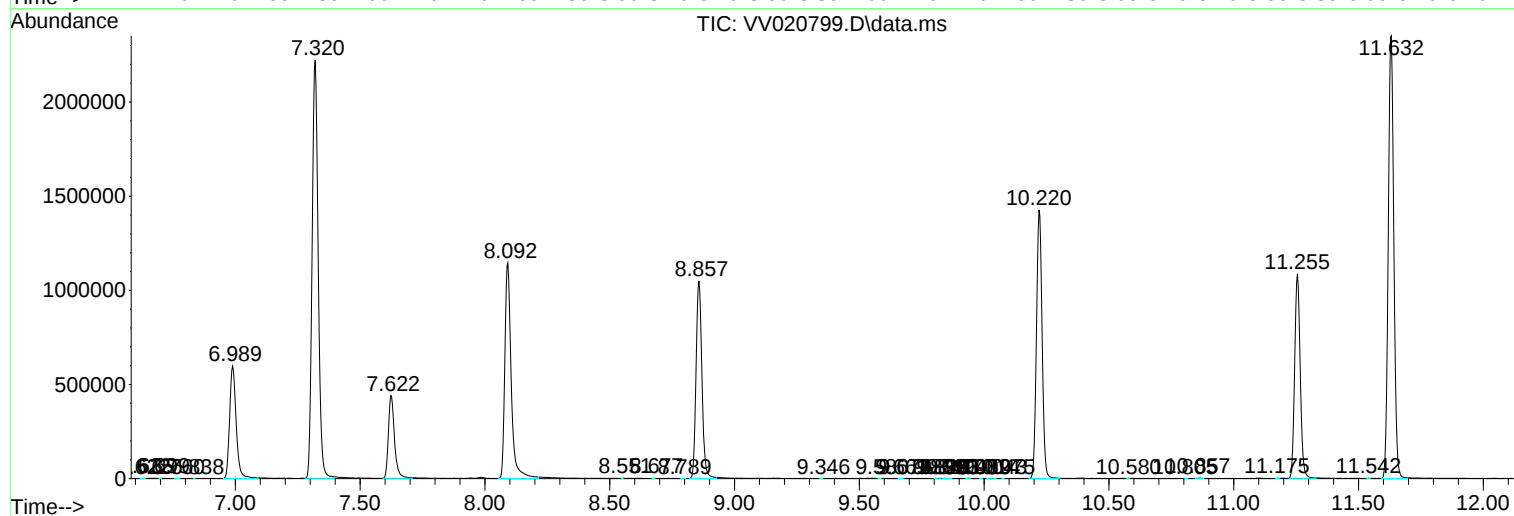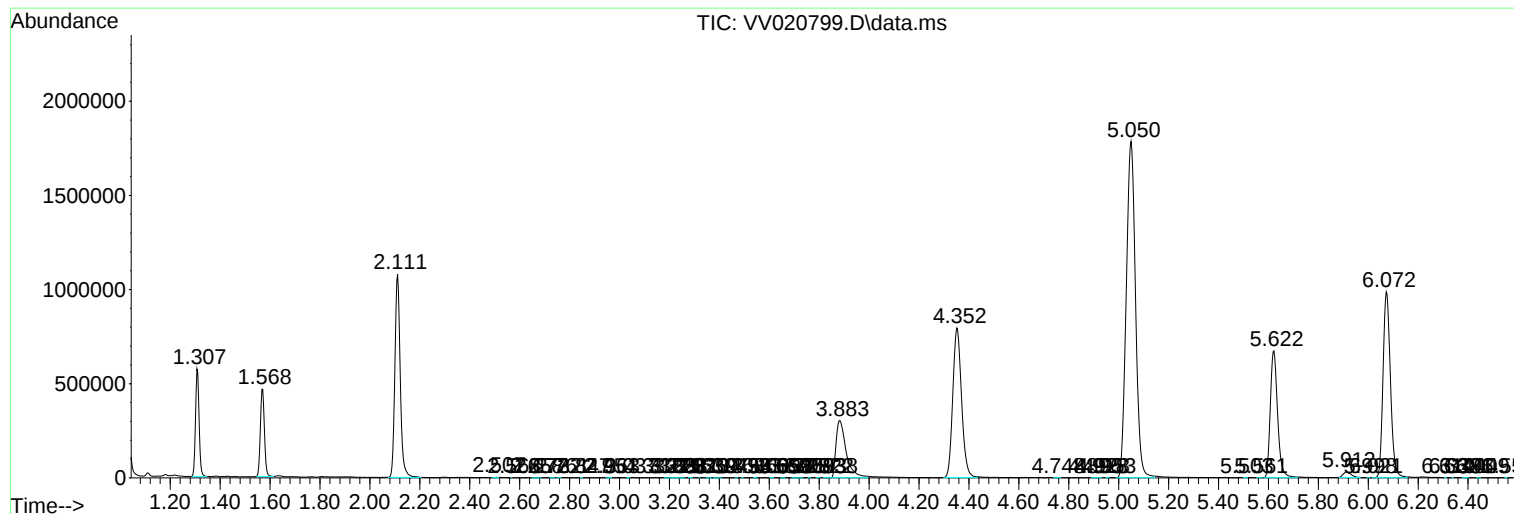

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032921\
Data File : VV020799.D
Acq On : 29 Mar 2021 12:53
Operator : SY/MD
Sample : M1824-15RE
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4W0RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032921\
Data File : VV020799.D
Acq On : 29 Mar 2021 12:53
Operator : SY/MD
Sample : M1824-15RE
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4W0RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------