

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032921\
 Data File : VV020807.D
 Acq On : 29 Mar 2021 16:19
 Operator : SY/MD
 Sample : M1784-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020807.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	98	rVB	286229	279881	11.72%	1.536%
2	1.568	157	164	175	rBV	239805	264052	11.06%	1.450%
3	2.111	322	333	363	rVB	546982	823707	34.49%	4.522%
4	2.397	416	422	425	rBV2	932	663	0.03%	0.004%
5	2.677	507	509	513	rVB2	624	393	0.02%	0.002%
6	2.709	516	519	521	rBV3	493	267	0.01%	0.001%
7	2.780	538	541	545	rBV2	810	670	0.03%	0.004%
8	2.809	548	550	552	rBV3	463	211	0.01%	0.001%
9	2.844	560	561	564	rBV	319	186	0.01%	0.001%
10	2.937	588	590	591	rBV	583	222	0.01%	0.001%
11	2.953	594	595	602	rVB3	624	481	0.02%	0.003%
12	3.056	625	627	630	rVB2	525	237	0.01%	0.001%
13	3.114	643	645	649	rBV3	482	390	0.02%	0.002%
14	3.178	662	665	667	rBV	313	200	0.01%	0.001%
15	3.198	669	671	675	rVV	481	218	0.01%	0.001%
16	3.378	725	727	730	rVB	542	237	0.01%	0.001%
17	3.407	734	736	741	rVB2	558	358	0.01%	0.002%
18	3.449	747	749	753	rVB2	494	258	0.01%	0.001%
19	3.519	769	771	776	rVB2	387	282	0.01%	0.002%
20	3.539	776	777	780	rVB2	548	220	0.01%	0.001%
21	3.558	780	783	785	rBV	338	197	0.01%	0.001%
22	3.580	787	790	793	rVV3	509	290	0.01%	0.002%
23	3.596	793	795	801	rVV3	394	346	0.01%	0.002%
24	3.703	825	828	830	rVB2	537	267	0.01%	0.001%
25	3.751	840	843	848	rVB2	505	342	0.01%	0.002%
26	3.773	848	850	854	rVB3	289	174	0.01%	0.001%
27	3.812	859	862	868	rVB2	488	404	0.02%	0.002%
28	3.847	868	873	875	rBV3	598	531	0.02%	0.003%
29	3.886	875	885	917	rBV	160317	439933	18.42%	2.415%
30	4.285	1005	1009	1011	rBV3	675	598	0.03%	0.003%
31	4.352	1015	1030	1059	rVV	408225	1011262	42.34%	5.551%
32	4.715	1141	1143	1150	rVB4	857	863	0.04%	0.005%
33	4.776	1160	1162	1167	rBV4	580	484	0.02%	0.003%
34	4.809	1170	1172	1176	rVV3	705	391	0.02%	0.002%
35	4.828	1176	1178	1182	rVB2	874	575	0.02%	0.003%
36	4.854	1182	1186	1188	rBV2	279	179	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032921\
 Data File : VV020807.D
 Acq On : 29 Mar 2021 16:19
 Operator : SY/MD
 Sample : M1784-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	4.870	1188	1191	1194	rBV2	462	403	0.02%	0.002%
38	4.889	1195	1197	1201	rVB2	585	243	0.01%	0.001%
39	4.918	1204	1206	1208	rBV	498	251	0.01%	0.001%
40	5.050	1230	1247	1284	rVV2	923343	2388472	100.00%	13.112%
41	5.384	1349	1351	1353	rBV2	391	173	0.01%	0.001%
42	5.477	1377	1380	1382	rBV3	851	567	0.02%	0.003%
43	5.561	1404	1406	1407	rBV2	529	223	0.01%	0.001%
44	5.622	1412	1425	1457	rBV	704989	1419529	59.43%	7.793%
45	5.911	1506	1515	1531	rVB3	19168	37402	1.57%	0.205%
46	6.072	1550	1565	1590	rBV	514965	1049716	43.95%	5.762%
47	6.394	1663	1665	1669	rBV	706	581	0.02%	0.003%
48	6.436	1676	1678	1681	rBV2	1001	422	0.02%	0.002%
49	6.490	1692	1695	1699	rBV4	360	282	0.01%	0.002%
50	6.516	1699	1703	1704	rBV2	637	337	0.01%	0.002%
51	6.648	1739	1744	1746	rBV3	1129	964	0.04%	0.005%
52	6.767	1774	1781	1784	rBV4	877	1046	0.04%	0.006%
53	6.786	1784	1787	1789	rBV3	533	335	0.01%	0.002%
54	6.834	1800	1802	1804	rBV2	510	218	0.01%	0.001%
55	6.866	1809	1812	1815	rBV2	344	207	0.01%	0.001%
56	6.895	1818	1821	1824	rBV	353	214	0.01%	0.001%
57	6.940	1831	1835	1838	rBV2	437	291	0.01%	0.002%
58	6.989	1838	1850	1875	rBV	289427	534866	22.39%	2.936%
59	7.320	1941	1953	1977	rBV	1113969	1900175	79.56%	10.431%
60	7.587	2035	2036	2038	rBV2	664	242	0.01%	0.001%
61	7.625	2038	2048	2071	rBV	215085	374396	15.68%	2.055%
62	8.030	2171	2174	2176	rBV3	589	407	0.02%	0.002%
63	8.091	2183	2193	2230	rBV	563149	1045018	43.75%	5.737%
64	8.423	2294	2296	2298	rBV2	594	261	0.01%	0.001%
65	8.529	2327	2329	2331	rBV2	533	238	0.01%	0.001%
66	8.789	2406	2410	2412	rBV2	481	364	0.02%	0.002%
67	8.857	2419	2431	2459	rBV	1127962	1817391	76.09%	9.977%
68	9.156	2521	2524	2527	rBV3	1175	687	0.03%	0.004%
69	9.220	2541	2544	2546	rBV2	460	292	0.01%	0.002%
70	9.246	2548	2552	2555	rVB2	669	498	0.02%	0.003%
71	9.336	2578	2580	2585	rVB2	957	686	0.03%	0.004%
72	9.368	2587	2590	2592	rBV3	555	391	0.02%	0.002%
73	9.410	2598	2603	2607	rBV4	979	874	0.04%	0.005%
74	9.487	2625	2627	2632	rVB	381	255	0.01%	0.001%
75	9.548	2643	2646	2649	rBV2	641	565	0.02%	0.003%
76	9.635	2671	2673	2677	rBV	503	293	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032921\
 Data File : VV020807.D
 Acq On : 29 Mar 2021 16:19
 Operator : SY/MD
 Sample : M1784-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

77	9.696	2688	2692	2694	rBV2	504	387	0.02%	0.002%
78	9.757	2708	2711	2714	rBV3	541	377	0.02%	0.002%
79	9.821	2727	2731	2732	rBV2	881	508	0.02%	0.003%
80	9.943	2767	2769	2775	rVB5	602	479	0.02%	0.003%
81	10.011	2787	2790	2796	rBV4	715	836	0.04%	0.005%
82	10.223	2843	2856	2877	rBV	747262	1167639	48.89%	6.410%
83	10.429	2916	2920	2924	rVB3	706	611	0.03%	0.003%
84	10.455	2925	2928	2930	rBV	639	304	0.01%	0.002%
85	10.561	2959	2961	2962	rBV2	518	212	0.01%	0.001%
86	10.638	2983	2985	2988	rBV2	592	328	0.01%	0.002%
87	10.677	2995	2997	3002	rVB3	676	403	0.02%	0.002%
88	10.857	3049	3053	3060	rVB6	1190	1509	0.06%	0.008%
89	10.889	3060	3063	3067	rBV2	494	469	0.02%	0.003%
90	10.943	3077	3080	3085	rVB2	831	599	0.03%	0.003%
91	11.185	3149	3155	3157	rBV5	1221	1139	0.05%	0.006%
92	11.255	3164	3177	3197	rBV	1150426	1767819	74.01%	9.704%
93	11.535	3261	3264	3267	rBV3	770	578	0.02%	0.003%
94	11.632	3282	3294	3316	rBV	1190955	1859588	77.86%	10.208%
95	11.799	3344	3346	3351	rBV4	1014	709	0.03%	0.004%
96	12.657	3611	3613	3615	rBV	618	403	0.02%	0.002%
97	12.850	3671	3673	3676	rBV	603	317	0.01%	0.002%
98	13.123	3756	3758	3762	rBV	728	446	0.02%	0.002%
99	13.345	3825	3827	3828	rBV	663	179	0.01%	0.001%
100	14.828	4286	4288	4291	rBV3	1433	993	0.04%	0.005%




Sum of corrected areas: 18216576

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032921\
Data File : VV020807.D
Acq On : 29 Mar 2021 16:19
Operator : SY/MD
Sample : M1784-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

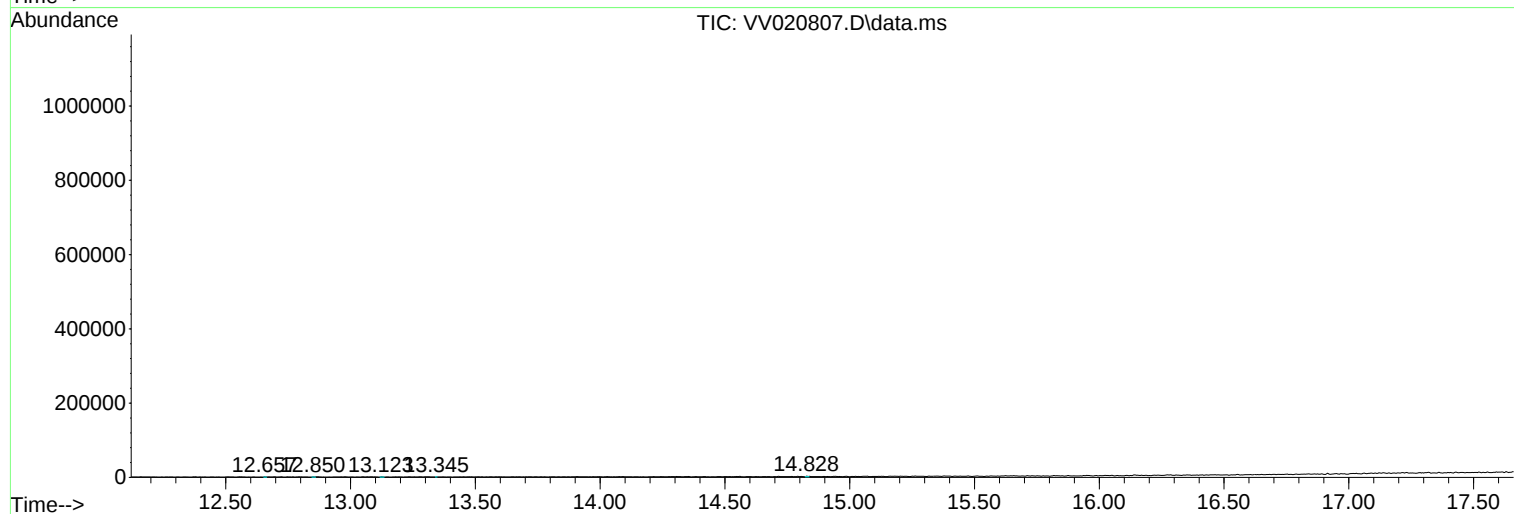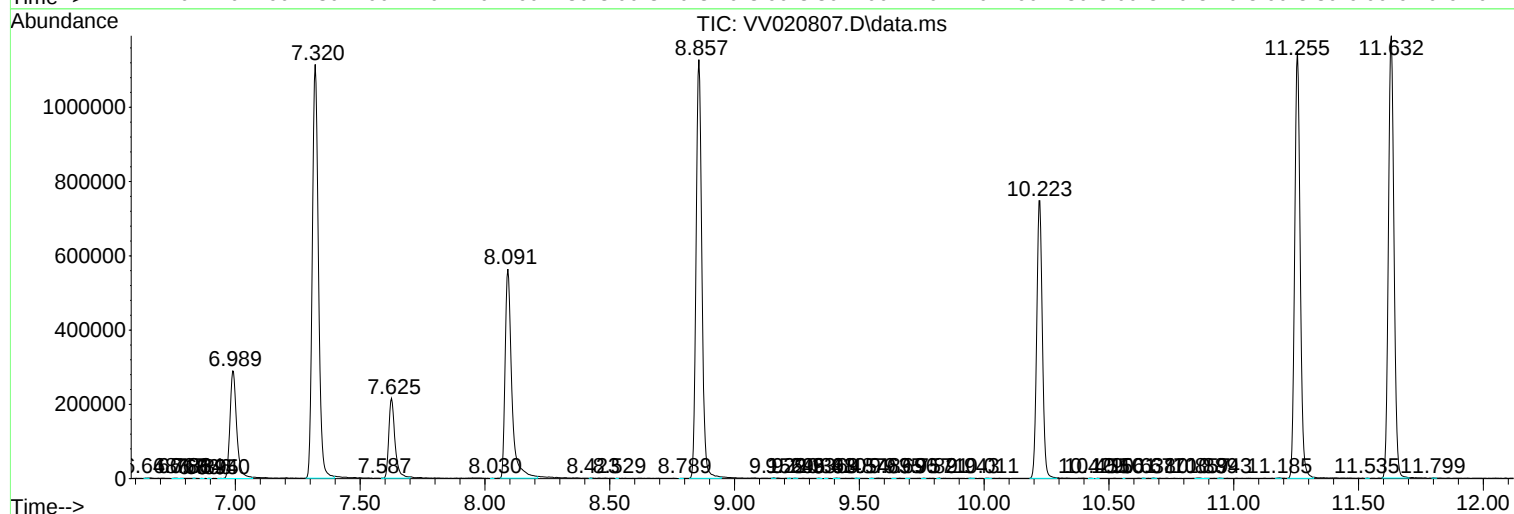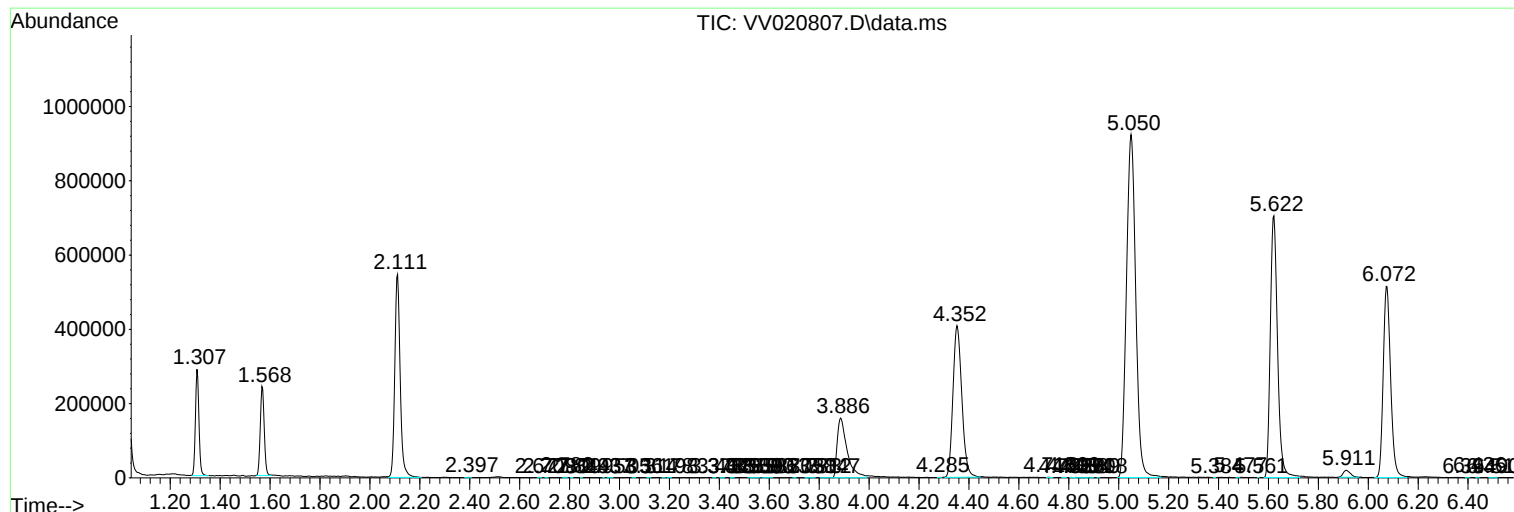

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032921\
Data File : VV020807.D
Acq On : 29 Mar 2021 16:19
Operator : SY/MD
Sample : M1784-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032921\
Data File : VV020807.D
Acq On : 29 Mar 2021 16:19
Operator : SY/MD
Sample : M1784-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
