
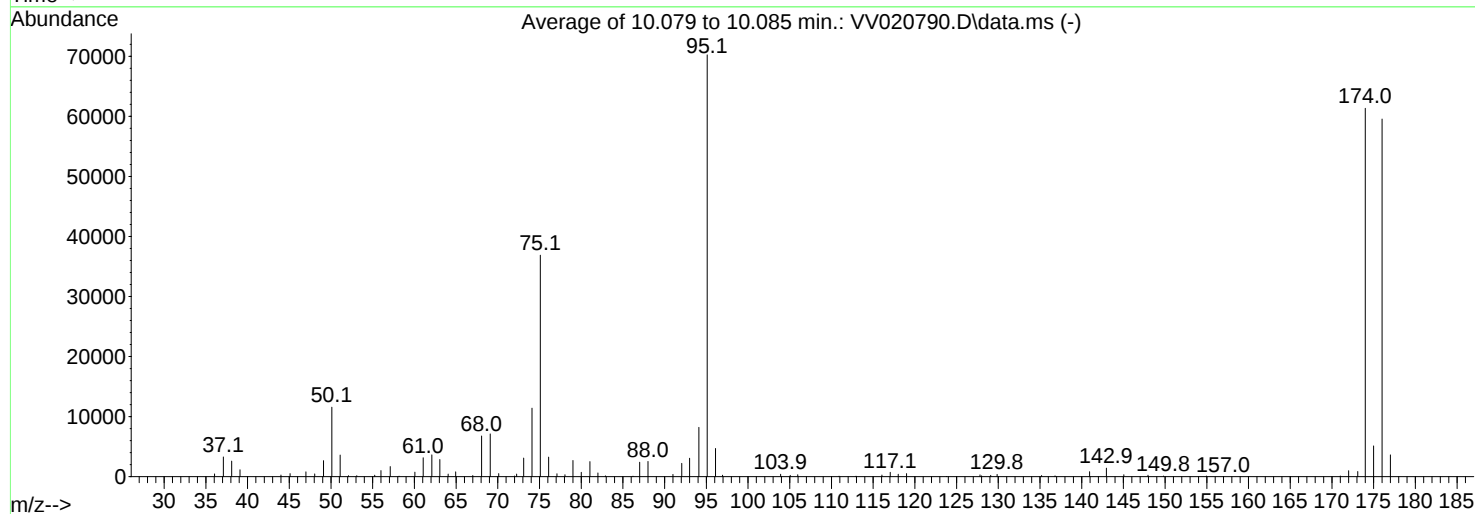


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032921\
Data File : VV020790.D
Acq On : 29 Mar 2021 09:04
Operator : SY/MD
Sample : BFB70
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB70

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Title : VOC Analysis
Last Update : Tue Mar 30 04:39:28 2021

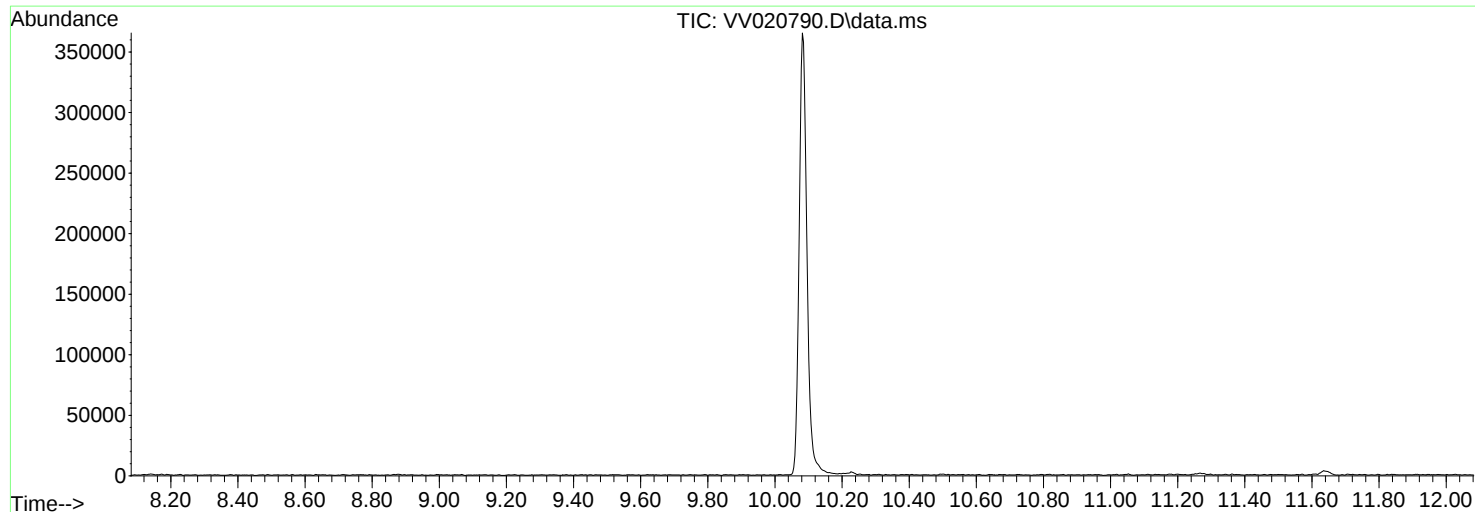

AutoFind: Scans 2811, 2812, 2813; Background Corrected with Scan 2800

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.5	11579	PASS
75	95	30	80	52.5	36883	PASS
95	95	100	100	100.0	70248	PASS
96	95	5	9	6.7	4697	PASS
173	174	0.00	2	1.4	860	PASS
174	95	50	120	87.3	61357	PASS
175	174	5	9	8.3	5112	PASS
176	174	95	101	97.1	59552	PASS
177	176	5	9	6.1	3631	PASS

Scan 2800 (10.043 min): VV020790.D\data.ms
BFB70

m/z	Abundance
36.60	142.0
37.60	102.0
40.10	259.0
44.00	467.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70

m/z	Abundance
36.00	439.0
37.10	3299.0
38.10	2632.0
39.10	1162.0
44.00	800.0
45.10	473.0
47.00	757.0
48.10	465.0
49.10	2700.0
50.10	11710.0
51.10	3483.0
53.10	142.0
55.20	266.0
56.00	1030.0
57.10	1652.0
58.20	112.0
60.00	651.0
61.00	3118.0
62.10	3699.0
63.10	2636.0
64.00	418.0
64.90	713.0
67.00	228.0
68.10	6403.0
69.10	6827.0
70.20	491.0
72.20	587.0
73.10	3085.0
74.10	10874.0
75.10	34568.0
76.10	3193.0
77.10	453.0
78.10	309.0
79.00	2658.0
80.00	621.0
81.10	2400.0
82.00	471.0
82.90	117.0
86.20	118.0
87.00	2515.0
88.00	2383.0
91.00	284.0
92.00	2168.0
93.00	3045.0
94.10	7965.0
95.10	67624.0
96.10	4604.0
97.00	241.0
103.90	326.0
105.00	232.0
105.90	316.0
110.90	137.0
113.00	171.0
116.00	318.0
117.10	600.0
118.00	376.0
119.00	498.0
127.80	452.0
129.10	175.0
129.80	383.0
135.30	148.0
136.80	111.0
140.90	858.0
143.00	1418.0
145.00	258.0
148.00	180.0
149.80	195.0
171.00	159.0
172.00	936.0
174.00	57384.0
175.00	4872.0
176.00	55664.0
177.00	3432.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70

m/z	Abundance
36.10	470.0
37.10	3424.0
38.10	2701.0
39.10	1127.0
39.90	229.0
44.00	706.0
45.10	545.0
47.00	858.0
48.00	466.0
49.10	2805.0
50.10	11921.0
51.10	3665.0
52.10	209.0
53.10	163.0
55.20	252.0
56.00	1000.0
57.10	1726.0
58.10	106.0
60.00	760.0
61.10	3284.0
62.10	3738.0
63.10	2971.0
64.00	446.0
65.00	849.0
67.00	208.0
68.00	6988.0
69.10	7347.0
70.10	491.0
72.30	466.0
73.10	3177.0
74.10	11777.0
75.10	38368.0
76.10	3344.0
77.10	532.0
78.10	344.0
79.00	2886.0
80.00	682.0
81.10	2623.0
82.00	597.0
82.90	157.0
86.20	127.0
87.00	2445.0
88.00	2493.0
91.00	385.0
92.10	2297.0
93.00	3136.0
94.10	8438.0
95.10	72656.0
96.10	4885.0
96.90	272.0
103.90	411.0
105.00	257.0
106.00	336.0
110.90	110.0
112.90	113.0
116.00	239.0
117.00	749.0
118.00	404.0
119.00	541.0
127.80	448.0
129.10	236.0
129.90	395.0
135.20	172.0
136.80	151.0
140.90	827.0
142.90	1535.0
145.00	317.0
147.90	246.0
149.80	148.0
155.00	111.0
157.00	109.0
171.00	136.0
172.00	1048.0
173.10	1296.0
174.00	63296.0
175.00	5368.0
176.00	61488.0
177.00	3651.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70

m/z	Abundance
36.10	492.0
37.10	3120.0
38.10	2462.0
39.10	1183.0
40.00	280.0
44.00	687.0
45.10	505.0
47.00	759.0
48.00	441.0
49.10	2523.0
50.10	11105.0
51.10	3619.0
52.10	285.0
53.10	157.0
55.30	179.0
56.00	984.0
57.10	1659.0
60.10	819.0
61.10	3069.0
62.10	3463.0
63.00	2980.0
64.10	414.0
65.00	834.0
67.00	148.0
68.10	6950.0
69.10	7138.0
70.00	546.0
72.00	290.0
72.20	254.0
73.10	3043.0
74.10	11574.0
75.10	37712.0
76.10	3228.0
77.10	465.0
78.00	325.0
79.00	2570.0
80.00	825.0
81.00	2464.0
82.00	773.0
82.90	145.0
87.00	2232.0
88.00	2688.0
91.00	432.0
92.10	2173.0
93.00	3003.0
94.10	8223.0
95.10	70464.0
96.10	4602.0
96.90	233.0
103.90	436.0
105.10	188.0
106.00	312.0
116.10	228.0
117.00	801.0
118.00	410.0
119.00	491.0
123.80	106.0
128.00	405.0
129.10	236.0
129.90	354.0
135.10	245.0
136.80	171.0
141.00	792.0
142.90	1320.0
145.10	398.0
147.90	331.0
154.90	200.0
172.00	1002.0
173.10	1285.0
174.00	63392.0
175.00	5096.0
176.00	61504.0
177.00	3811.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70