




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032923\
 Data File : VV030324.D
 Acq On : 29 Mar 2023 14:04
 Operator : SY/MD
 Sample : 02092-20
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB993

Manual IntegrationsAPPROVED

Quant Time: Mar 30 02:10:32 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Mar 30 01:55:26 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/31/2023
 Supervised By :Mahesh Dadoda 03/31/2023

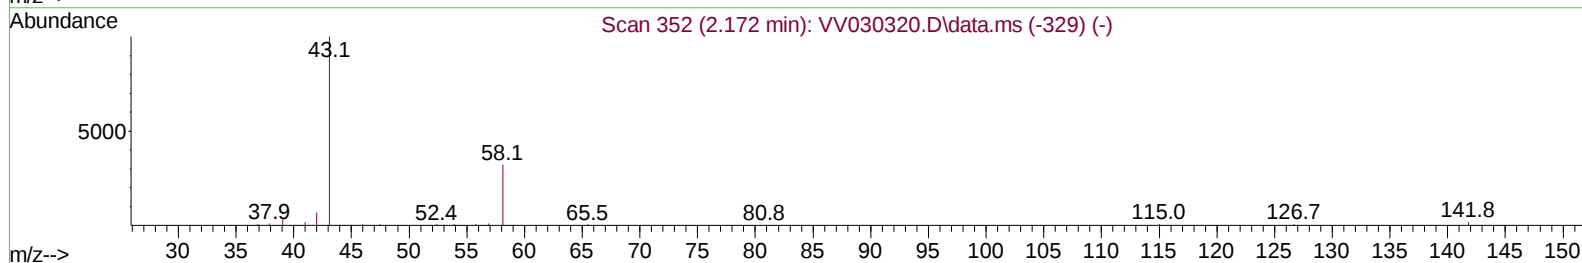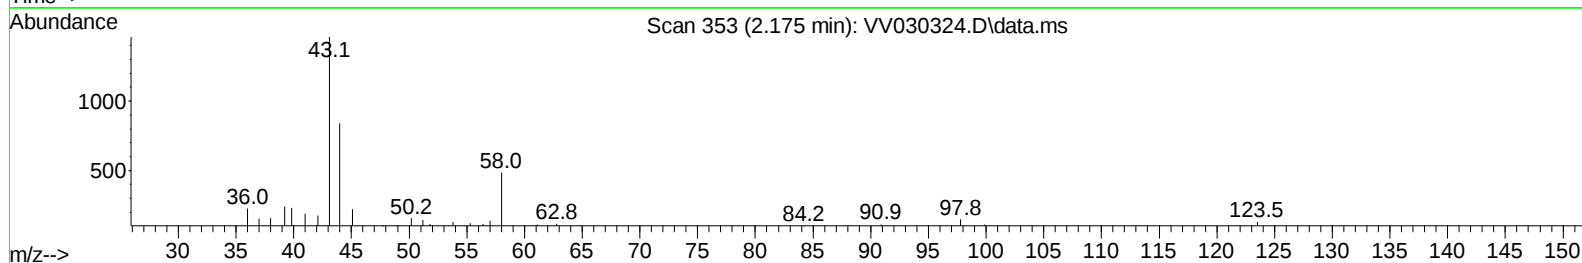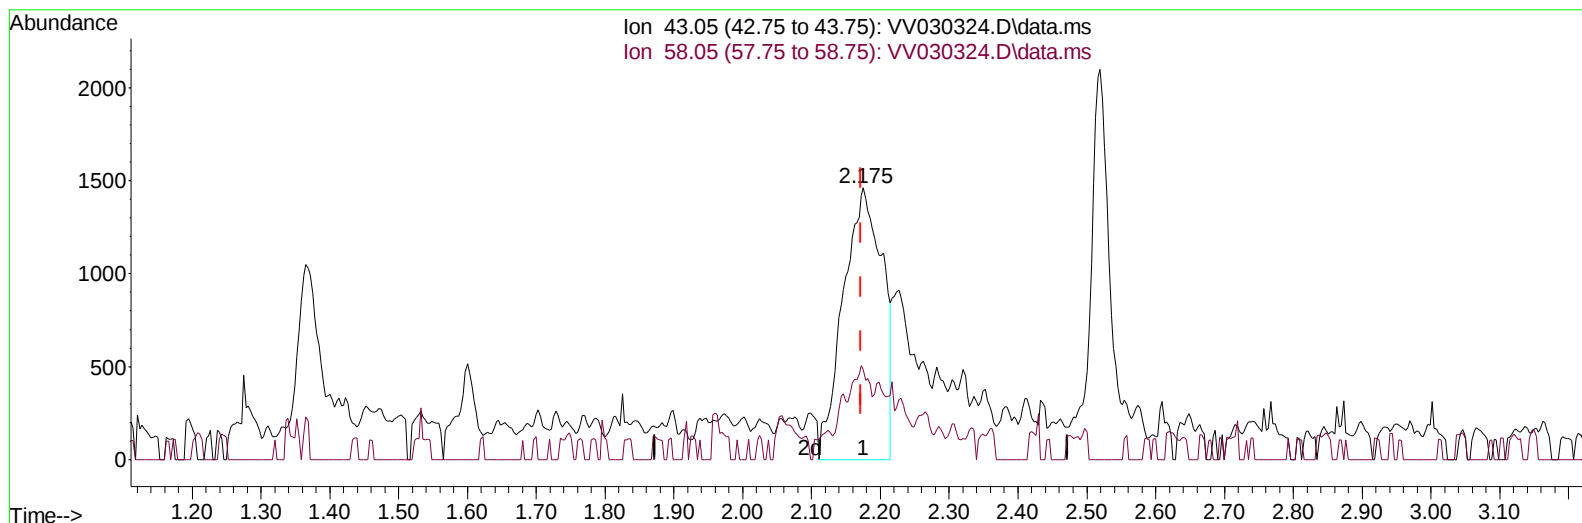

TIC: VV030324.D\data.ms

(13) Acetone (T)

2.175min (+ 0.003) 2.55 ug/L

response 5750

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.40	4.92
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032923\
 Data File : VV030324.D
 Acq On : 29 Mar 2023 14:04
 Operator : SY/MD
 Sample : 02092-20
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB993

Manual IntegrationsAPPROVED

Quant Time: Mar 30 02:10:32 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Mar 30 01:55:26 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/31/2023
 Supervised By :Mahesh Dadoda 03/31/2023

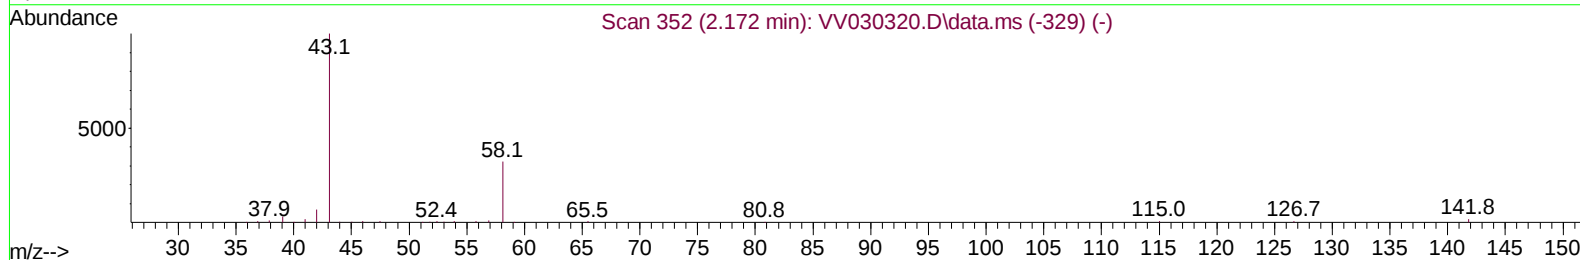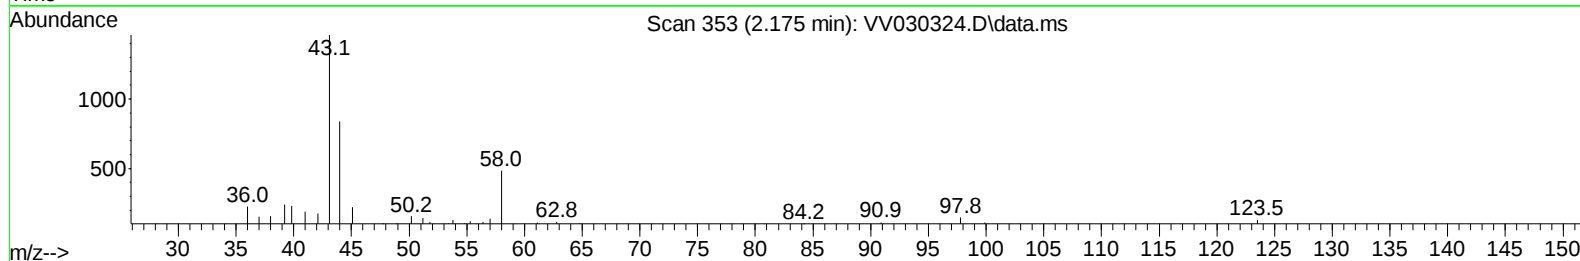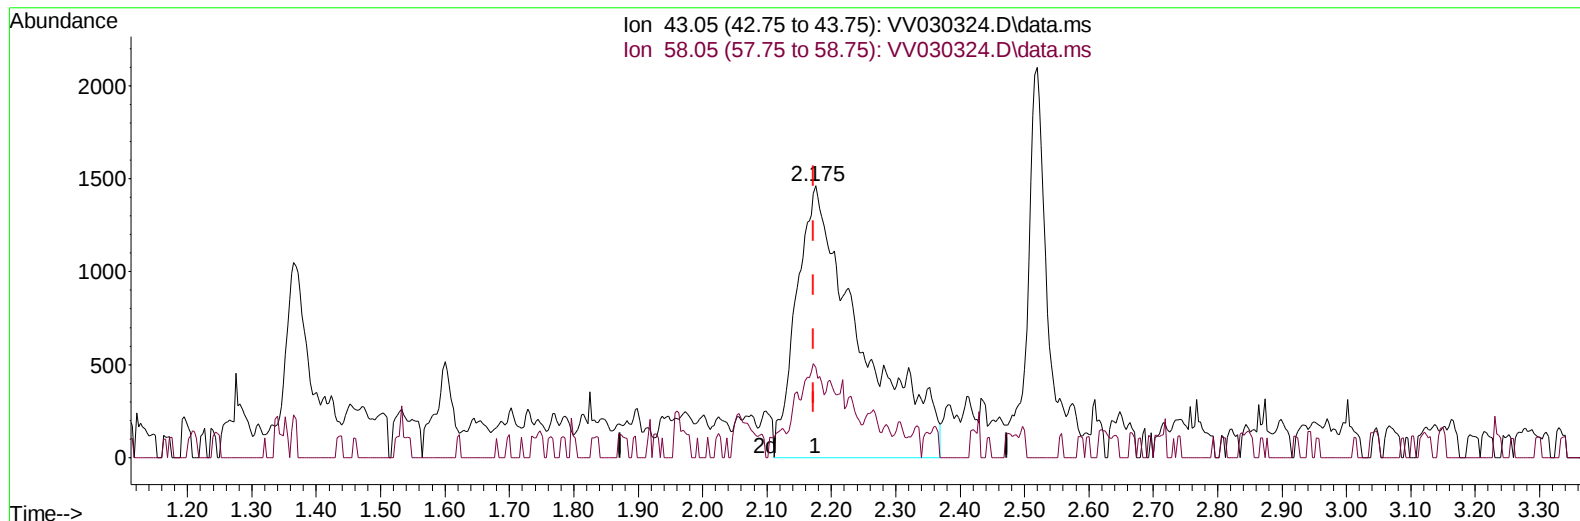

TIC: VV030324.D\data.ms

(13) Acetone (T)

2.175min (+ 0.003) 4.49 ug/L m

response 10120

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.40	2.80
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032923\
 Data File : VV030324.D
 Acq On : 29 Mar 2023 14:04
 Operator : SY/MD
 Sample : 02092-20
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB993

Manual IntegrationsAPPROVED

Quant Time: Mar 30 02:10:32 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Mar 30 01:55:26 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/31/2023
 Supervised By :Mahesh Dadoda 03/31/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.542	114		137541	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.793	117		135943	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152		65285	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.278	65		38595	4.237	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	84.800%	
7) Chloroethane-d5	1.536	69		40535	4.585	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.800%	
11) 1,1-Dichloroethene-d2	2.063	63		65756	3.042	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	60.800%	
20) 2-Butanone-d5	3.838	46		102078	43.354	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	86.700%	
24) Chloroform-d	4.262	84		102326	4.641	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.800%	
26) 1,2-Dichloroethane-d4	4.953	65		50821	4.886	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.800%	
32) Benzene-d6	4.970	84		182260	4.758	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.200%	
36) 1,2-Dichloropropane-d6	5.998	67		59066	4.925	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.400%	
41) Toluene-d8	7.252	98		148859	4.231	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.600%	
43) trans-1,3-Dichloroprop...	7.561	79		19155	4.242	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.800%	
46) 2-Hexanone-d5	8.037	63		86178	47.495	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.980%	
56) 1,1,2,2-Tetrachloroeth...	10.162	84		44656	4.724	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.400%	
66) 1,2-Dichlorobenzene-d4	11.571	152		58792	5.039	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.800%	
Target Compounds							
13) Acetone	2.175	43		10120m	4.495	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032923\
Data File : VV030324.D
Acq On : 29 Mar 2023 14:04
Operator : SY/MD
Sample : 02092-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB993

Manual IntegrationsAPPROVED

Quant Time: Mar 30 02:10:32 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Mar 30 01:55:26 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 03/31/2023
Supervised By :Mahesh Dadoda 03/31/2023

