




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032923\
 Data File : VV030334.D
 Acq On : 29 Mar 2023 18:09
 Operator : SY/MD
 Sample : 02092-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB975

Manual IntegrationsAPPROVED

Quant Time: Mar 30 02:13:39 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Mar 30 01:55:26 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/31/2023
 Supervised By :Mahesh Dadoda 03/31/2023

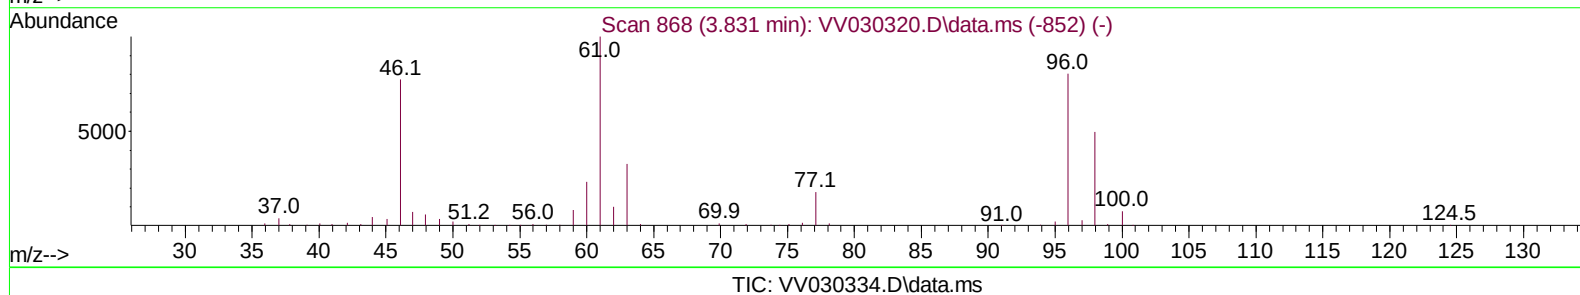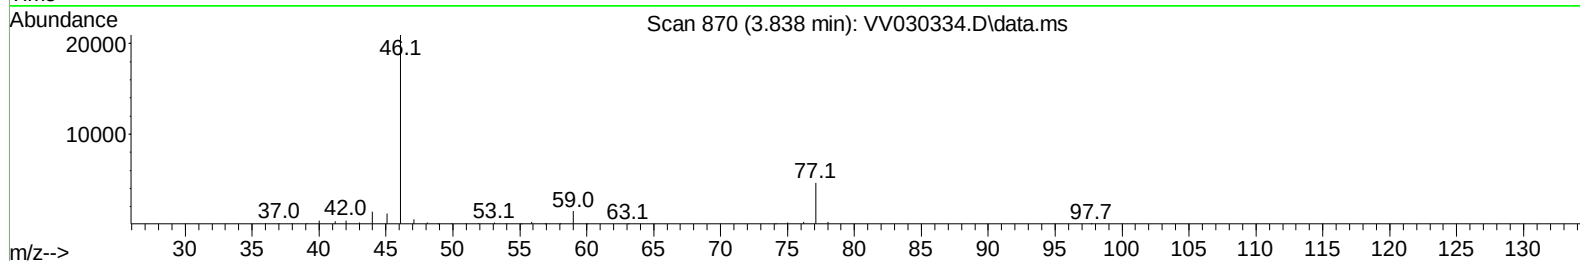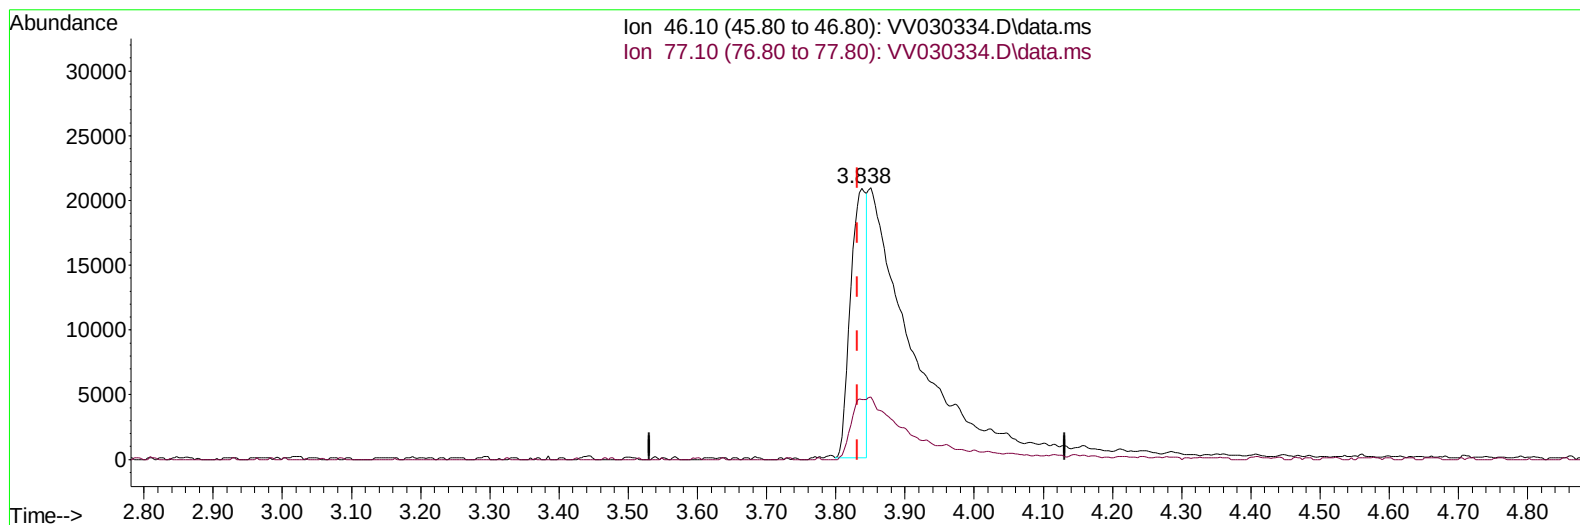

(20) 2-Butanone-d5 (S)

3.838min (+ 0.006) 13.35 ug/L

response 33086

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	11.10	19.43#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032923\
 Data File : VV030334.D
 Acq On : 29 Mar 2023 18:09
 Operator : SY/MD
 Sample : 02092-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB975

Manual IntegrationsAPPROVED

Quant Time: Mar 30 02:13:39 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Mar 30 01:55:26 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/31/2023
 Supervised By :Mahesh Dadoda 03/31/2023

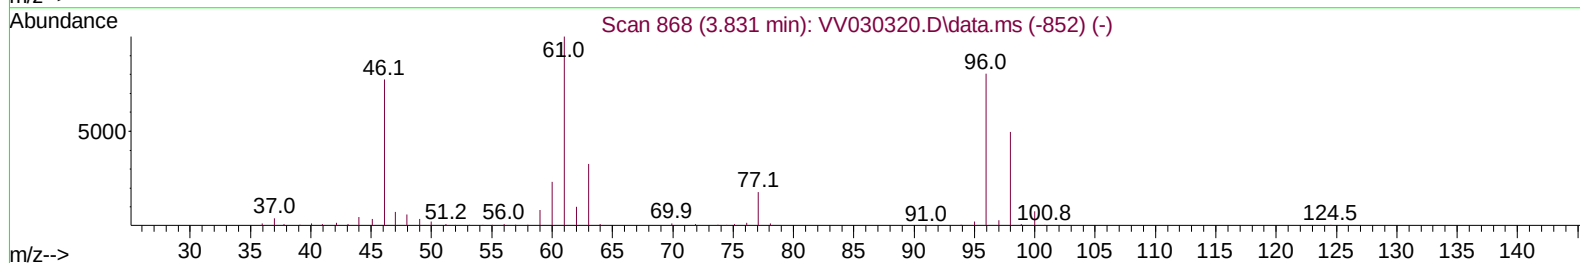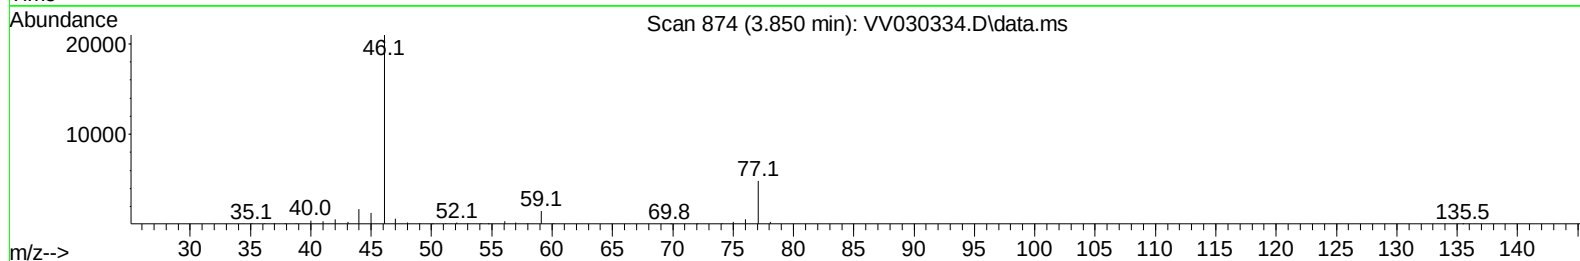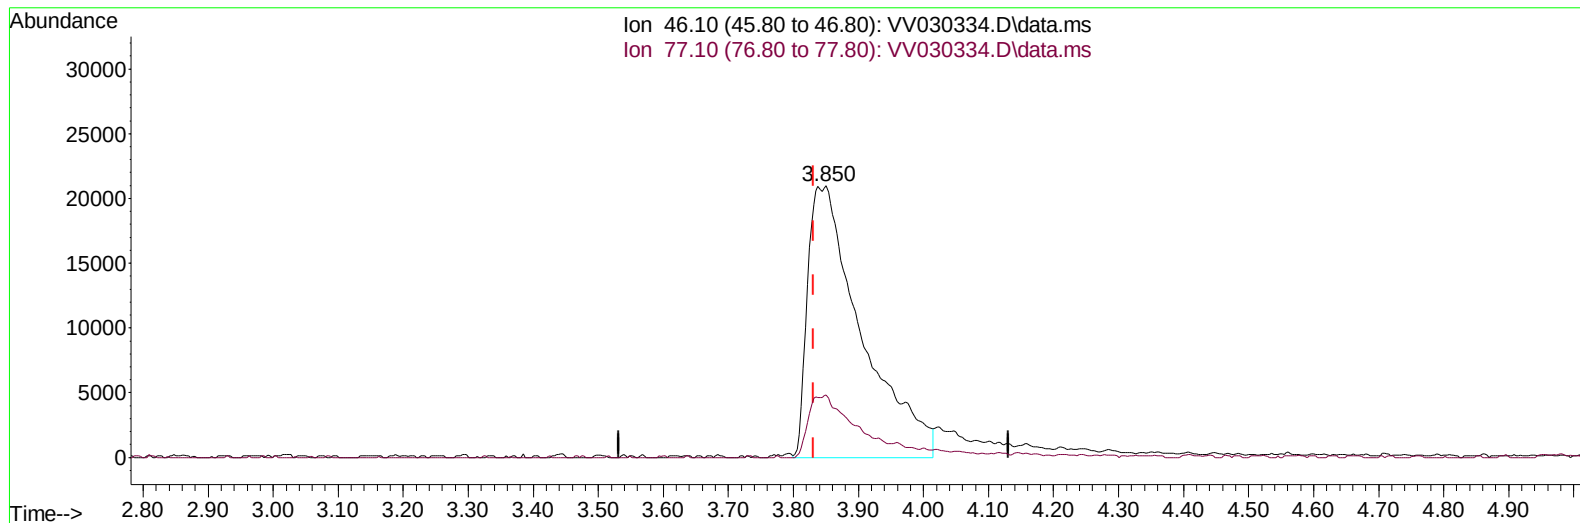

TIC: VV030334.D\data.ms

(20) 2-Butanone-d5 (S)

3.850min (+ 0.019) 48.49 ug/L m

response 120150

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	11.10	5.35#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032923\
 Data File : VV030334.D
 Acq On : 29 Mar 2023 18:09
 Operator : SY/MD
 Sample : 02092-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB975

Manual IntegrationsAPPROVED

Quant Time: Mar 30 02:13:39 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Mar 30 01:55:26 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/31/2023
 Supervised By :Mahesh Dadoda 03/31/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.545	114		144738	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117		140516	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152		67435	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.278	65		38776	4.045	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	81.000%	
7) Chloroethane-d5	1.535	69		40590	4.363	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.200%	
11) 1,1-Dichloroethene-d2	2.063	63		67838	2.982	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	59.600%#	
20) 2-Butanone-d5	3.850	46		120150m	48.492	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	96.980%	
24) Chloroform-d	4.259	84		104102	4.487	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.800%	
26) 1,2-Dichloroethane-d4	4.953	65		53069	4.848	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.000%	
32) Benzene-d6	4.969	84		183963	4.646	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.000%	
36) 1,2-Dichloropropane-d6	5.998	67		60367	4.870	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.400%	
41) Toluene-d8	7.252	98		150902	4.150	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.000%	
43) trans-1,3-Dichloroprop...	7.561	79		19394	4.155	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.200%	
46) 2-Hexanone-d5	8.037	63		98032	52.269	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	104.540%	
56) 1,1,2,2-Tetrachloroeth...	10.162	84		47622	4.874	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.400%	
66) 1,2-Dichlorobenzene-d4	11.570	152		61463	5.099	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.000%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032923\
Data File : VV030334.D
Acq On : 29 Mar 2023 18:09
Operator : SY/MD
Sample : 02092-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 3

Instrument :
MSVOA_V
ClientSampleId :
CB975

Manual IntegrationsAPPROVED

Quant Time: Mar 30 02:13:39 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Mar 30 01:55:26 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 03/31/2023
Supervised By :Mahesh Dadoda 03/31/2023

