

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032923\
 Data File : VV030321.D
 Acq On : 29 Mar 2023 12:51
 Operator : SY/MD
 Sample : VV0329WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK319

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030321.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	82	rBV	60785	61920	11.18%	1.435%
2	1.535	146	154	165	rBV	68342	80940	14.62%	1.876%
3	2.063	307	318	333	rBV	131007	193319	34.92%	4.480%
4	2.452	431	439	455	rVB2	14379	26296	4.75%	0.609%
5	3.838	854	870	871	rBV9	32825	48091	8.69%	1.114%
6	4.259	988	1001	1020	rVB	97338	242284	43.76%	5.615%
7	4.966	1201	1221	1245	rBV3	211241	553663	100.00%	12.831%
8	5.542	1387	1400	1426	rBV	164285	355146	64.14%	8.230%
9	5.998	1526	1542	1562	rBV	131588	284817	51.44%	6.600%
10	6.921	1819	1829	1845	rBV3	51082	98383	17.77%	2.280%
11	7.252	1917	1932	1957	rBV	228549	424007	76.58%	9.826%
12	7.561	2019	2028	2047	rBV	32505	60051	10.85%	1.392%
13	8.040	2165	2177	2209	rBV	222719	500142	90.33%	11.590%
14	8.371	2273	2280	2293	rVB10	5421	10586	1.91%	0.245%
15	8.792	2397	2411	2430	rBV	253454	431099	77.86%	9.990%
16	10.162	2823	2837	2856	rBV	100049	162774	29.40%	3.772%
17	11.194	3143	3158	3175	rBV	250753	396207	71.56%	9.182%
18	11.570	3257	3275	3290	rBV	233793	379256	68.50%	8.789%
19	13.692	3925	3935	3944	rBV	3188	6174	1.12%	0.143%




Sum of corrected areas: 4315155

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032923\
Data File : VV030321.D
Acq On : 29 Mar 2023 12:51
Operator : SY/MD
Sample : VV0329WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK319

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

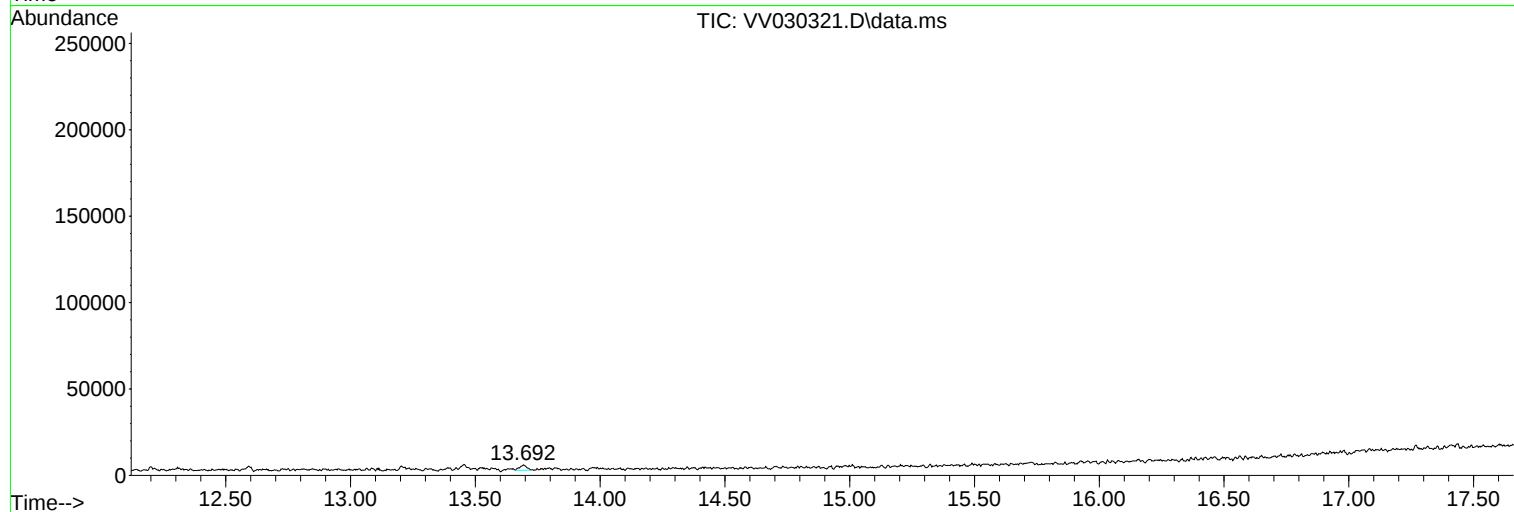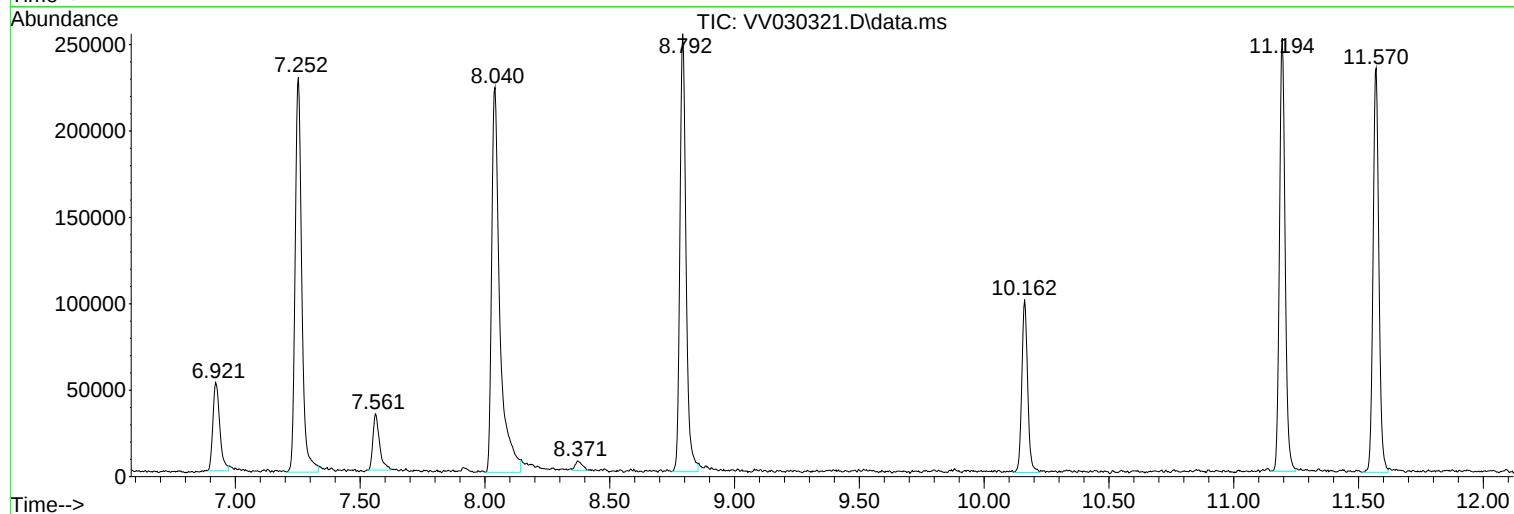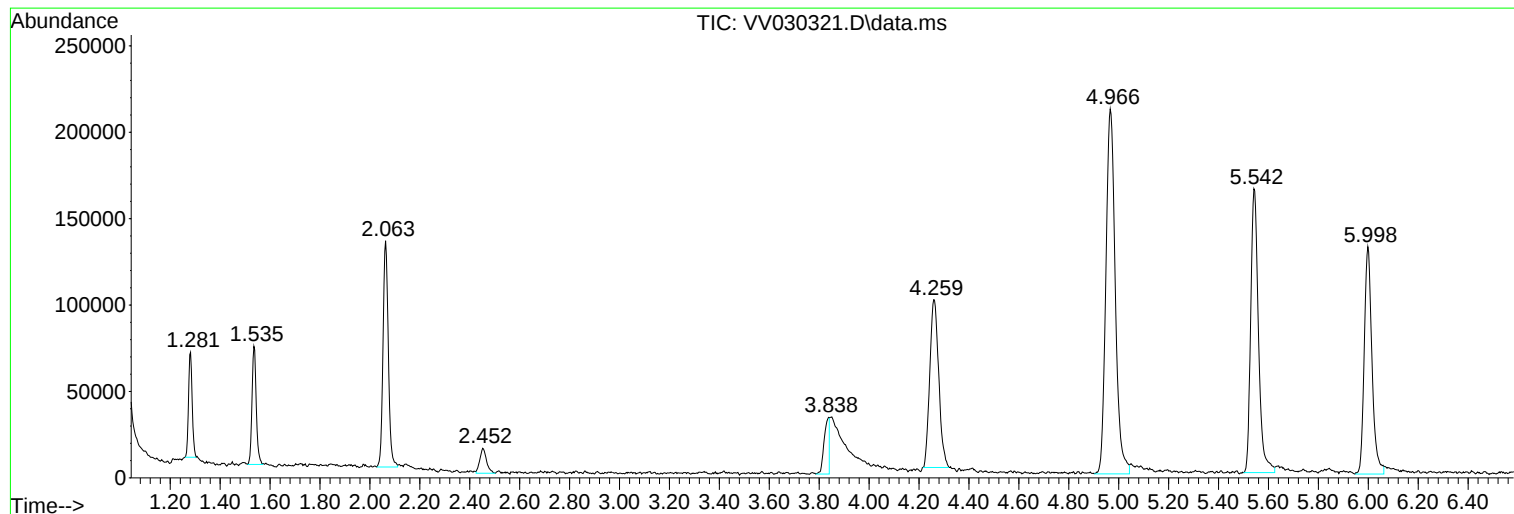

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032923\
Data File : VV030321.D
Acq On : 29 Mar 2023 12:51
Operator : SY/MD
Sample : VV0329WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK319

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032923\
Data File : VV030321.D
Acq On : 29 Mar 2023 12:51
Operator : SY/MD
Sample : VV0329WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK319

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------