

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032923\
 Data File : VV030323.D
 Acq On : 29 Mar 2023 13:39
 Operator : SY/MD
 Sample : 02092-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB981

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030323.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	87	rVB	61990	64847	12.06%	1.447%
2	1.536	147	154	170	rVB	68093	82766	15.39%	1.846%
3	2.066	306	319	333	rBV	126121	188858	35.12%	4.213%
4	3.818	853	864	889	rBV	49280	176917	32.90%	3.946%
5	4.259	981	1001	1021	rBV	99192	255422	47.50%	5.698%
6	4.966	1205	1221	1243	rBV3	207896	537746	100.00%	11.995%
7	5.542	1387	1400	1421	rBV	174204	369971	68.80%	8.253%
8	5.998	1530	1542	1564	rBV	129688	272777	50.73%	6.085%
9	6.924	1817	1830	1846	rBV	53989	106584	19.82%	2.378%
10	7.252	1920	1932	1949	rBV	230433	409148	76.09%	9.127%
11	7.561	2017	2028	2040	rBV	32404	60507	11.25%	1.350%
12	7.889	2118	2130	2134	rBV4	5089	9075	1.69%	0.202%
13	8.037	2164	2176	2214	rBV	234926	496599	92.35%	11.078%
14	8.793	2400	2411	2431	rBV	268728	452594	84.17%	10.096%
15	10.162	2827	2837	2850	rBV	93602	147725	27.47%	3.295%
16	10.333	2880	2890	2903	rBV2	19917	34062	6.33%	0.760%
17	11.194	3145	3158	3180	rBV	267185	421921	78.46%	9.412%
18	11.571	3264	3275	3290	rVB	232793	372445	69.26%	8.308%
19	12.201	3466	3471	3481	rVB4	5978	10199	1.90%	0.228%
20	12.300	3494	3502	3510	rBV4	8389	12760	2.37%	0.285%




Sum of corrected areas: 4482923

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032923\
Data File : VV030323.D
Acq On : 29 Mar 2023 13:39
Operator : SY/MD
Sample : 02092-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB981

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

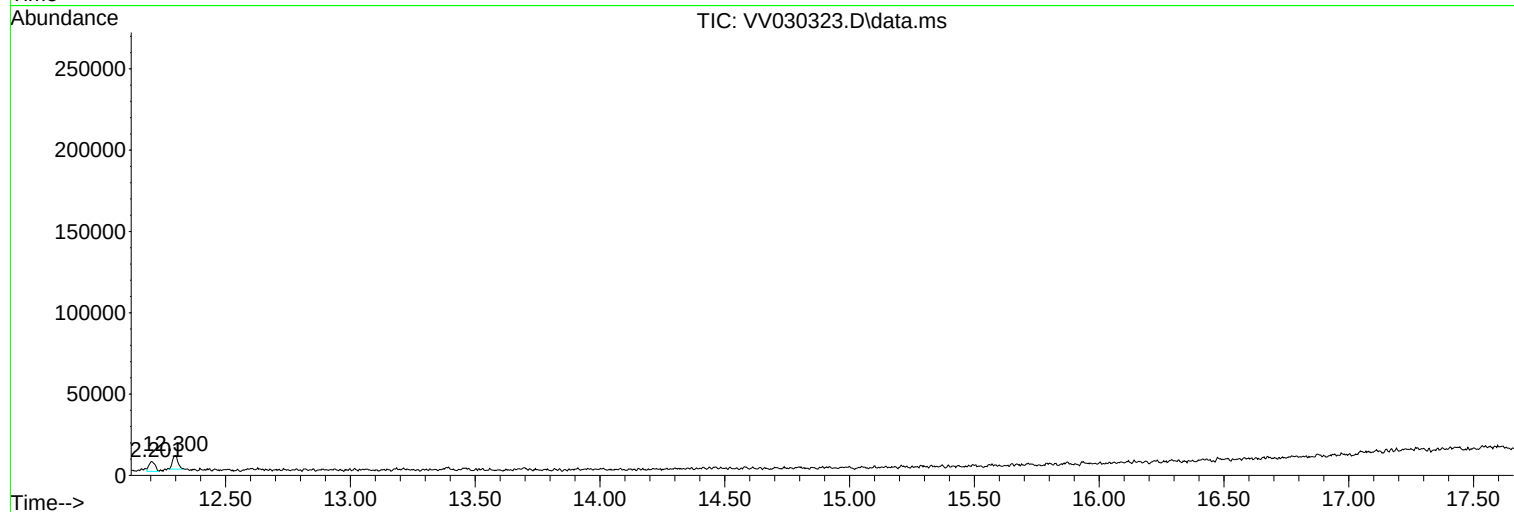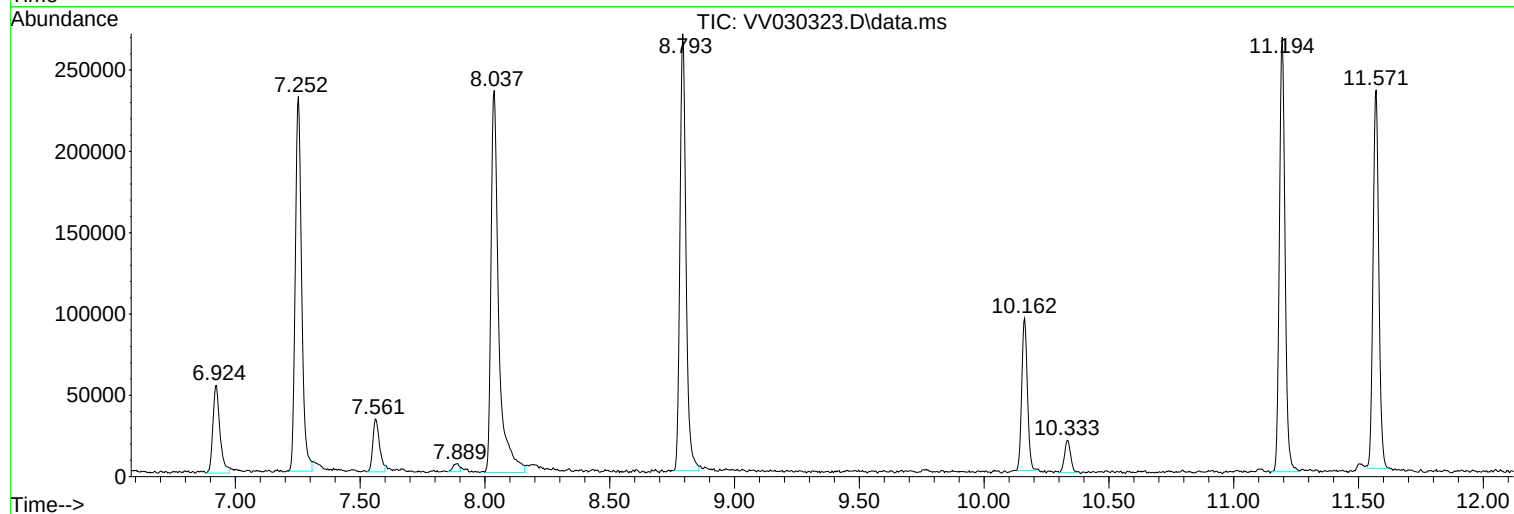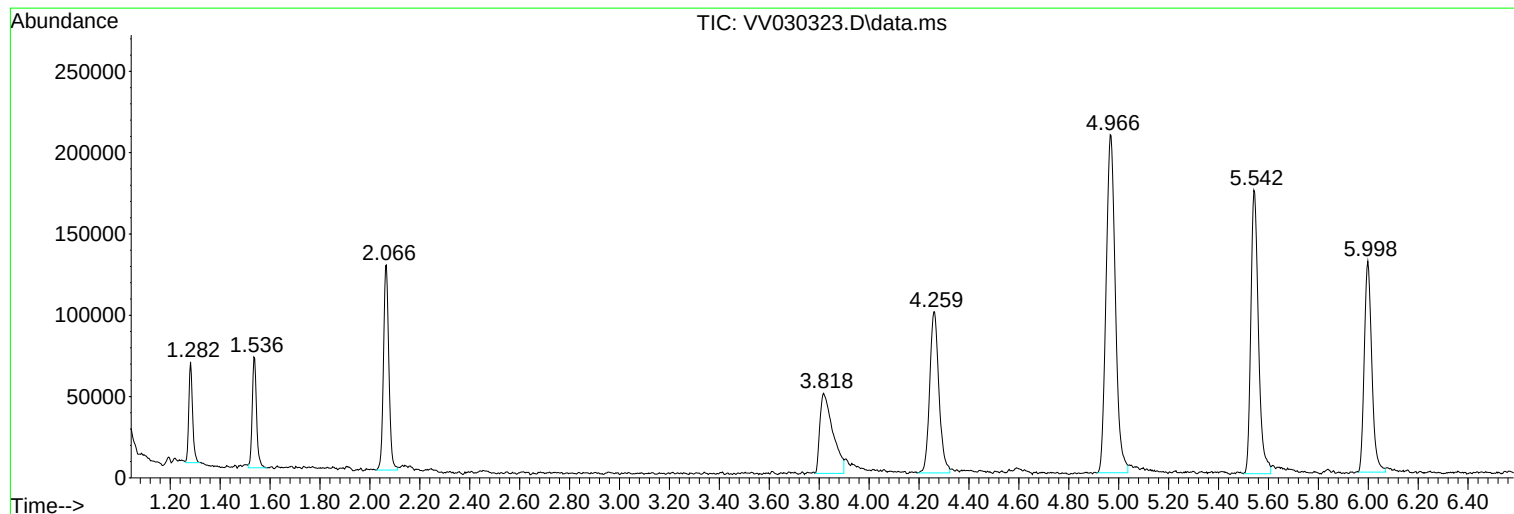

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032923\
Data File : VV030323.D
Acq On : 29 Mar 2023 13:39
Operator : SY/MD
Sample : 02092-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB981

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032923\
Data File : VV030323.D
Acq On : 29 Mar 2023 13:39
Operator : SY/MD
Sample : 02092-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB981

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------