

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032923\
 Data File : VV030326.D
 Acq On : 29 Mar 2023 14:52
 Operator : SY/MD
 Sample : 02099-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0AA5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030326.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.086	10	14	31	rVB	45614	57886	2.03%	0.590%
2	1.278	65	74	85	rBV2	73478	93747	3.30%	0.955%
3	1.536	147	154	166	rVB	70546	81930	2.88%	0.835%
4	1.973	282	290	304	rVB	50526	74257	2.61%	0.757%
5	2.063	308	318	341	rVB	135070	210618	7.40%	2.146%
6	2.712	503	520	554	rBV	1293462	2844743	100.00%	28.981%
7	3.838	859	870	907	rBV	31332	166058	5.84%	1.692%
8	4.259	985	1001	1034	rVB	100703	269228	9.46%	2.743%
9	4.966	1205	1221	1250	rBV2	222659	615730	21.64%	6.273%
10	5.542	1388	1400	1423	rBV	166041	348848	12.26%	3.554%
11	5.998	1528	1542	1560	rBV	134184	285842	10.05%	2.912%
12	6.921	1819	1829	1851	rBV	55913	109391	3.85%	1.114%
13	7.252	1920	1932	1946	rBV	239819	428297	15.06%	4.363%
14	7.326	1947	1955	1974	rVB	36107	70297	2.47%	0.716%
15	7.561	2020	2028	2040	rBV	33866	60361	2.12%	0.615%
16	7.912	2119	2137	2159	rBV	1246989	2133106	74.98%	21.731%
17	8.040	2166	2177	2218	rVB	254138	556638	19.57%	5.671%
18	8.793	2399	2411	2431	rBV	251796	424926	14.94%	4.329%
19	10.162	2817	2837	2849	rBV	105234	173731	6.11%	1.770%
20	11.194	3146	3158	3176	rBV	258449	411255	14.46%	4.190%
21	11.571	3262	3275	3291	rBV	249089	398862	14.02%	4.063%




Sum of corrected areas: 9815751

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032923\
Data File : VV030326.D
Acq On : 29 Mar 2023 14:52
Operator : SY/MD
Sample : 02099-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AA5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

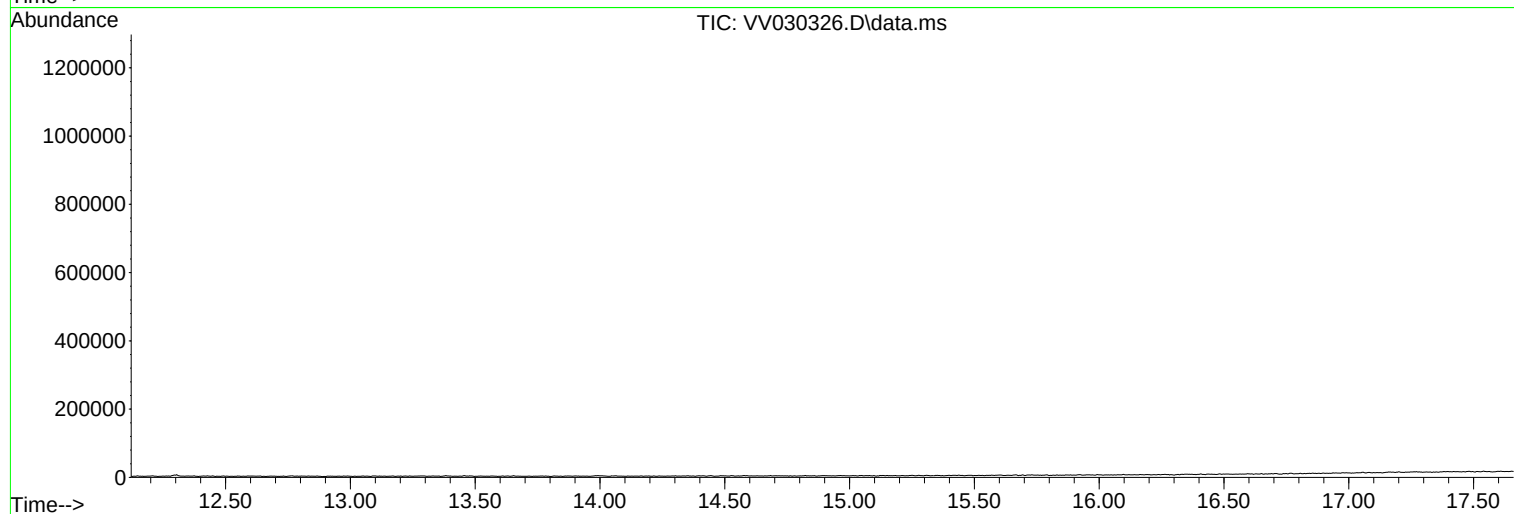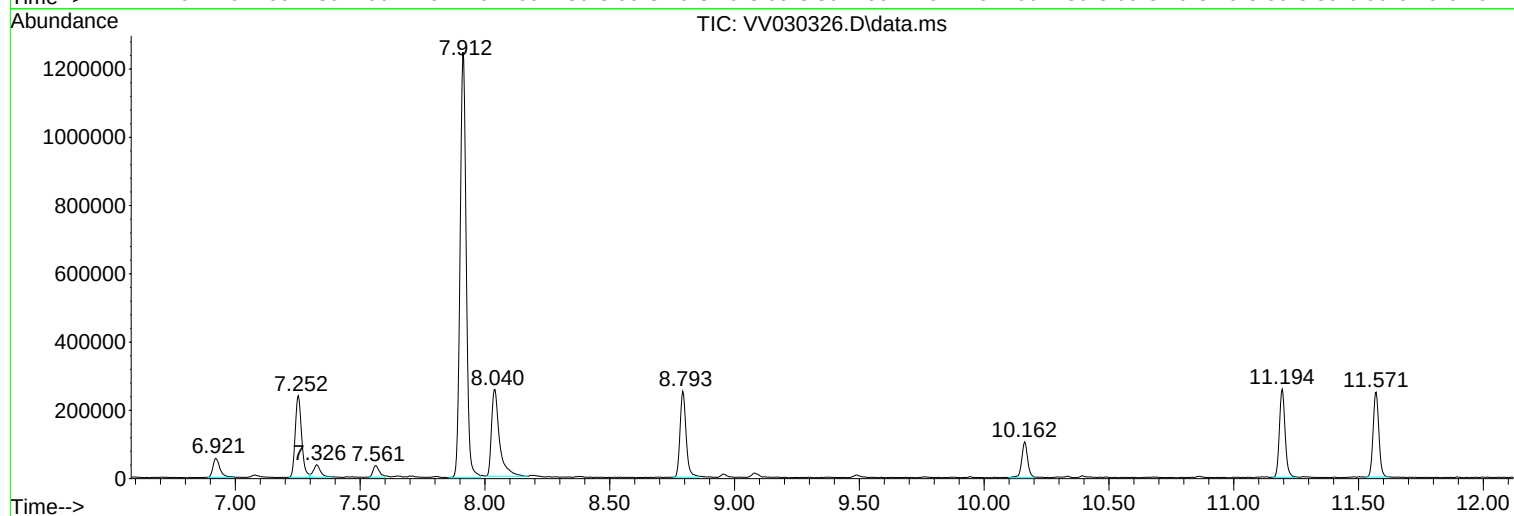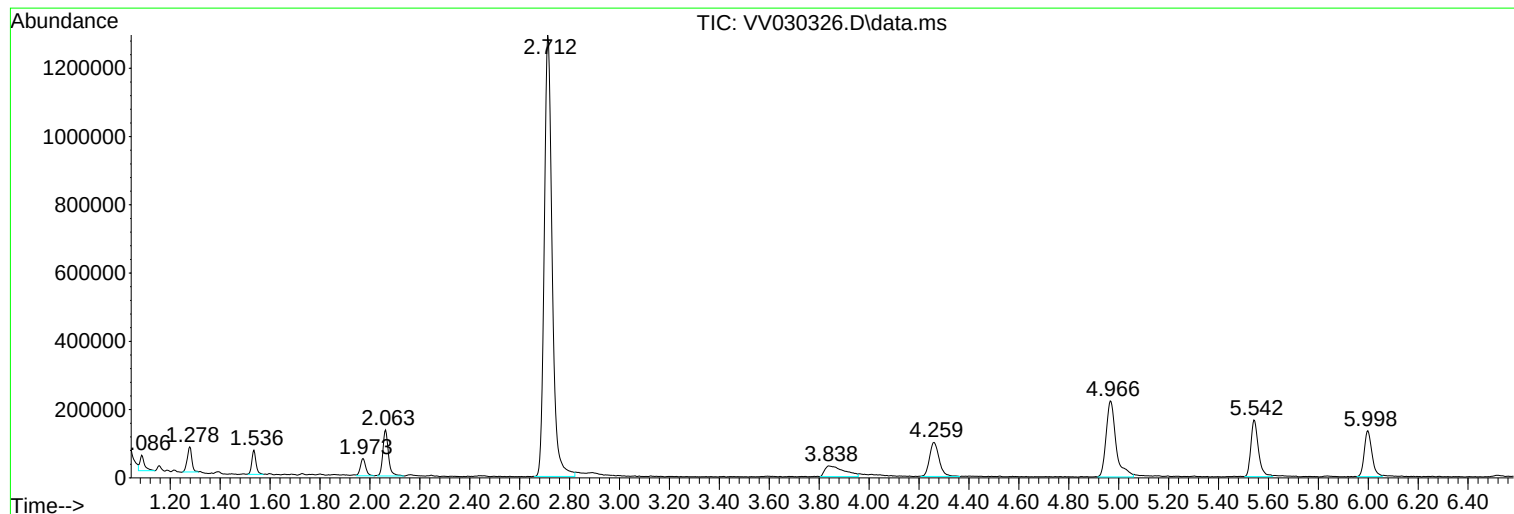

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032923\
Data File : VV030326.D
Acq On : 29 Mar 2023 14:52
Operator : SY/MD
Sample : 02099-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AA5










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.085	0.83 ug/L	57886	1,4-Difluorobenzene	5.542

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propene	42	C3H6	000115-07-1	90
2			Furan, 2,5-dihydro-	70	C4H6O	001708-29-8	83
3			3-Butenoic acid	86	C4H6O2	000625-38-7	78
4			2-Butenal, (E)-	70	C4H6O	000123-73-9	78
5			N-Methyl-7-azabicyclo(2,2,1)hept...	109	C7H11N	055590-26-6	64

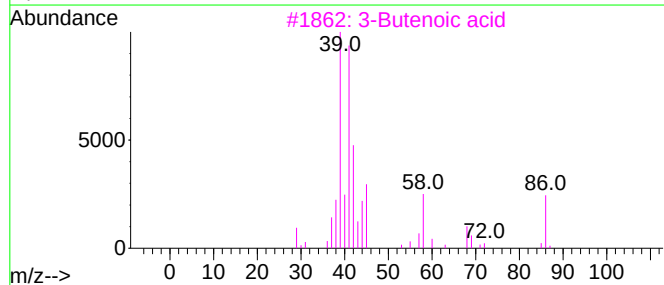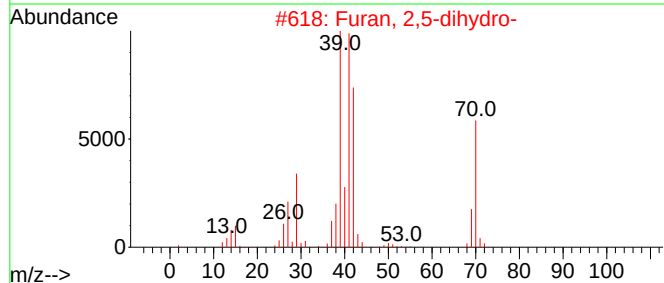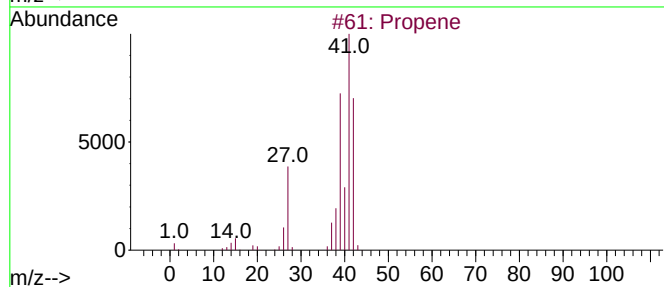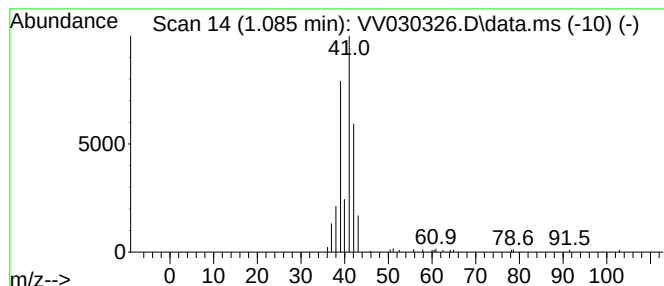

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032923\
Data File : VV030326.D
Acq On : 29 Mar 2023 14:52
Operator : SY/MD
Sample : 02099-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AA5










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Propane, 2-chloro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.973	1.06 ug/L	74257	1,4-Difluorobenzene	5.542

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propane, 2-chloro-	78	C3H7Cl	000075-29-6	58
2			Propane, 2-chloro-	78	C3H7Cl	000075-29-6	50
3			Propane, 2-chloro-	78	C3H7Cl	000075-29-6	43
4			2-(2'-Chloroethoxy)-propene	120	C5H9ClO	099586-46-6	36
5			2-Chloroethanol	80	C2H5ClO	000107-07-3	9

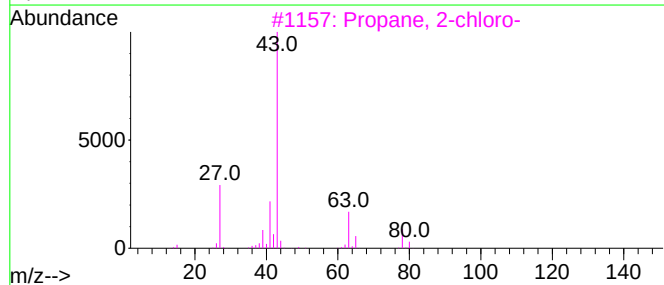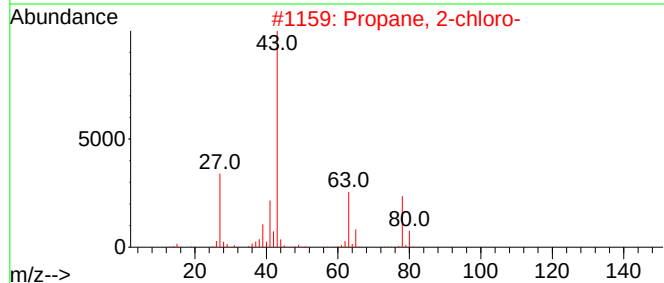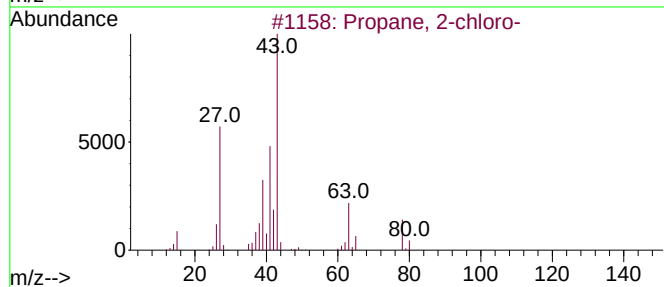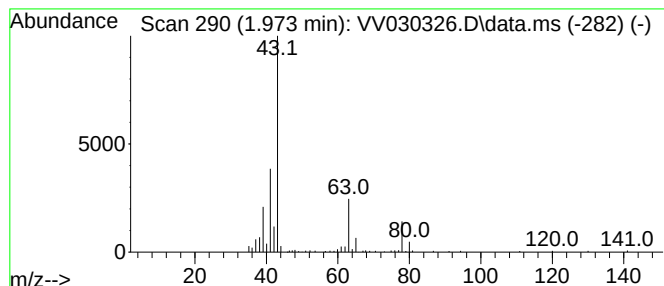

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032923\
Data File : VV030326.D
Acq On : 29 Mar 2023 14:52
Operator : SY/MD
Sample : 02099-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AA5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	1.085	0.8	ug/L	57886	1	5.542	348848	5.0
Propane, 2-chloro-	1.973	1.1	ug/L	74257	1	5.542	348848	5.0