

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032923\
 Data File : VV030334.D
 Acq On : 29 Mar 2023 18:09
 Operator : SY/MD
 Sample : 02092-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB975

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030334.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	61799	66065	12.24%	1.512%
2	1.532	147	153	166	rVB	63077	77148	14.29%	1.766%
3	2.063	308	318	328	rBV	126051	179109	33.18%	4.099%
4	3.838	858	870	871	rBV2	33688	49087	9.09%	1.123%
5	4.265	986	1003	1023	rBV2	97388	249652	46.25%	5.714%
6	4.966	1206	1221	1247	rBV3	210271	539808	100.00%	12.355%
7	5.542	1388	1400	1424	rBV	168009	356016	65.95%	8.148%
8	5.998	1530	1542	1561	rBV	125963	264319	48.97%	6.050%
9	6.921	1816	1829	1849	rBV2	52185	106424	19.72%	2.436%
10	7.252	1919	1932	1956	rBV	224638	418179	77.47%	9.571%
11	7.561	2017	2028	2048	rBV	33876	67957	12.59%	1.555%
12	8.037	2166	2176	2206	rBV	247994	537615	99.59%	12.305%
13	8.792	2399	2411	2436	rBV	255133	438220	81.18%	10.030%
14	10.162	2825	2837	2849	rBV	101455	167206	30.98%	3.827%
15	11.194	3146	3158	3176	rBV	255038	413169	76.54%	9.457%
16	11.496	3239	3252	3261	rBV4	16207	34338	6.36%	0.786%
17	11.570	3264	3275	3294	rVB	238440	389776	72.21%	8.921%
18	15.062	4352	4361	4368	rBV	4631	7916	1.47%	0.181%
19	16.728	4872	4879	4886	rBV6	6086	7139	1.32%	0.163%




Sum of corrected areas: 4369143

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032923\
Data File : VV030334.D
Acq On : 29 Mar 2023 18:09
Operator : SY/MD
Sample : 02092-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB975

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

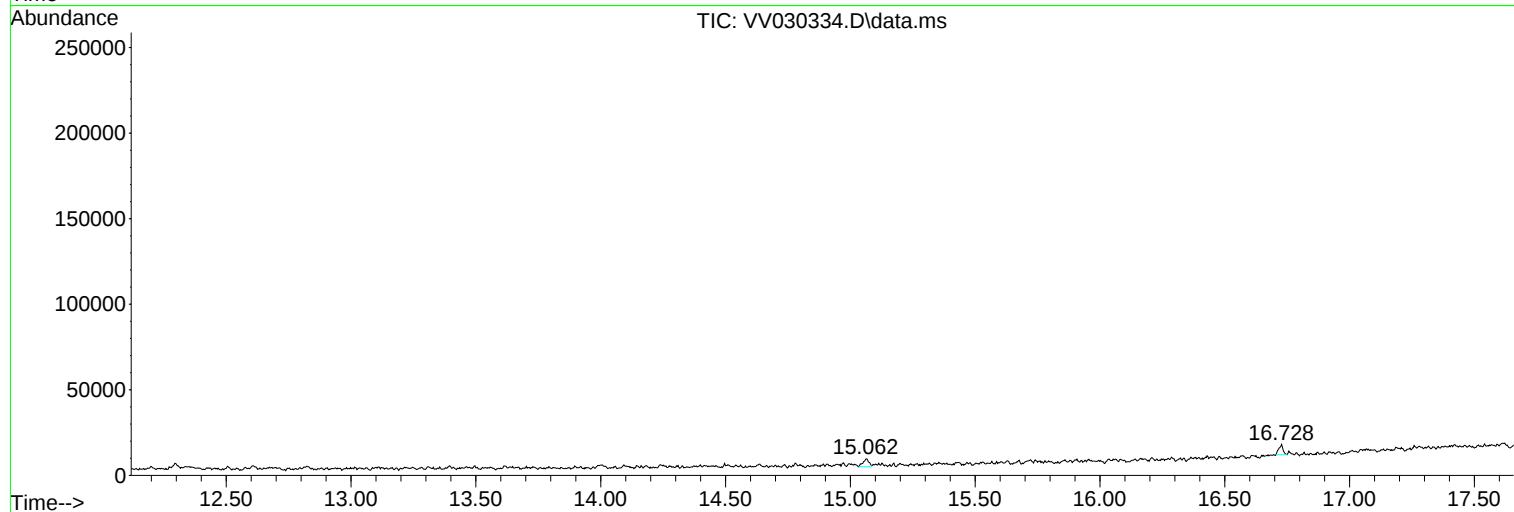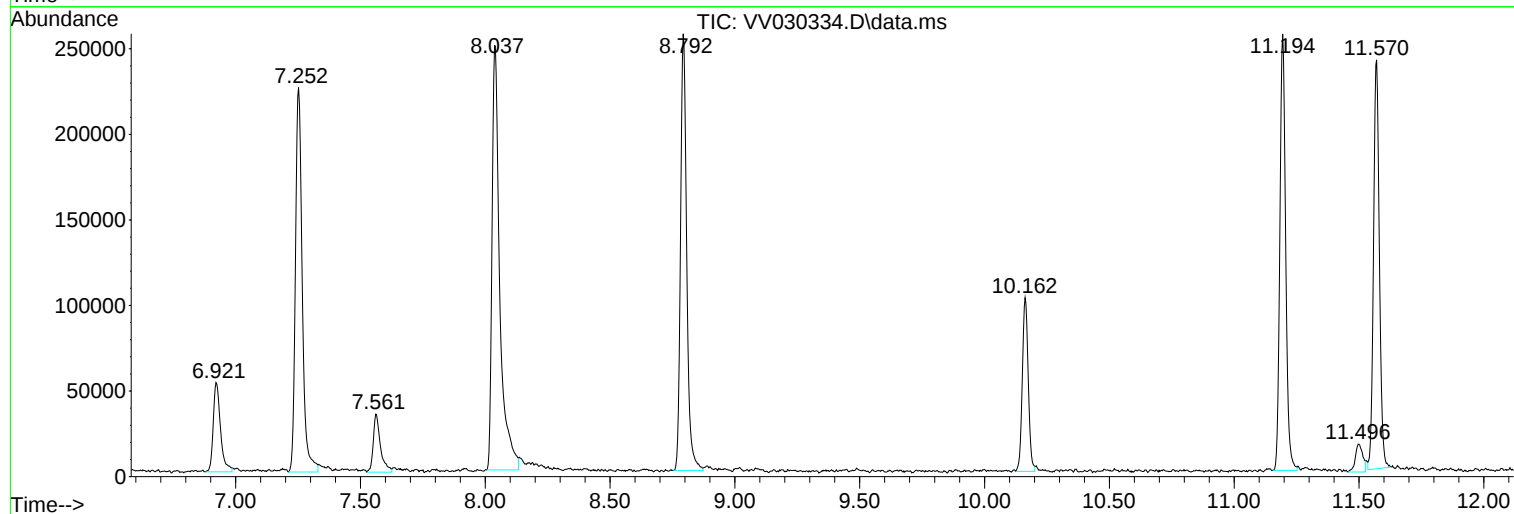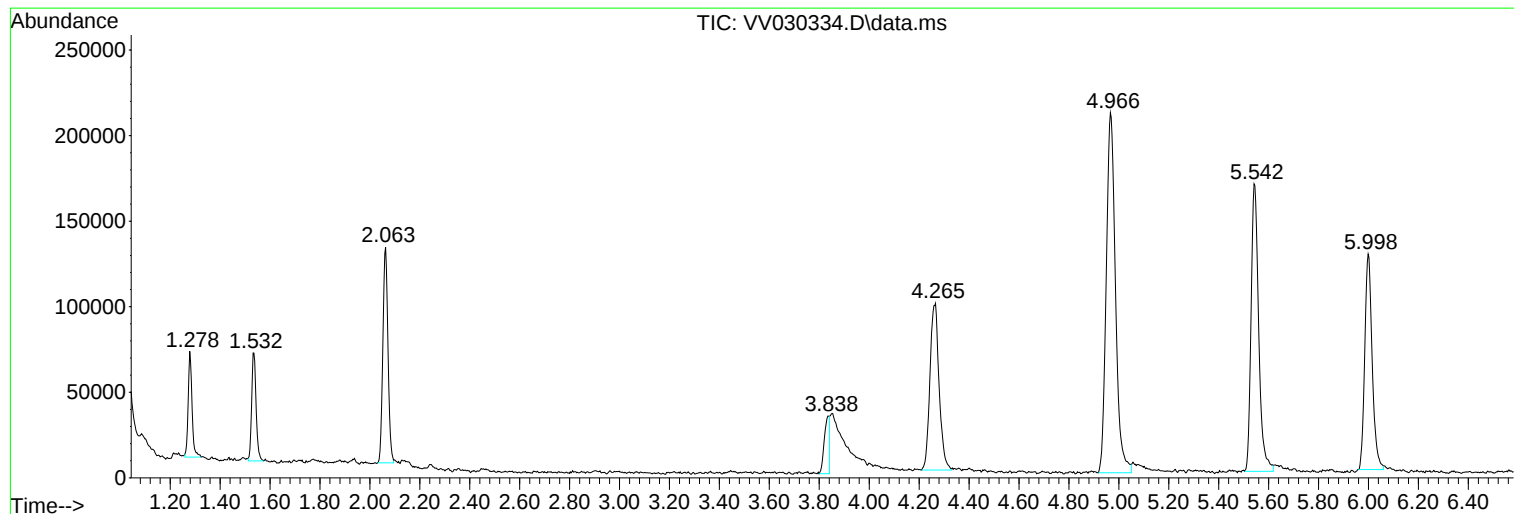

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032923\
Data File : VV030334.D
Acq On : 29 Mar 2023 18:09
Operator : SY/MD
Sample : 02092-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB975

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032923\
Data File : VV030334.D
Acq On : 29 Mar 2023 18:09
Operator : SY/MD
Sample : 02092-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB975

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------