

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032923\
 Data File : VV030339.D
 Acq On : 29 Mar 2023 20:12
 Operator : SY/MD
 Sample : 02092-23 200X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB998

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030339.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.221	51	56	66	rVV	4816	6042	1.18%	0.142%
2	1.282	68	75	92	rVB	60023	65333	12.72%	1.534%
3	1.536	147	154	167	rVB	65001	78693	15.32%	1.847%
4	2.066	308	319	330	rBV	112786	166518	32.41%	3.909%
5	2.452	430	439	449	rBV2	14093	24542	4.78%	0.576%
6	3.812	847	862	893	rBV2	66716	241366	46.98%	5.665%
7	4.265	984	1003	1027	rBV2	98197	251109	48.88%	5.894%
8	4.966	1205	1221	1243	rBV4	197606	513748	100.00%	12.059%
9	5.545	1388	1401	1419	rBV	151989	323184	62.91%	7.586%
10	5.998	1528	1542	1560	rBV	124936	265740	51.73%	6.238%
11	6.921	1819	1829	1843	rBV	50036	95899	18.67%	2.251%
12	7.252	1917	1932	1951	rBV	213422	385621	75.06%	9.051%
13	7.564	2017	2029	2040	rBV2	30982	58548	11.40%	1.374%
14	8.034	2163	2175	2206	rBV	234157	475180	92.49%	11.154%
15	8.368	2268	2279	2298	rBV	27477	53980	10.51%	1.267%
16	8.793	2400	2411	2428	rBV	234139	395382	76.96%	9.281%
17	10.162	2824	2837	2850	rBV	91697	145981	28.41%	3.427%
18	11.194	3147	3158	3174	rBV	232849	366020	71.25%	8.591%
19	11.571	3264	3275	3293	rVB	217499	347416	67.62%	8.155%




Sum of corrected areas: 4260302

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032923\
Data File : VV030339.D
Acq On : 29 Mar 2023 20:12
Operator : SY/MD
Sample : 02092-23 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB998

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

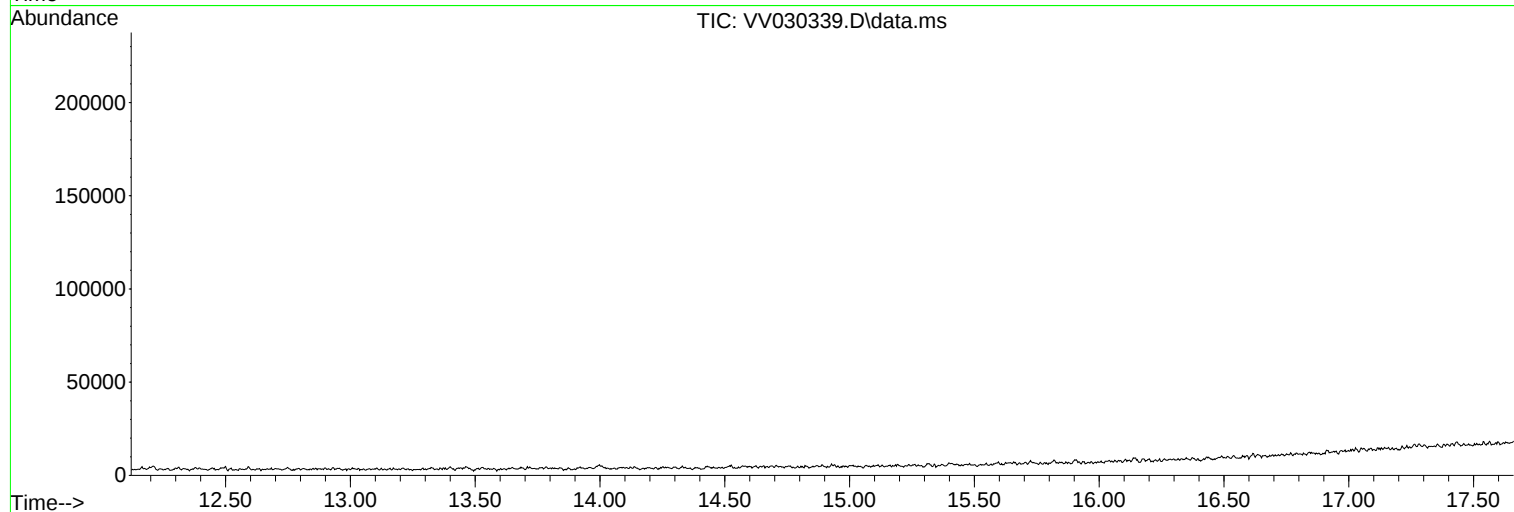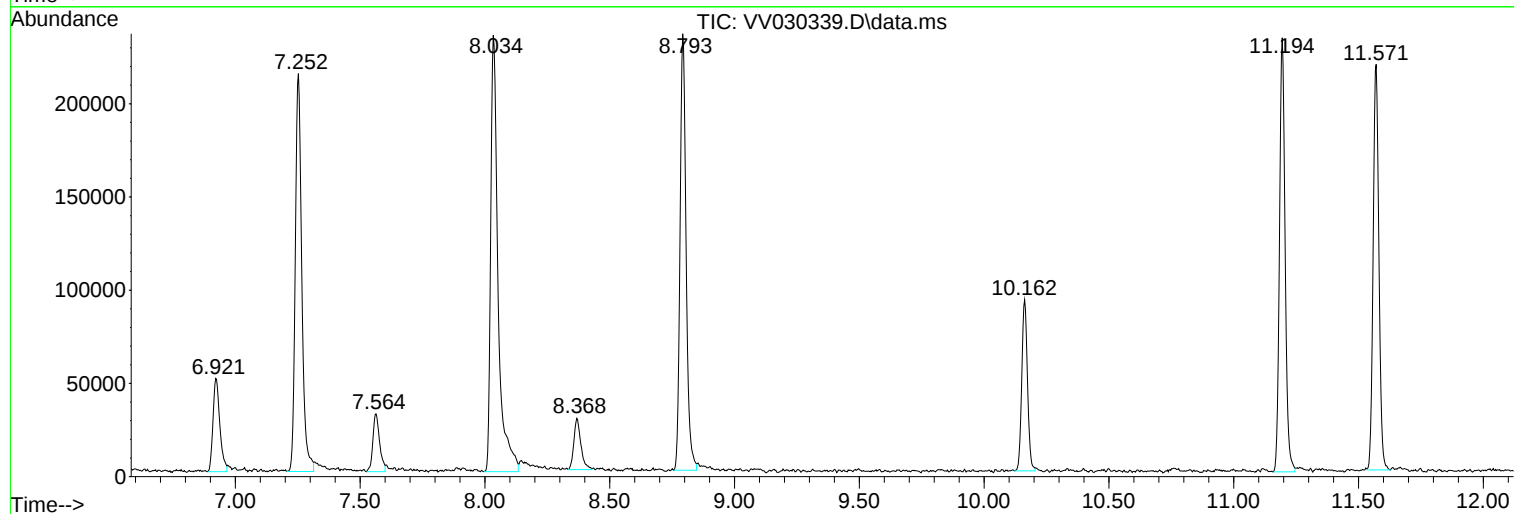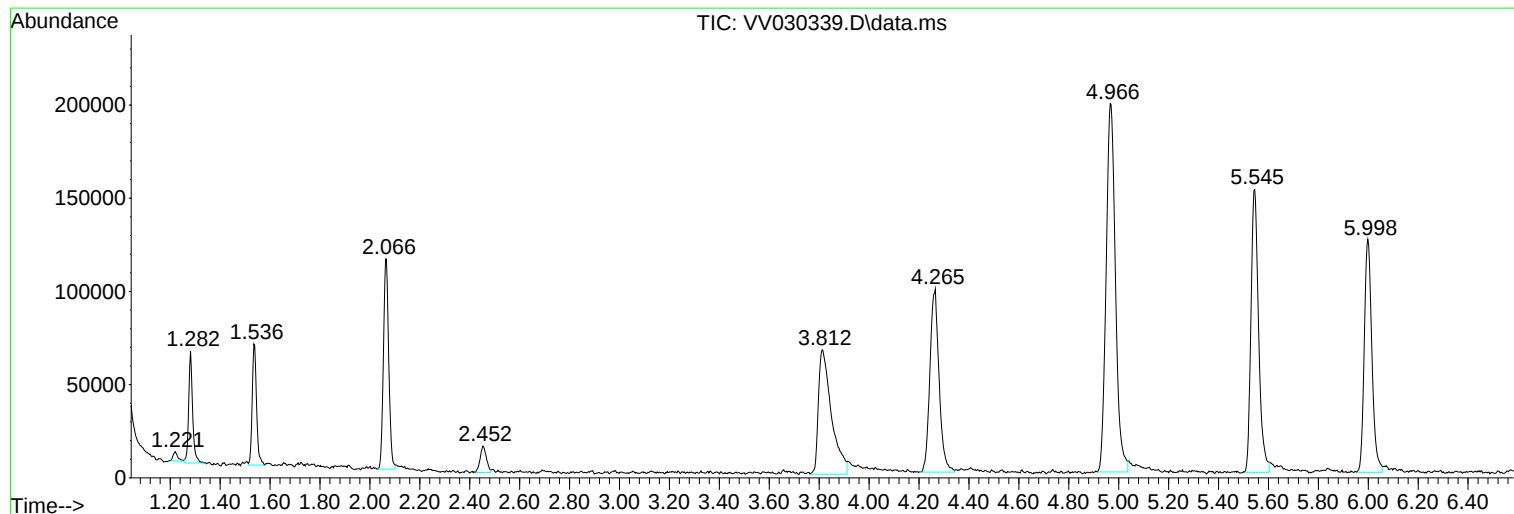

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032923\
Data File : VV030339.D
Acq On : 29 Mar 2023 20:12
Operator : SY/MD
Sample : 02092-23 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB998










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.368	0.68 ug/L	53980	Chlorobenzene-d5	8.793

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Oxalamide, N-(isochroman-1-yl)me...	310	C18H18N2O3	1000304-26-0	35
2			Thioglycolic acid, tert-butyldim...	206	C8H18O2SSi	1000476-01-2	35
3			1H-Indole-3-thiol	149	C8H7NS	000480-94-4	32
4			Oxalamide, N-(2-hydroxyethyl)-N'...	278	C14H18N2O4	1000304-26-2	27
5			Benzamide, N-[(3,4-dihydro-1H-2-...	281	C18H19NO2	1000320-15-7	25

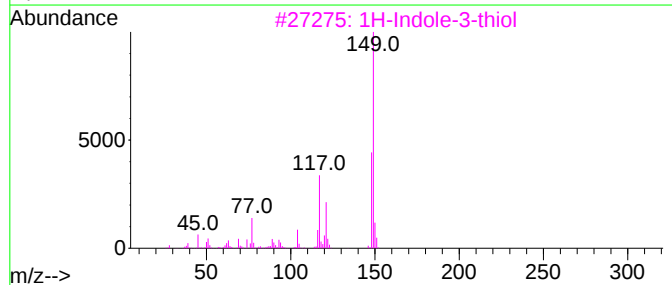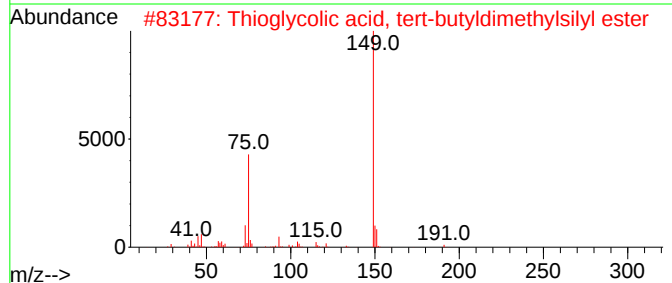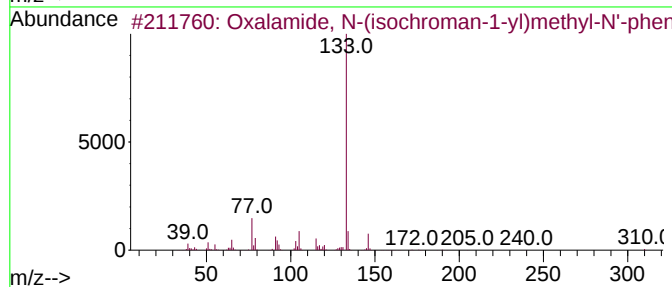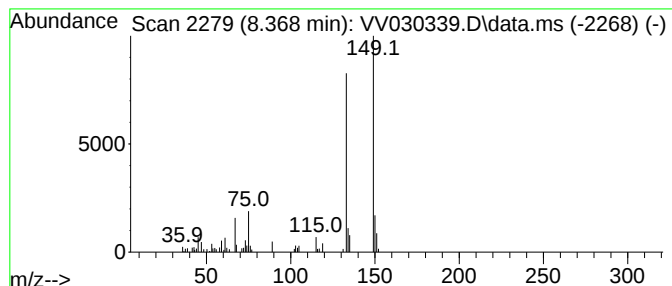

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032923\
Data File : VV030339.D
Acq On : 29 Mar 2023 20:12
Operator : SY/MD
Sample : 02092-23 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB998

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	8.368	0.7	ug/L	53980	2	8.793	395382	5.0