

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032923\
 Data File : VV030340.D
 Acq On : 29 Mar 2023 20:37
 Operator : SY/MD
 Sample : 02122-02 200X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB9A2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030340.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	88	rVB	58508	62261	11.86%	1.430%
2	1.536	146	154	166	rBV	63902	77095	14.69%	1.771%
3	2.066	309	319	332	rBV	117618	173820	33.12%	3.992%
4	2.455	431	440	455	rVB	12902	23004	4.38%	0.528%
5	3.815	849	863	895	rBV2	69726	252071	48.03%	5.789%
6	4.259	982	1001	1031	rBV	95893	251105	47.85%	5.767%
7	4.966	1205	1221	1251	rBV2	198919	524803	100.00%	12.053%
8	5.542	1388	1400	1419	rBV	156891	330911	63.05%	7.600%
9	5.998	1529	1542	1563	rBV2	124206	265564	50.60%	6.099%
10	6.924	1818	1830	1845	rBV	48854	95370	18.17%	2.190%
11	7.252	1918	1932	1959	rBV	210715	395352	75.33%	9.080%
12	7.564	2019	2029	2043	rBV2	30746	58939	11.23%	1.354%
13	8.034	2162	2175	2211	rBV	233991	482931	92.02%	11.091%
14	8.368	2269	2279	2292	rBV2	33207	62852	11.98%	1.443%
15	8.793	2398	2411	2430	rBV	242466	414961	79.07%	9.530%
16	10.162	2823	2837	2853	rBV	94777	152204	29.00%	3.496%
17	11.194	3145	3158	3175	rBV	235377	374777	71.41%	8.607%
18	11.571	3263	3275	3291	rBV	218968	356159	67.87%	8.180%




Sum of corrected areas: 4354179

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032923\
Data File : VV030340.D
Acq On : 29 Mar 2023 20:37
Operator : SY/MD
Sample : 02122-02 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB9A2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

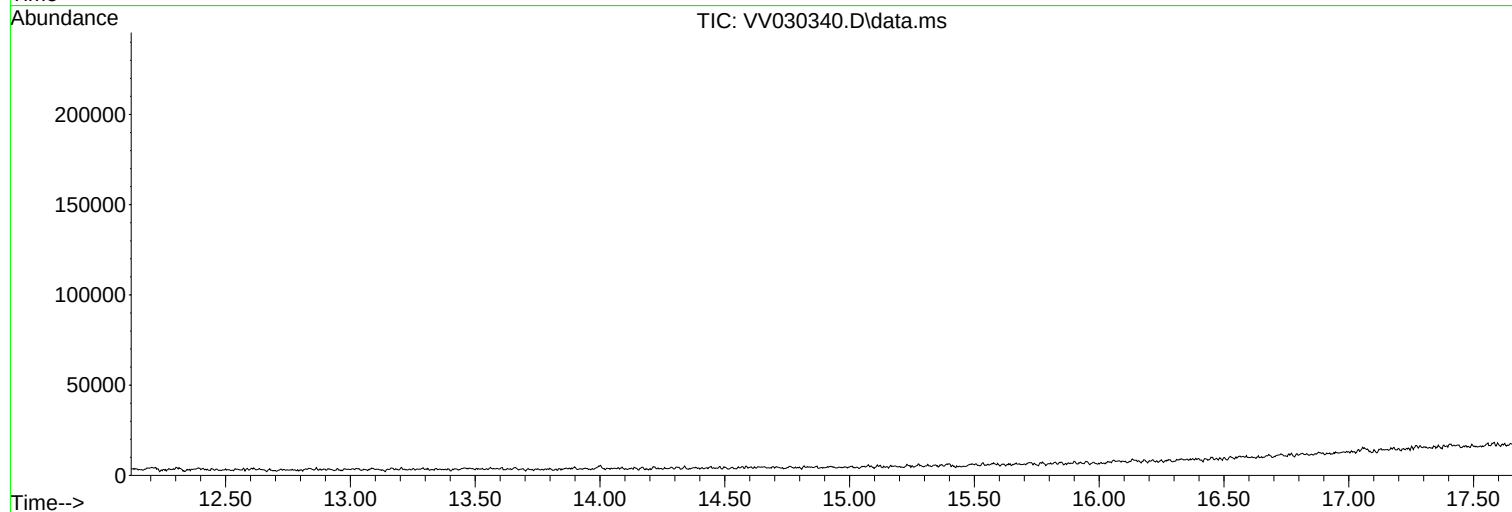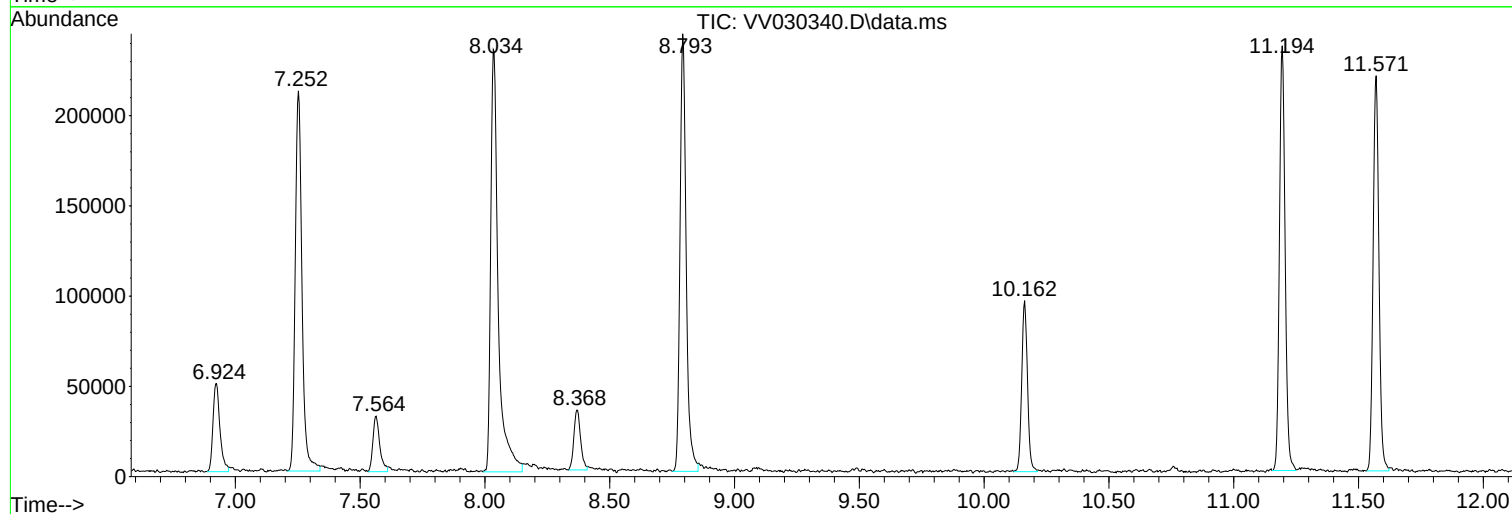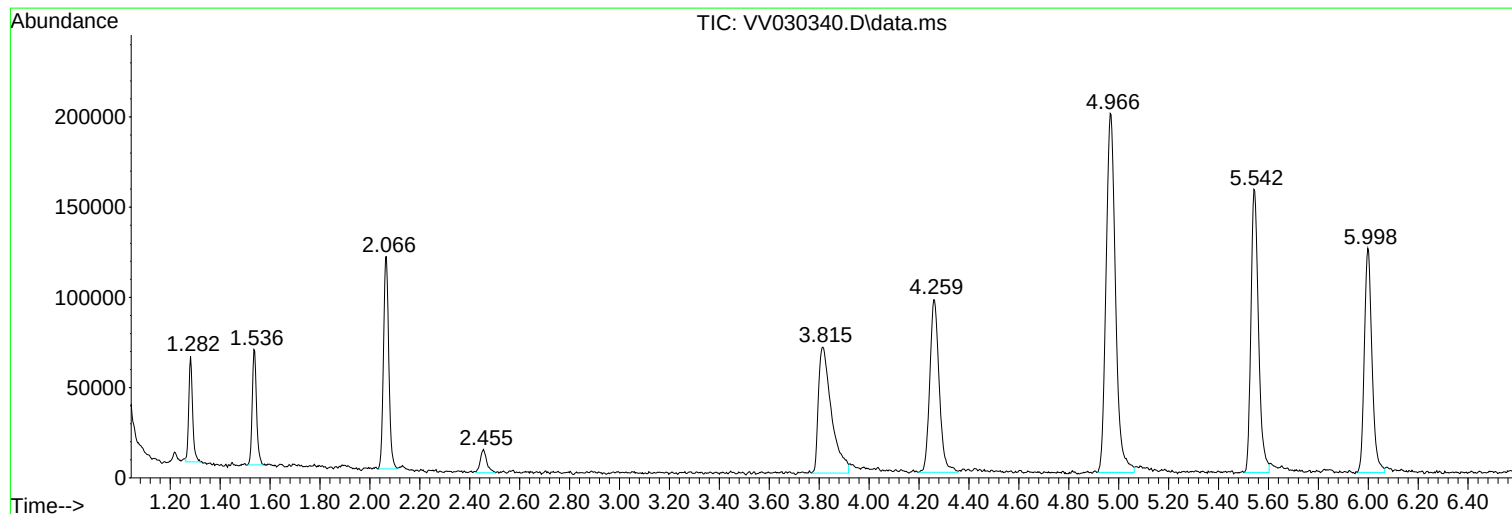

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032923\
Data File : VV030340.D
Acq On : 29 Mar 2023 20:37
Operator : SY/MD
Sample : 02122-02 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB9A2










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.368	0.76 ug/L	62852	Chlorobenzene-d5	8.793

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1H-Indole-3-thiol	149	C8H7NS	000480-94-4	38
2			Silane, dodecyldiethoxymethyl-	302	C17H38O2Si	060317-40-0	35
3			Oxalamide, N-(2-hydroxyethyl)-N'...	278	C14H18N2O4	1000304-26-2	27
4			Oxalamide, N-(isochroman-1-yl)me...	310	C18H18N2O3	1000304-26-0	25
5			1,2,4-Triazole, 3,5-dithioxo-	133	C2H3N3S2	005650-03-3	25

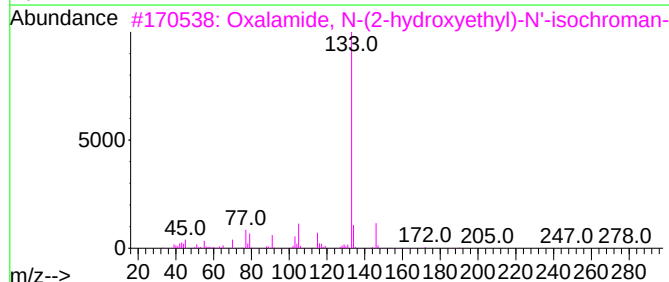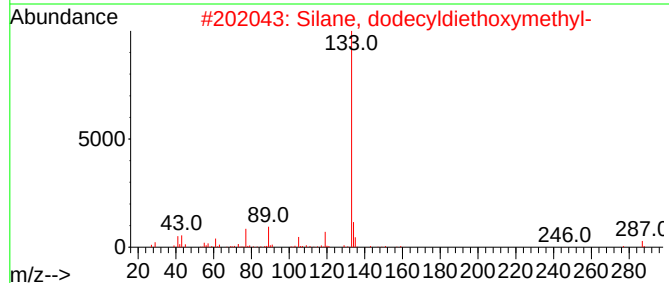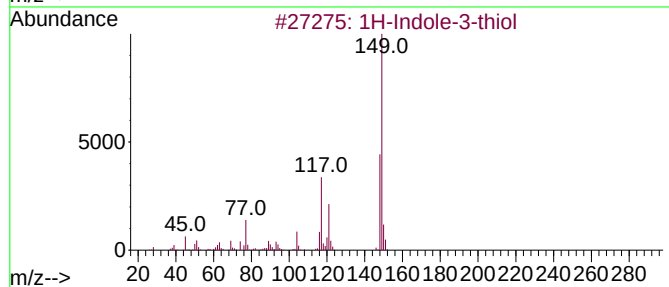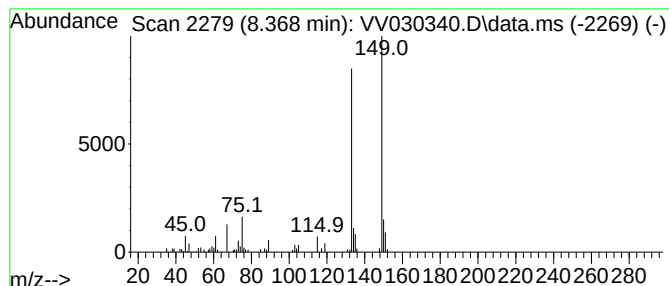

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032923\
Data File : VV030340.D
Acq On : 29 Mar 2023 20:37
Operator : SY/MD
Sample : 02122-02 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB9A2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	8.368	0.8	ug/L	62852	2	8.793	414961	5.0