

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032923\
 Data File : VV030341.D
 Acq On : 29 Mar 2023 21:01
 Operator : SY/MD
 Sample : 02122-04 200X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB9A6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030341.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	51	55	66	rBV	6234	7709	1.38%	0.169%
2	1.282	69	75	85	rVB	60512	63027	11.29%	1.381%
3	1.536	147	154	168	rVB	67914	81006	14.51%	1.775%
4	2.063	304	318	332	rBV	124008	185266	33.18%	4.060%
5	2.452	430	439	449	rBV	12792	20386	3.65%	0.447%
6	3.818	852	864	899	rBV3	68376	253599	45.42%	5.557%
7	4.259	986	1001	1026	rBV2	98705	254134	45.51%	5.569%
8	4.966	1204	1221	1251	rBV2	210624	558362	100.00%	12.236%
9	5.542	1387	1400	1424	rBV	168217	355559	63.68%	7.792%
10	5.998	1528	1542	1566	rBV	130282	277334	49.67%	6.078%
11	6.921	1816	1829	1848	rBV	52943	103468	18.53%	2.267%
12	7.252	1919	1932	1955	rBV	226538	417317	74.74%	9.145%
13	7.561	2018	2028	2040	rBV	33515	60921	10.91%	1.335%
14	8.034	2164	2175	2207	rBV	246830	498645	89.30%	10.927%
15	8.368	2269	2279	2291	rBV	25765	47496	8.51%	1.041%
16	8.793	2400	2411	2433	rBV	261484	441696	79.11%	9.679%
17	10.162	2824	2837	2851	rBV	94610	156744	28.07%	3.435%
18	11.194	3145	3158	3174	rBV	252744	400876	71.80%	8.785%
19	11.571	3262	3275	3292	rBV	238258	379697	68.00%	8.321%




Sum of corrected areas: 4563242

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032923\
Data File : VV030341.D
Acq On : 29 Mar 2023 21:01
Operator : SY/MD
Sample : 02122-04 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB9A6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

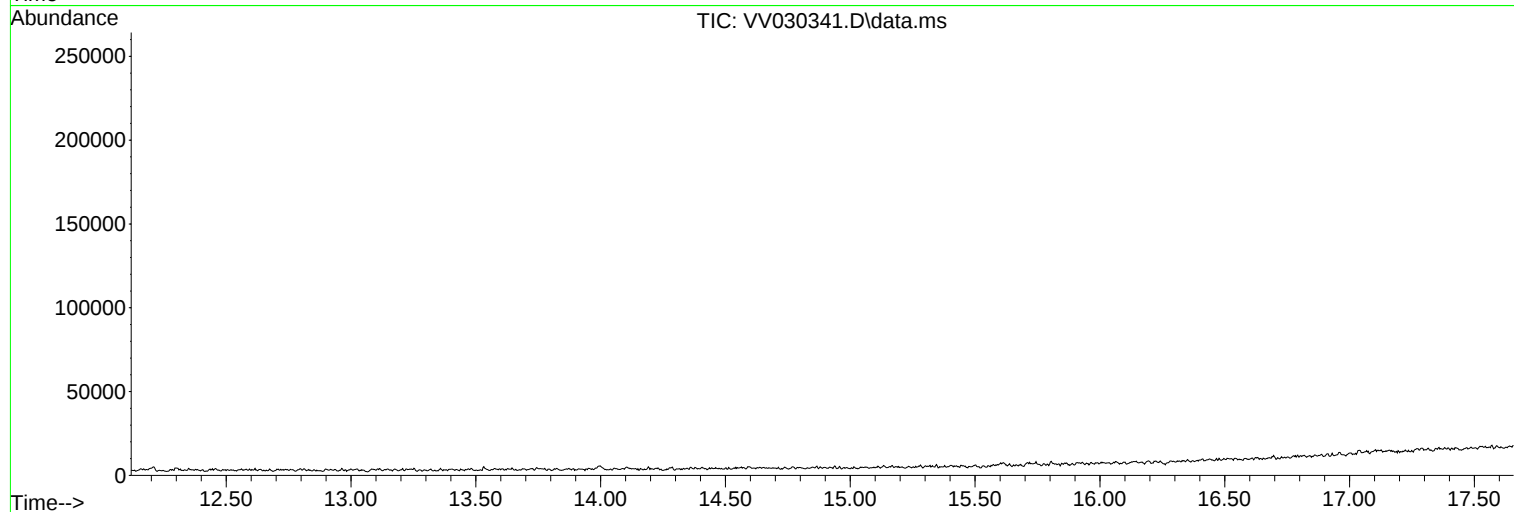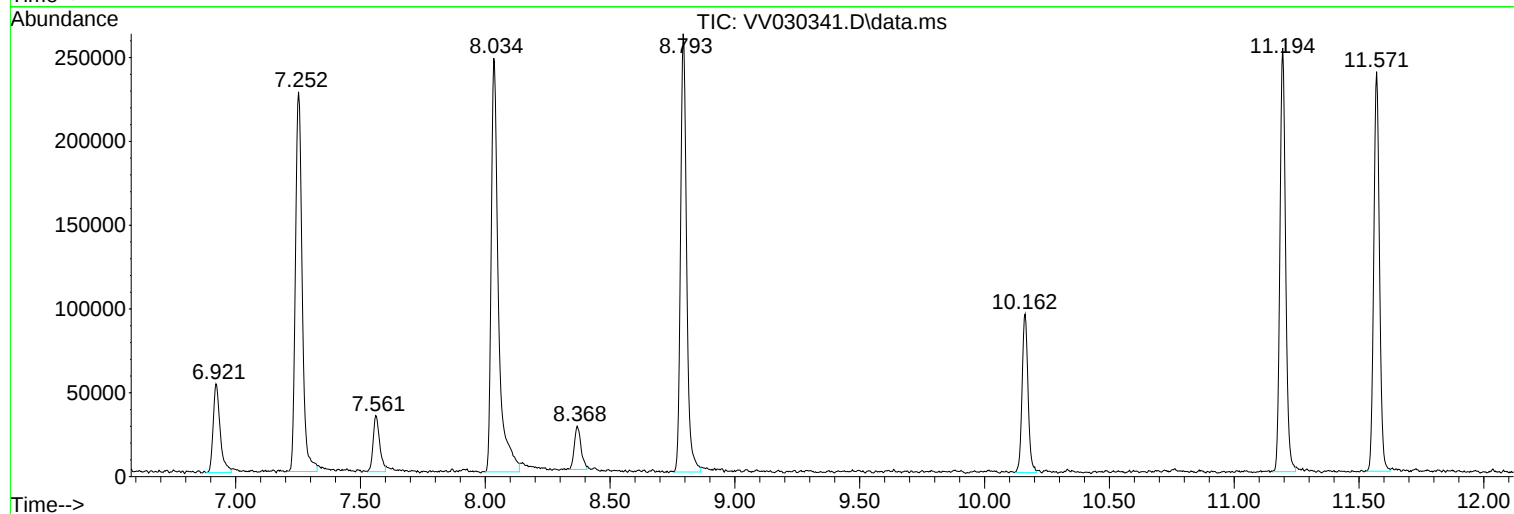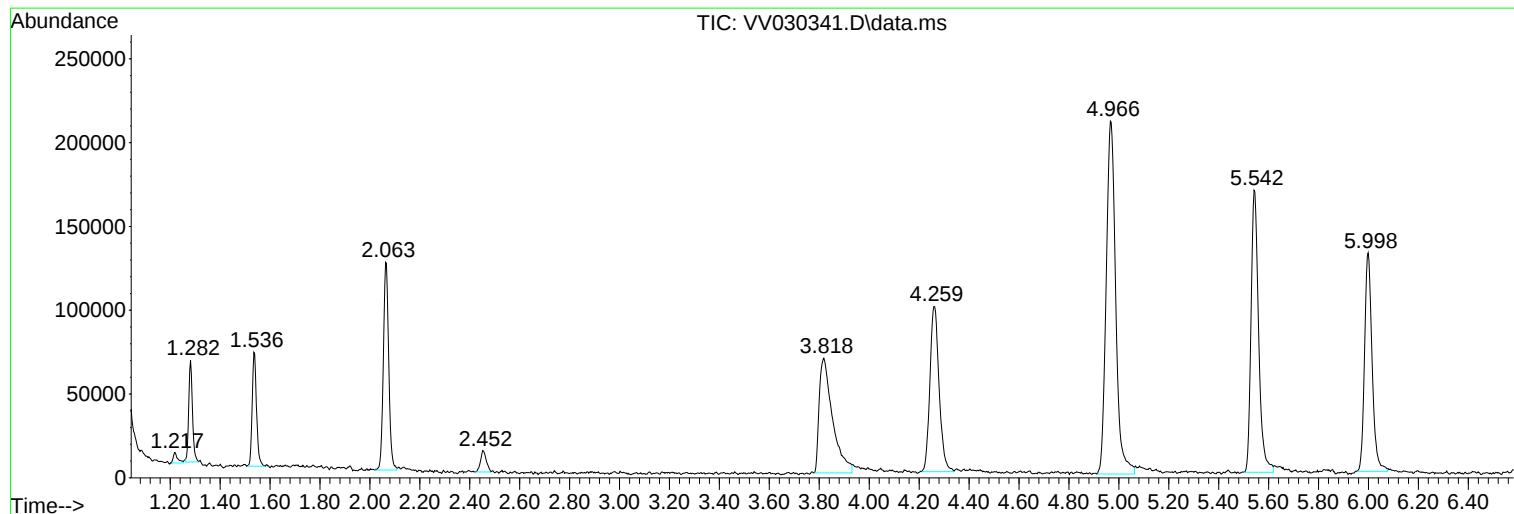

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032923\
Data File : VV030341.D
Acq On : 29 Mar 2023 21:01
Operator : SY/MD
Sample : 02122-04 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB9A6










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.368	0.54 ug/L	47496	Chlorobenzene-d5	8.793

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2,4,6-Trimethylbenzyl mercaptan,...	362	C14H13F7OS	1000469-60-5	35		
2	1,2,4-Triazole, 3,5-dithioxo-	133	C2H3N3S2	005650-03-3	35		
3	Benzene, 1,1'-(oxydi-2,1-ethaned...	282	C20H26O	055044-09-2	23		
4	Silane, dodecyl-diethoxymethyl-	302	C17H38O2Si	060317-40-0	17		
5	Benzoic acid, 4-[(3,4-dihydro-1...	325	C19H19NO4	1000316-21-6	17		

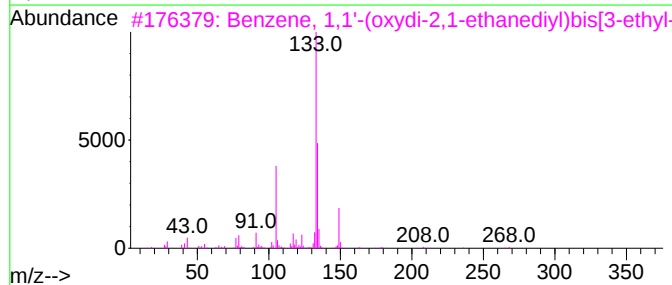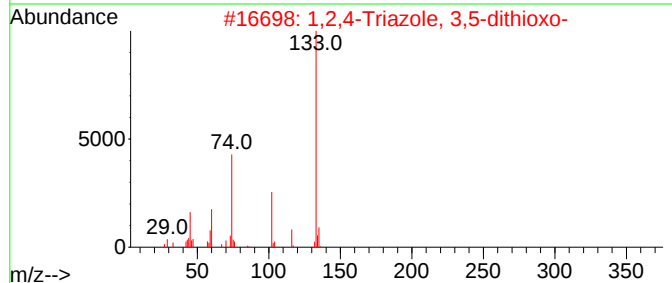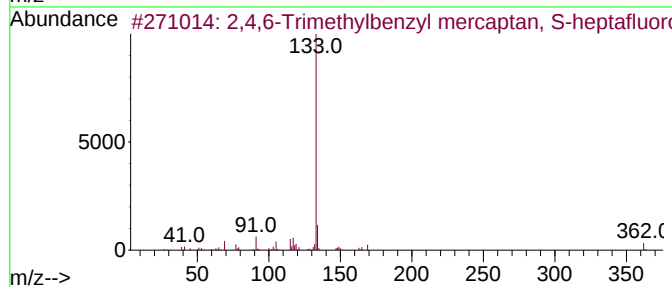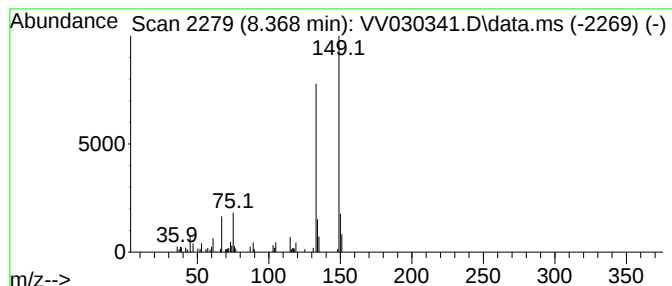

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032923\
Data File : VV030341.D
Acq On : 29 Mar 2023 21:01
Operator : SY/MD
Sample : 02122-04 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB9A6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	8.368	0.5	ug/L	47496	2	8.793	441696	5.0