
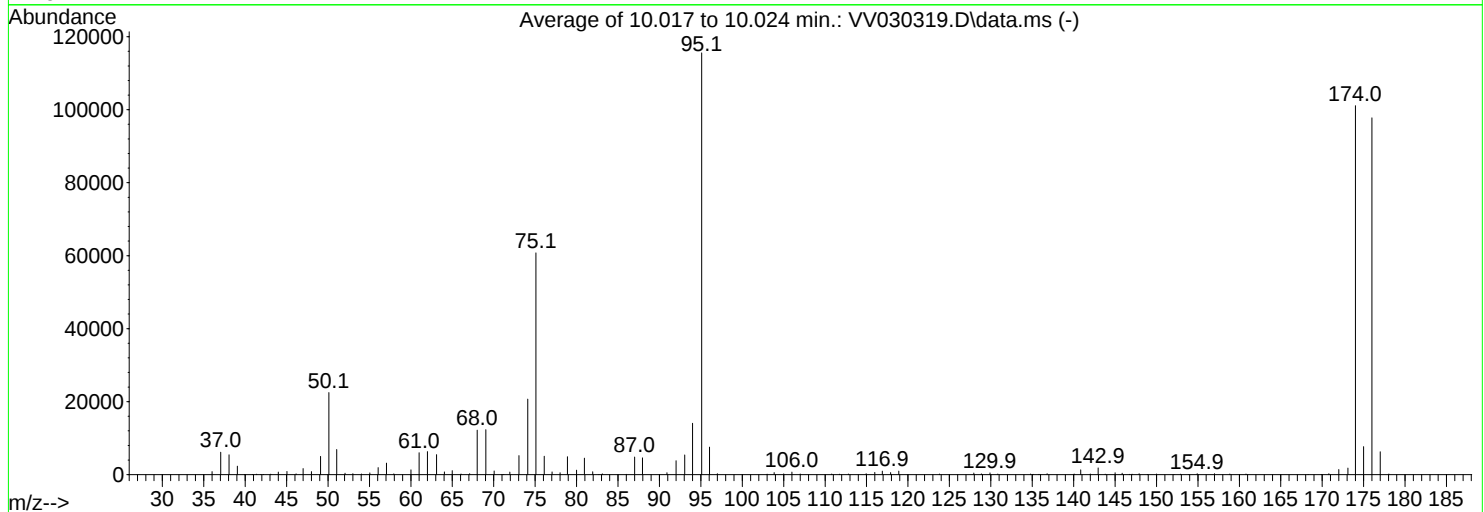


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032923\
Data File : VV030319.D
Acq On : 29 Mar 2023 11:21
Operator : SY/MD
Sample : BFB239
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB239

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Mar 31 05:37:21 2023

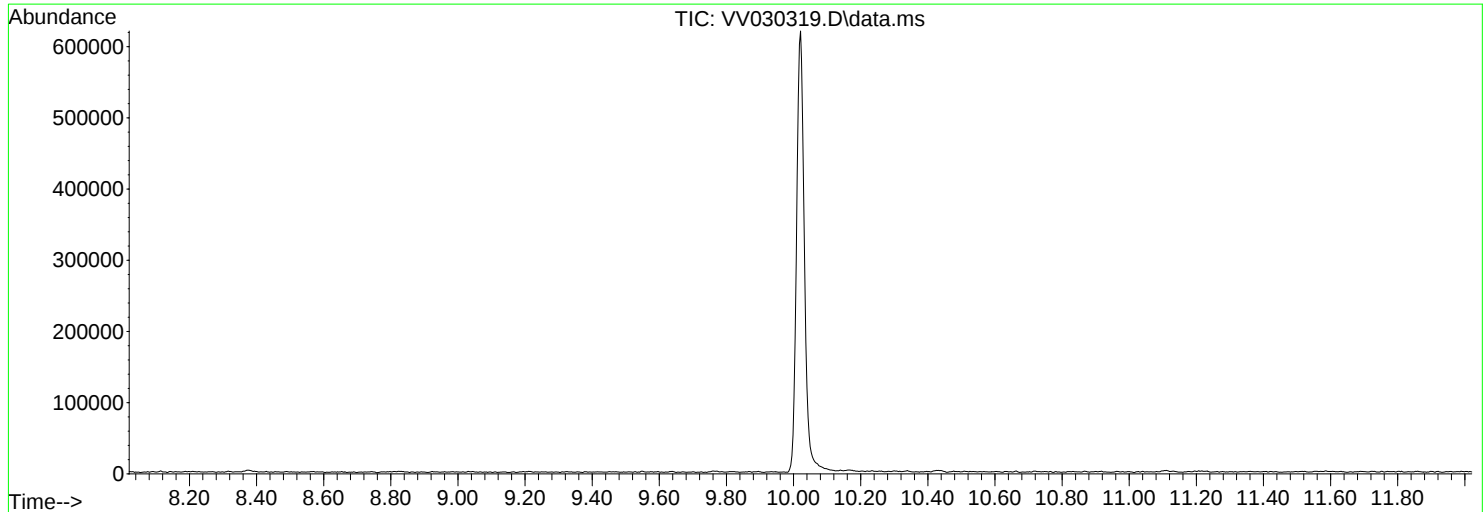

AutoFind: Scans 2792, 2793, 2794; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	22507	PASS
75	95	30	80	52.6	60789	PASS
95	95	100	100	100.0	115581	PASS
96	95	5	9	6.5	7535	PASS
173	174	0.00	2	1.8	1812	PASS
174	95	50	120	87.5	101096	PASS
175	174	5	9	7.6	7678	PASS
176	174	95	105	96.7	97779	PASS
177	176	5	10	6.4	6271	PASS

m/z	Abundance
36.00	152.0
37.00	183.0
38.00	156.0
39.00	107.0
39.90	284.0
42.30	136.0
42.70	126.0
44.10	327.0
45.00	117.0
47.40	115.0
49.80	111.0
72.50	134.0
77.10	118.0
82.00	118.0

Instrument :
MSVOA_V
ClientSampleId :
BFB239

m/z	Abundance
36.00	960.0
37.10	6503.0
38.10	5642.0
39.10	2543.0
39.90	294.0
40.90	152.0
41.40	121.0
41.90	162.0
42.30	167.0
42.90	225.0
44.00	954.0
45.10	1009.0
46.20	280.0
47.00	1756.0
48.00	909.0
49.10	5245.0
50.10	22616.0
51.10	7097.0
52.10	411.0
53.00	236.0
54.10	189.0
55.00	507.0
56.10	1960.0
57.00	3109.0
58.00	185.0
60.00	1296.0
61.00	6235.0
62.00	6290.0
63.10	5602.0
64.10	843.0
65.00	993.0
66.10	211.0
67.10	270.0
68.00	12680.0
69.00	12487.0
70.00	1114.0
71.00	114.0
72.00	673.0
73.00	5115.0
74.10	21024.0
75.10	61464.0
76.10	5131.0
77.10	835.0
78.00	569.0
78.90	5083.0
80.00	1230.0
80.90	4648.0
82.00	961.0
83.10	215.0
87.00	4787.0
88.00	4997.0
90.90	493.0
92.00	3906.0
93.10	5367.0
94.00	14305.0
95.10	116008.0
96.10	7708.0
97.00	298.0
103.00	128.0
103.90	638.0
105.00	193.0
106.00	667.0
107.00	167.0
110.80	158.0
111.70	127.0
112.80	179.0
115.00	251.0
116.00	569.0
116.90	1013.0
117.90	622.0
118.90	930.0
123.80	189.0
127.90	383.0
128.90	294.0
129.80	463.0
130.90	206.0
135.10	204.0
135.80	170.0
136.80	303.0
140.00	159.0
140.90	1299.0
142.00	185.0
143.00	1903.0
143.80	132.0
145.00	547.0
145.90	421.0
146.70	120.0
147.10	129.0
147.90	285.0
150.00	199.0
152.90	113.0
153.90	104.0

Instrument :
MSVOA_V
ClientSampleId :
BFB239

154.90	291.0
157.00	281.0
159.00	142.0
160.80	159.0
170.80	226.0
172.00	1379.0
173.10	1758.0
174.00	99456.0
175.00	7632.0
176.00	96160.0
177.00	6289.0
178.10	195.0

Instrument :
MSVOA_V
ClientSampleId :
BFB239

m/z	Abundance
36.10	1011.0
37.10	6507.0
38.10	5781.0
39.10	2509.0
40.00	291.0
41.40	122.0
42.10	179.0
43.10	177.0
44.00	1037.0
45.10	1023.0
46.20	246.0
47.00	1765.0
48.00	876.0
49.10	5111.0
50.10	23264.0
51.10	7093.0
52.10	405.0
53.00	246.0
54.10	195.0
55.00	468.0
56.10	2062.0
57.10	3286.0
57.90	205.0
60.00	1371.0
61.00	6195.0
62.00	6551.0
63.10	5645.0
64.00	781.0
65.00	1101.0
66.00	197.0
67.10	271.0
68.00	12569.0
69.10	12807.0
70.00	1070.0
71.20	112.0
72.00	722.0
73.10	5404.0
74.10	21352.0
75.10	62760.0
76.10	5210.0
77.00	912.0
78.00	541.0
78.90	5116.0
80.00	1283.0
81.00	4614.0
82.00	953.0
83.10	224.0
86.10	155.0
87.00	4989.0
87.90	4727.0
90.90	548.0
92.00	3959.0
93.00	5546.0
94.00	14527.0
95.10	119384.0
96.10	7681.0
97.00	270.0
103.00	138.0
103.90	574.0
105.00	221.0
106.00	745.0
107.00	191.0
110.80	183.0
111.70	146.0
112.80	163.0
114.90	290.0
116.00	636.0
116.90	995.0
117.90	576.0
118.90	1001.0
123.80	174.0
128.00	418.0
128.80	234.0
129.90	466.0
130.80	203.0
134.80	259.0
135.80	125.0
136.80	278.0
140.10	180.0
140.90	1353.0
142.00	204.0
142.90	1889.0
143.80	146.0
145.00	534.0
145.90	439.0
146.80	131.0
147.10	126.0
147.90	299.0
150.00	193.0
152.10	105.0
152.90	124.0
154.90	290.0

Instrument :
MSVOA_V
ClientSampleId :
BFB239

157.00	246.0
158.80	180.0
160.80	180.0
170.80	306.0
172.00	1450.0
173.10	1856.0
174.00	104656.0
175.00	7907.0
176.00	101136.0
177.00	6546.0
178.10	196.0

Instrument :
MSVOA_V
ClientSampleId :
BFB239

m/z	Abundance
36.10	1026.0
37.10	5922.0
38.10	5411.0
39.10	2241.0
40.00	282.0
41.40	135.0
42.10	205.0
43.10	161.0
44.00	1061.0
45.10	939.0
46.10	197.0
47.00	1461.0
48.00	792.0
49.10	4622.0
50.10	21640.0
51.00	6490.0
52.00	380.0
53.00	263.0
54.00	179.0
55.10	455.0
56.00	1829.0
57.10	3152.0
57.90	218.0
60.00	1273.0
61.00	5537.0
62.00	6175.0
63.10	5181.0
64.00	689.0
65.00	1143.0
66.00	173.0
67.10	279.0
68.00	11355.0
69.10	11664.0
70.10	904.0
71.90	729.0
73.10	5154.0
74.10	19728.0
75.10	58144.0
76.10	4754.0
77.00	865.0
78.00	434.0
78.90	4592.0
80.00	1237.0
81.00	4251.0
81.90	873.0
82.70	165.0
83.10	200.0
85.90	170.0
87.00	4705.0
87.90	4082.0
90.90	580.0
92.00	3614.0
93.00	5277.0
94.00	13464.0
95.10	111352.0
96.00	7217.0
97.00	204.0
103.00	111.0
103.80	461.0
105.00	209.0
106.00	709.0
107.00	183.0
110.80	194.0
111.80	169.0
112.80	139.0
114.90	284.0
116.00	600.0
116.90	898.0
117.90	519.0
118.90	917.0
123.80	121.0
128.00	460.0
128.80	201.0
130.00	476.0
130.80	182.0
134.80	266.0
136.00	108.0
136.80	275.0
140.10	149.0
140.80	1271.0
142.00	204.0
142.90	1705.0
143.80	131.0
145.00	458.0
145.80	349.0
147.00	135.0
147.90	268.0
148.90	103.0
150.00	152.0
152.90	107.0
154.90	277.0
157.00	212.0

Instrument :
MSVOA_V
ClientSampleId :
BFB239

158.80	165.0
160.80	184.0
168.30	104.0
169.90	100.0
170.80	306.0
172.00	1430.0
173.10	1823.0
174.00	99176.0
175.00	7495.0
176.00	96040.0
177.00	5979.0
178.00	196.0

Instrument :
MSVOA_V
ClientSampleId :
BFB239