


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033019\
Data File : VV010028.D
Acq On : 30 Mar 2019 18:56
Operator : SY/MD
Sample : K2166-14
Misc : 5.87G/10mL/MSVOA V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BF0M4

Manual Integrations
APPROVED

MMDadoda
4/1/2019 4:01:39 AM

Quant Time: Mar 31 21:18:05 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM032619S.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 30 23:31:11 2019
Response via : Initial Calibration

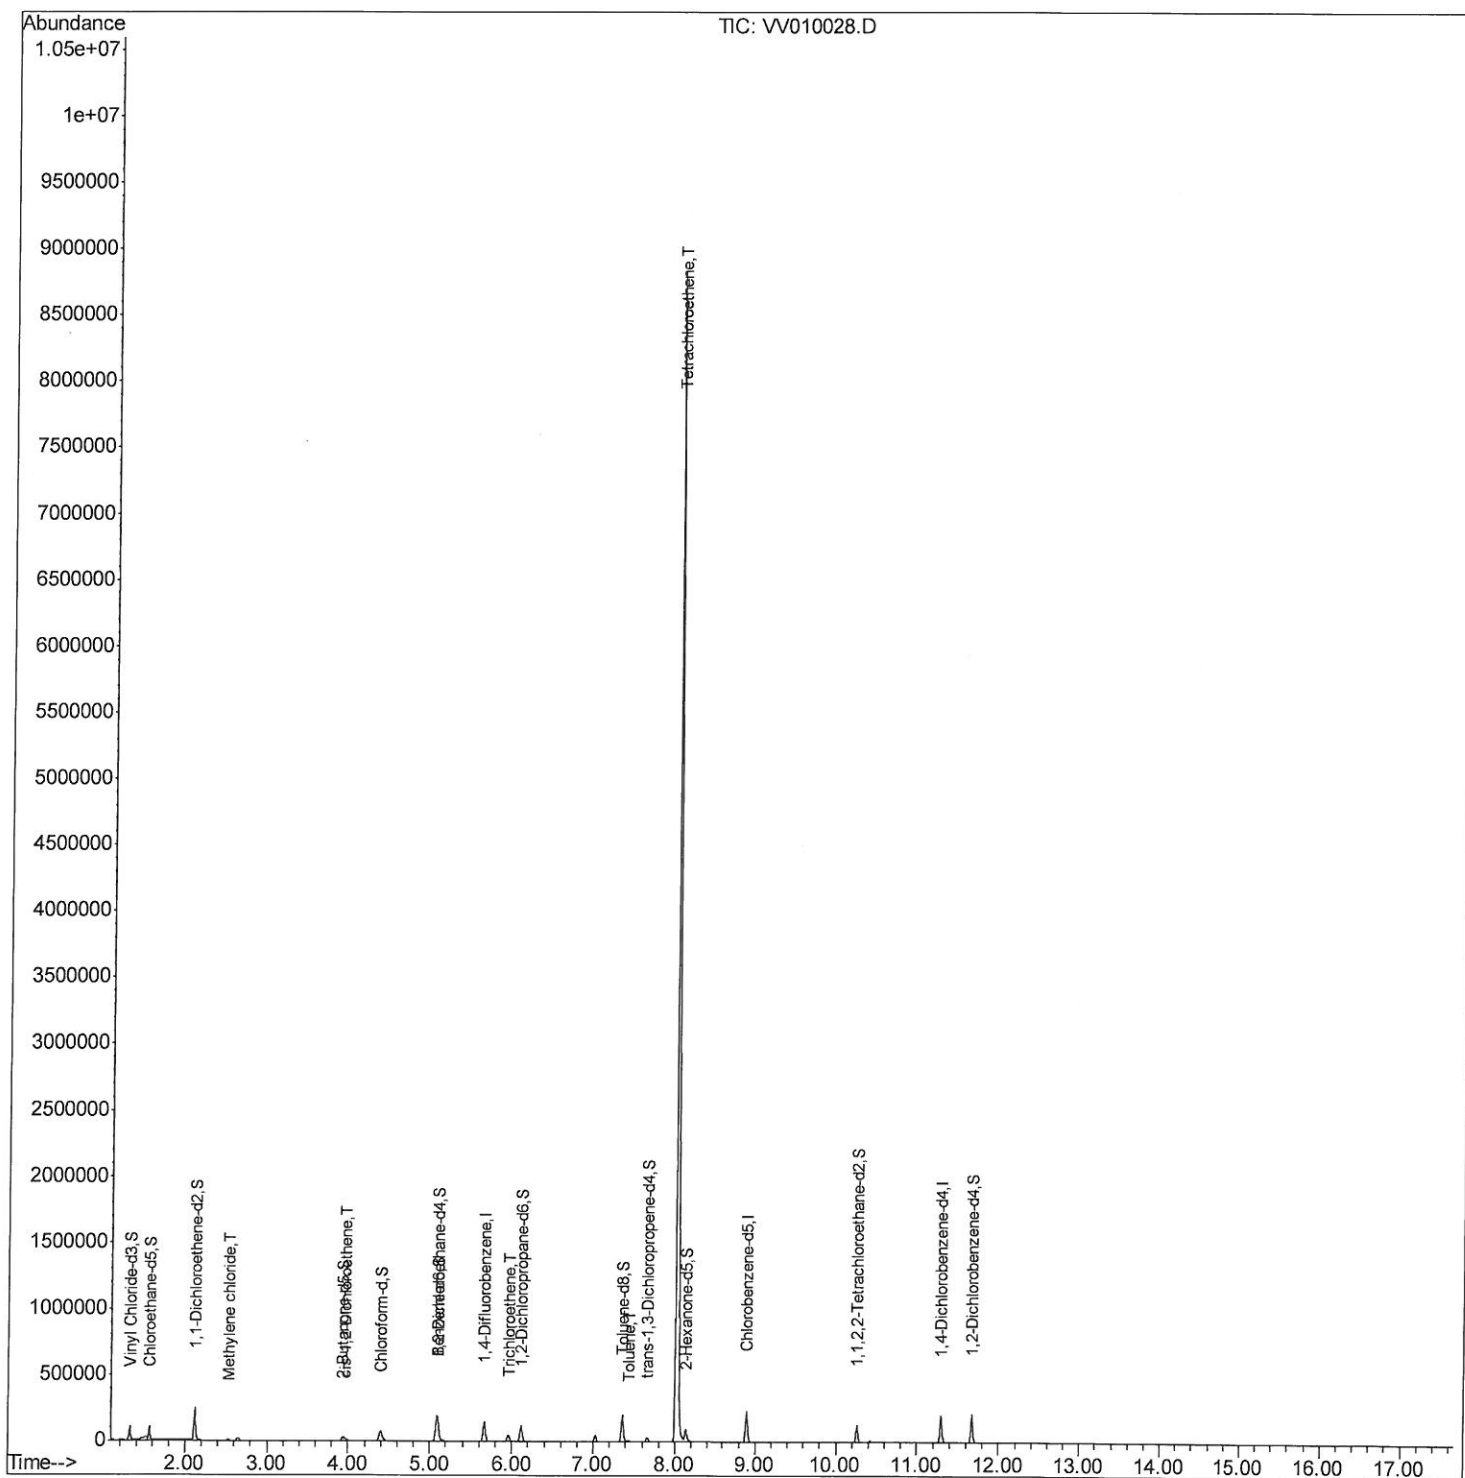

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV033019\
 Data File : VV010028.D
 Acq On : 30 Mar 2019 18:56
 Operator : SY/MD
 Sample : K2166-14
 Misc : 5.87G/10mL/MSVOA_V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BF0M4

Manual Integrations
 APPROVED

MMDadoda
 4/1/2019 4:01:39 AM

Quant Time: Mar 30 23:36:11 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM032619S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 30 23:31:11 2019
 Response via : Initial Calibration

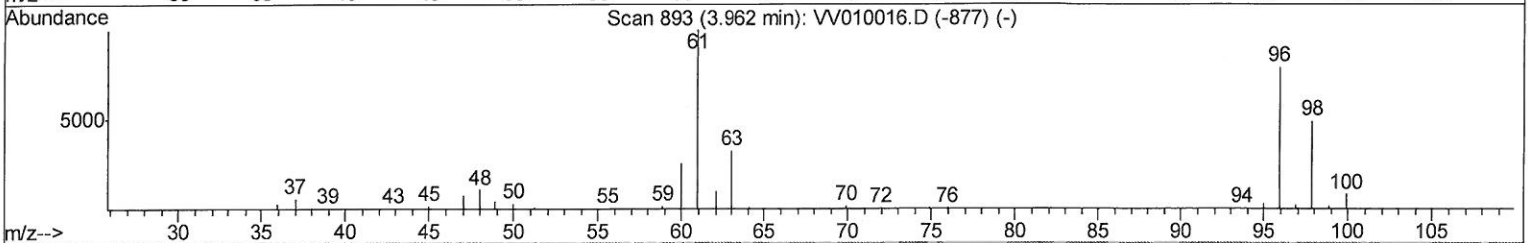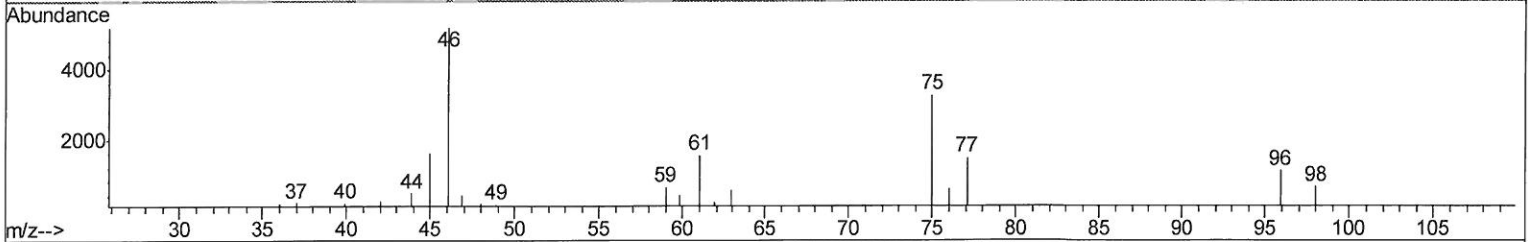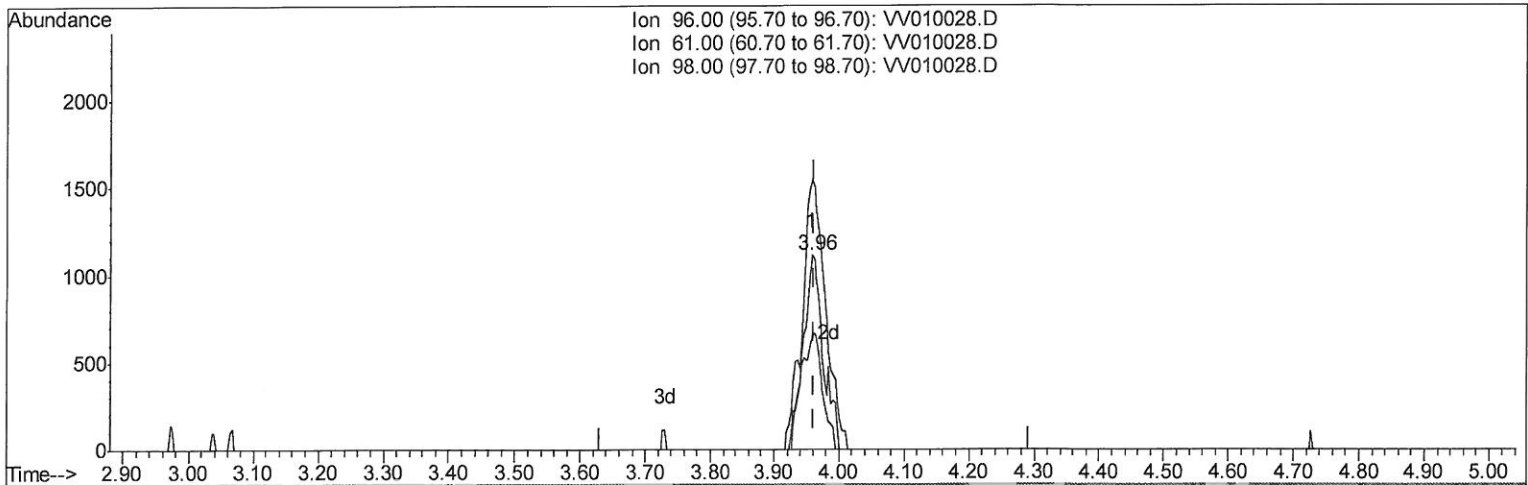

TIC: VV010028.D

(22) cis-1,2-Dichloroethene (T)

3.958min (-0.003) 1.38ug/L m

response 2355

MD
 4/1/3/19

Ion	Exp%	Act%
96.00	100	100
61.00	130.60	138.44
98.00	68.60	58.60
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV033019\
 Data File : VV010028.D
 Acq On : 30 Mar 2019 18:56
 Operator : SY/MD
 Sample : K2166-14
 Misc : 5.87G/10mL/MSVOA_V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BF0M4

Manual Integrations
 APPROVED

MMDadoda
 4/1/2019 4:01:39 AM

Quant Time: Mar 30 23:36:11 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM032619S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 30 23:31:11 2019
 Response via : Initial Calibration

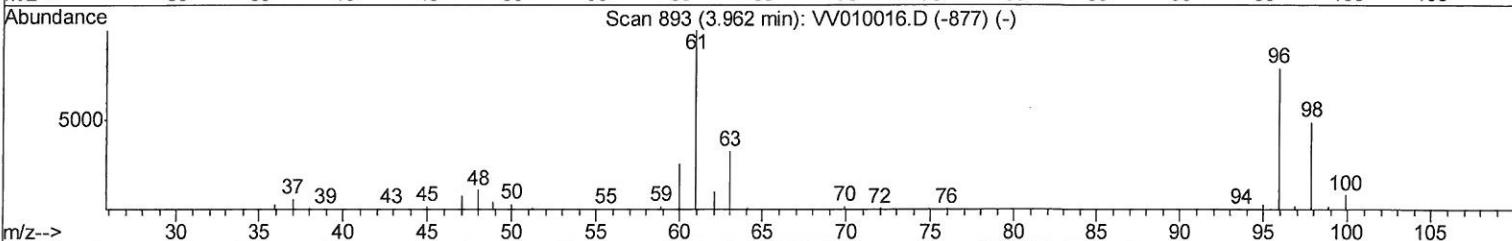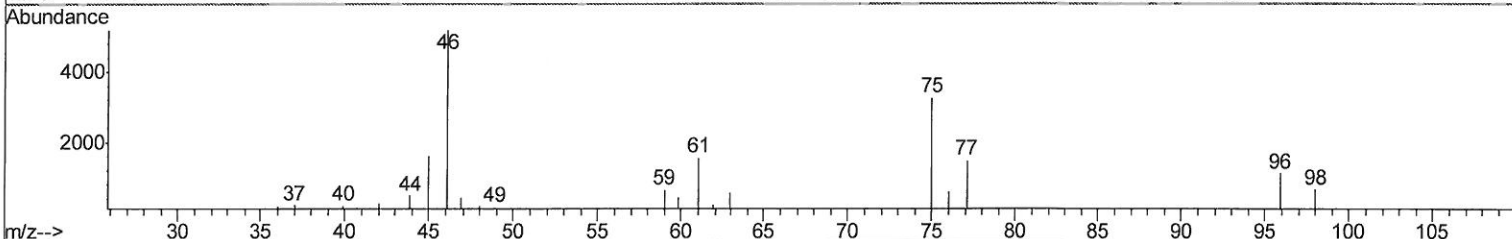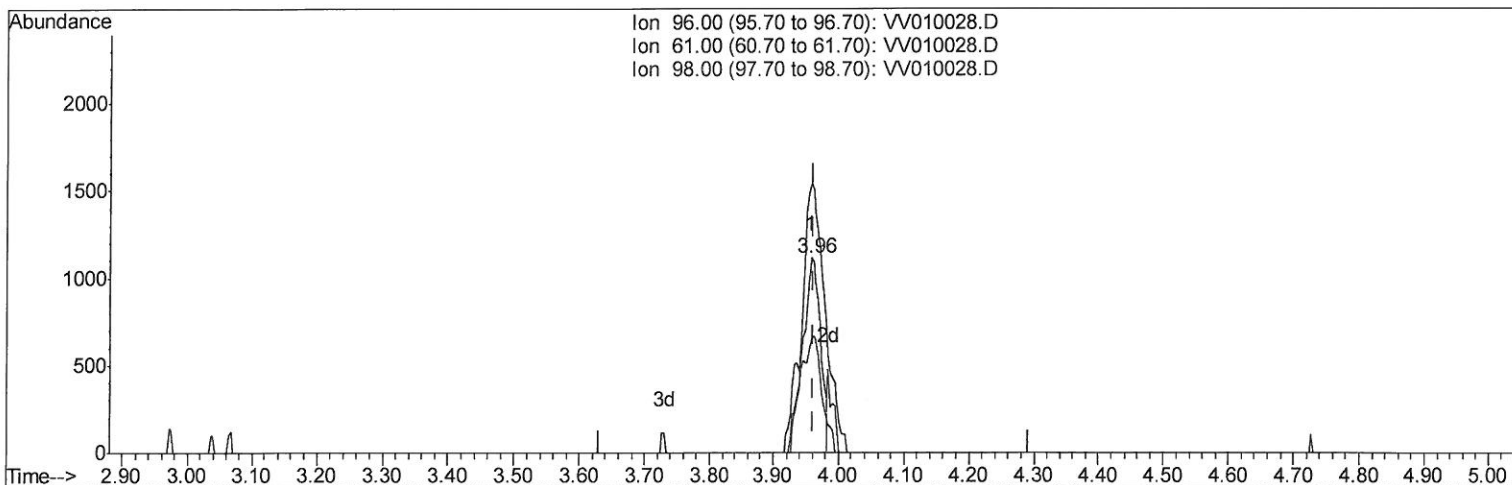

TIC: VV010028.D

(22) cis-1,2-Dichloroethene (T)

3.958min (-0.003) 1.22ug/L

response 2074

Ion	Exp%	Act%
96.00	100	100
61.00	130.60	138.44
98.00	68.60	58.60
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VW033019\
 Data File : VV010028.D
 Acq On : 30 Mar 2019 18:56
 Operator : SY/MD
 Sample : K2166-14
 Misc : 5.87G/10mL/MSVOA V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BF0M4

Manual Integrations
 APPROVED

MMDadoda
 4/1/2019 4:01:39 AM

Quant Time: Mar 31 21:18:05 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM032619S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 30 23:31:11 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	117773	25.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	119717	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	48445	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	53078	22.21	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	88.84%
7) Chloroethane-d5	1.56	69	63324	24.53	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	98.12%
10) 1,1-Dichloroethene-d2	2.12	63	119825	18.33	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	73.32%
20) 2-Butanone-d5	3.93	46	35968	80.76	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	161.52%#
24) Chloroform-d	4.40	84	66508	22.17	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	88.68%
26) 1,2-Dichloroethane-d4	5.08	65	54358	30.10	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	120.40%
29) Benzene-d6	5.10	84	152705	24.29	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	97.16%
33) 1,2-Dichloropropane-d6	6.12	67	50243	27.32	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	109.28%
37) Toluene-d8	7.36	98	132036	22.19	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	88.76%
38) trans-1,3-Dichloropropene-	7.66	79	15892	21.12	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	84.48%
39) 2-Hexanone-d5	8.13	63	27187	79.19	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	158.38%#
48) 1,1,2,2-Tetrachloroethane-	10.26	84	56819	31.20	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	124.80%#
61) 1,2-Dichlorobenzene-d4	11.68	152	49293	26.73	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	106.92%

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
16) Methylene chloride	2.53	84	4142	2.136	ug/L	80
22) cis-1,2-Dichloroethene	3.96	96	2355m	1.382	ug/L	90
35) Trichloroethene	5.96	95	14133	8.150	ug/L	82
44) Toluene	7.43	91	3301	0.455	ug/L	96
47) Tetrachloroethene	8.02	164	1632602	1193.098	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed