


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033019\
Data File : VV010031.D
Acq On : 30 Mar 2019 20:15
Operator : SY/MD
Sample : K2166-17
Misc : 5.97G/10mL/MSVOA V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BF0N4

Manual Integrations
APPROVED

MMDadoda
4/1/2019 4:01:39 AM

Quant Time: Mar 31 21:19:25 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM032619S.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 30 23:31:11 2019
Response via : Initial Calibration

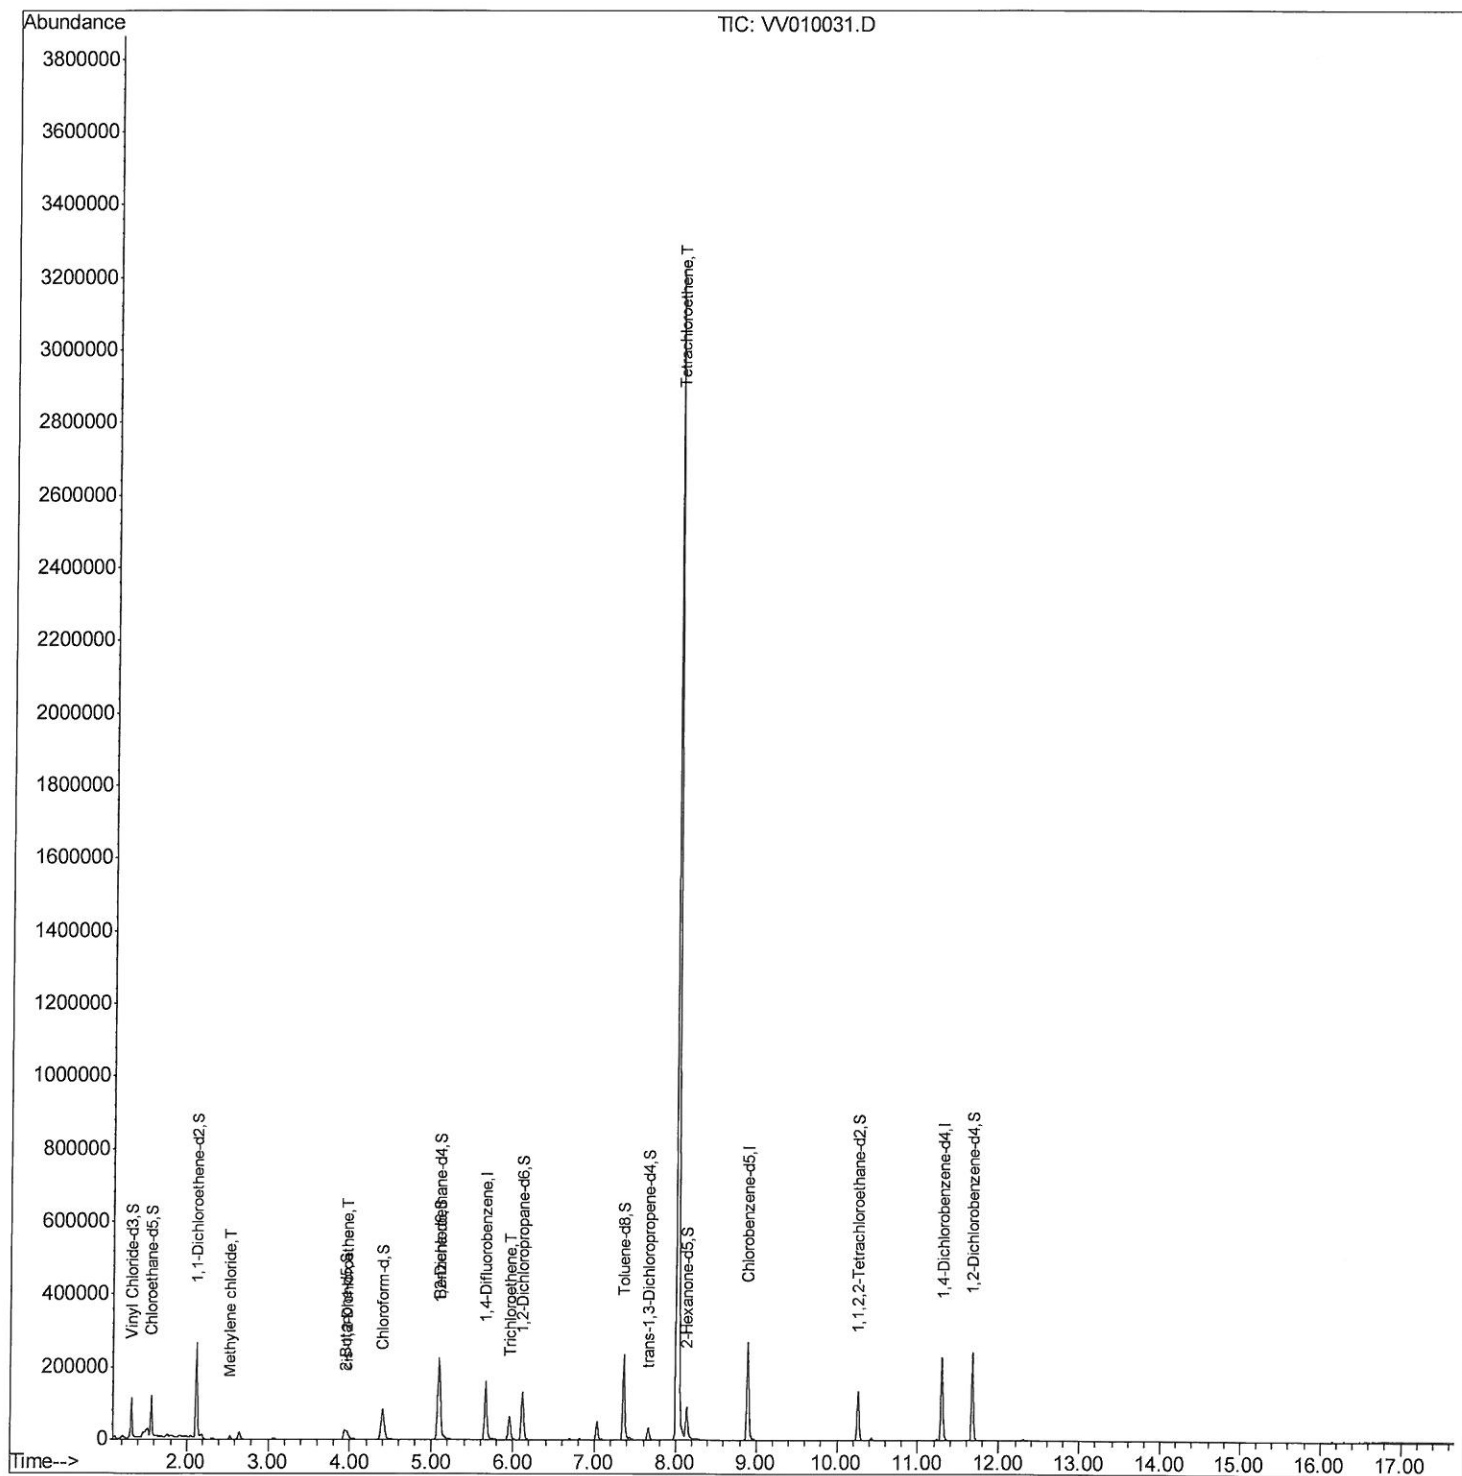

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV033019\
 Data File : VV010031.D
 Acq On : 30 Mar 2019 20:15
 Operator : SY/MD
 Sample : K2166-17
 Misc : 5.97G/10mL/MSVOA_V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
ClientSampleId :
 BF0N4

Manual Integrations
APPROVED

MMDadoda
 4/1/2019 4:01:39 AM

Quant Time: Mar 30 23:36:31 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM032619S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 30 23:31:11 2019
 Response via : Initial Calibration

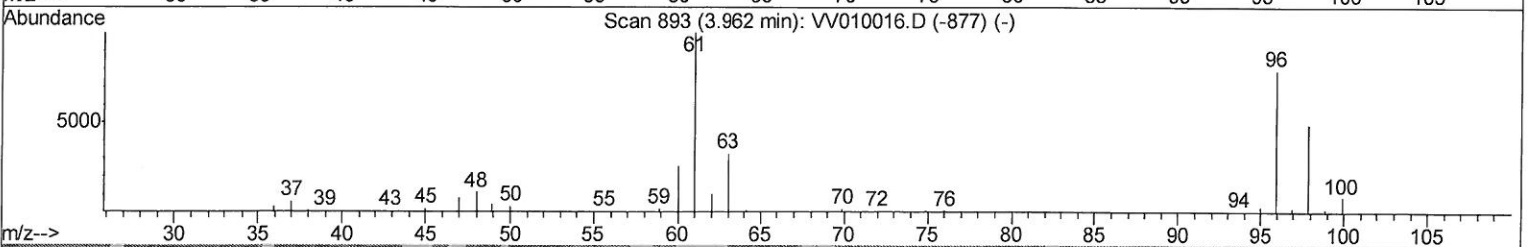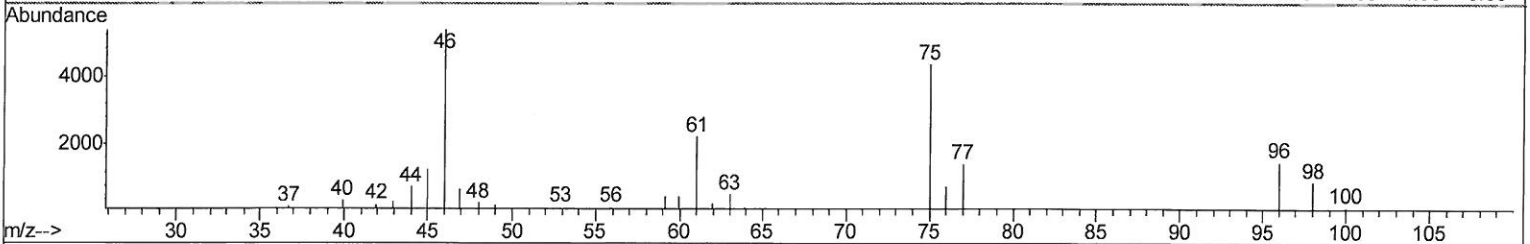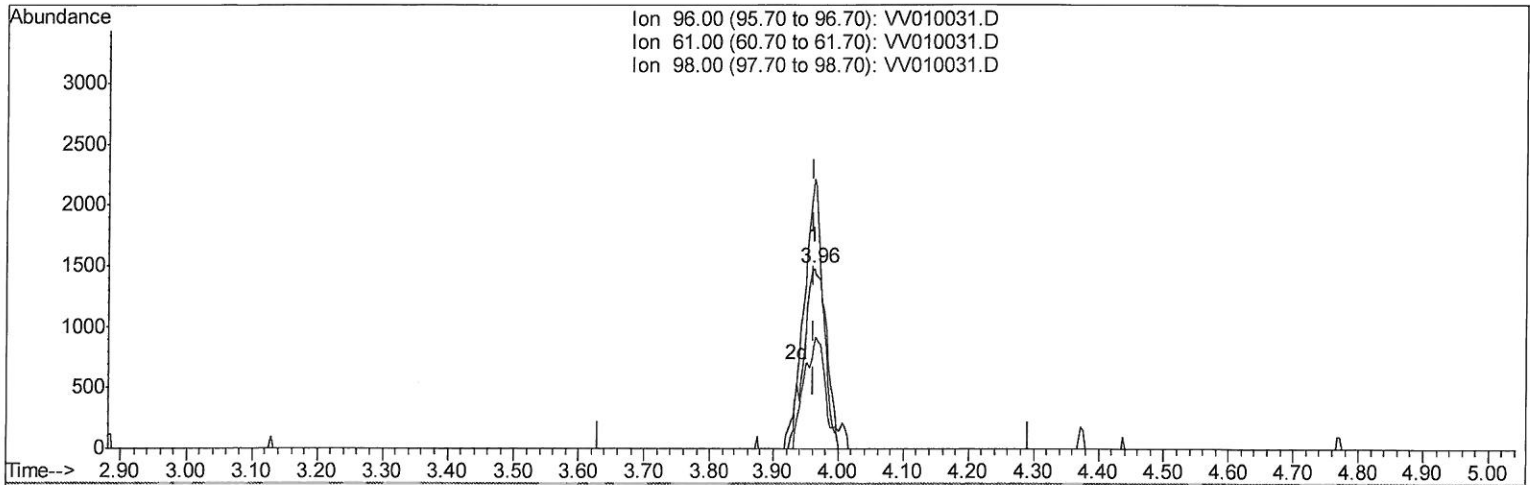

TIC: VV010031.D

(22) cis-1,2-Dichloroethene (T)

3.961min (-0.000) 1.84ug/L m

response 3417

MD
4/13/19

Ion	Exp%	Act%
96.00	100	100
61.00	130.60	149.33
98.00	68.60	59.30
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV033019\
 Data File : VV010031.D
 Acq On : 30 Mar 2019 20:15
 Operator : SY/MD
 Sample : K2166-17
 Misc : 5.97G/10mL/MSVOA_V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BF0N4

Manual Integrations
 APPROVED

MMDadoda
 4/1/2019 4:01:39 AM

Quant Time: Mar 30 23:36:31 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM032619S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 30 23:31:11 2019
 Response via : Initial Calibration

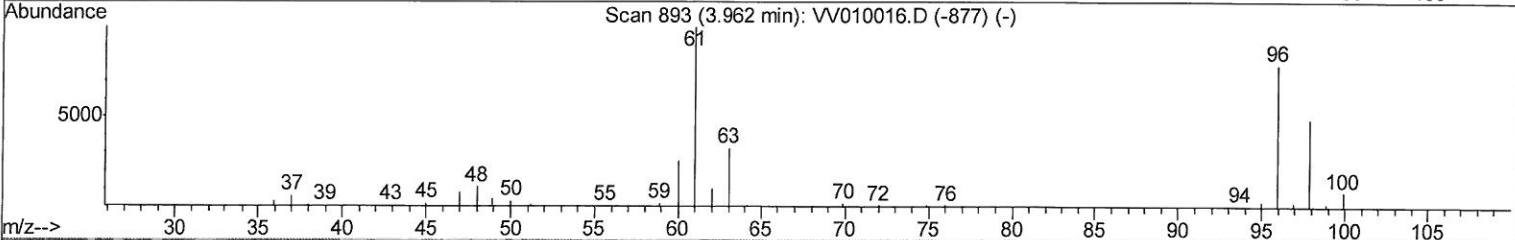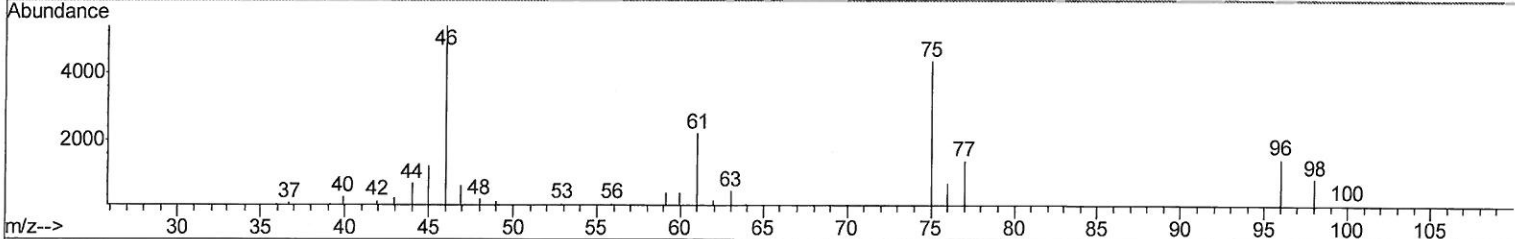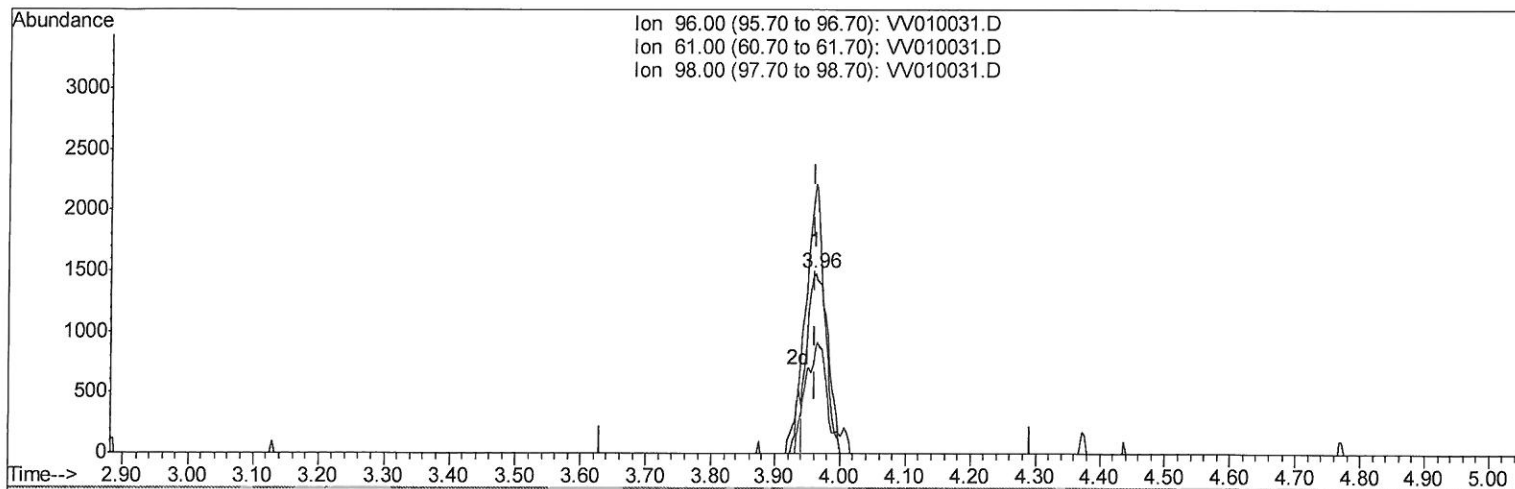

TIC: VV010031.D

(22) cis-1,2-Dichloroethene (T)

3.961min (-0.000) 1.68ug/L

response 3117

Ion	Exp%	Act%
96.00	100	100
61.00	130.60	149.33
98.00	68.60	59.30
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV033019\
 Data File : VV010031.D
 Acq On : 30 Mar 2019 20:15
 Operator : SY/MD
 Sample : K2166-17
 Misc : 5.97G/10mL/MSVOA V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BF0N4

Manual Integrations
 APPROVED

MMDadoda
 4/1/2019 4:01:39 AM

Quant Time: Mar 31 21:19:25 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM032619S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 30 23:31:11 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	128344	25.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	136507	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	58143	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	58721	22.55	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	90.20%		
7) Chloroethane-d5	1.56	69	71682	25.48	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	101.92%		
10) 1,1-Dichloroethene-d2	2.12	63	129100	18.12	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	72.48%		
20) 2-Butanone-d5	3.93	46	36374	74.95	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	149.90%#		
24) Chloroform-d	4.40	84	76470	23.39	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	93.56%		
26) 1,2-Dichloroethane-d4	5.08	65	59066	30.02	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	120.08%		
29) Benzene-d6	5.10	84	171254	23.89	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	95.56%		
33) 1,2-Dichloropropane-d6	6.12	67	55498	26.46	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	105.84%		
37) Toluene-d8	7.36	98	153456	22.62	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	90.48%		
38) trans-1,3-Dichloropropene-	7.66	79	16115	18.78	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	75.12%		
39) 2-Hexanone-d5	8.13	63	26401	67.44	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	134.88%		
48) 1,1,2,2-Tetrachloroethane-	10.26	84	59755	28.78	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	115.12%		
61) 1,2-Dichlorobenzene-d4	11.68	152	57265	25.87	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	103.48%		

Target Compounds

					Ovalue
16) Methylene chloride	2.53	84	3193	1.511 ug/L	97
22) cis-1,2-Dichloroethene	3.96	96	3417m	1.840 ug/L	
35) Trichloroethene	5.96	95	20215	10.224 ug/L	98
47) Tetrachloroethene	8.02	164	603328	386.679 ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

> MMD
 4/1/19